
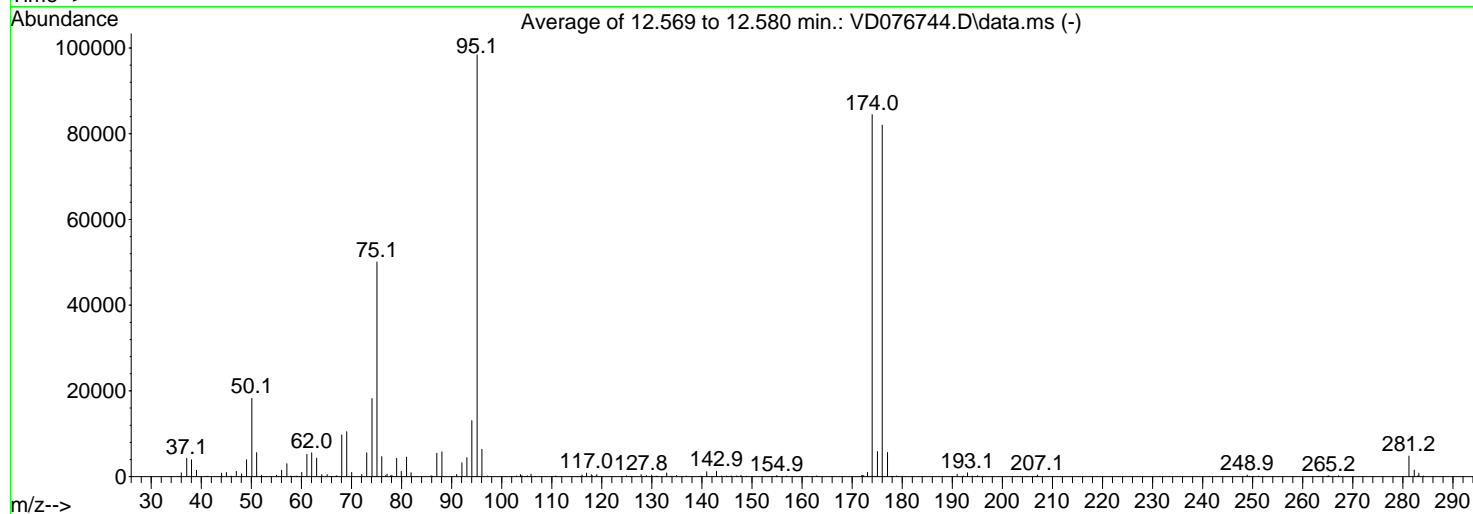


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD071723\  
 Data File : VD076744.D  
 Acq On : 17 Jul 2023 09:08  
 Operator : KP/SY  
 Sample : BFB  
 Misc : 5.00G/5.0ml/MSVOA\_D/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_D  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D071423S.M  
 Title : SW846 8260  
 Last Update : Mon Jul 17 08:07:52 2023

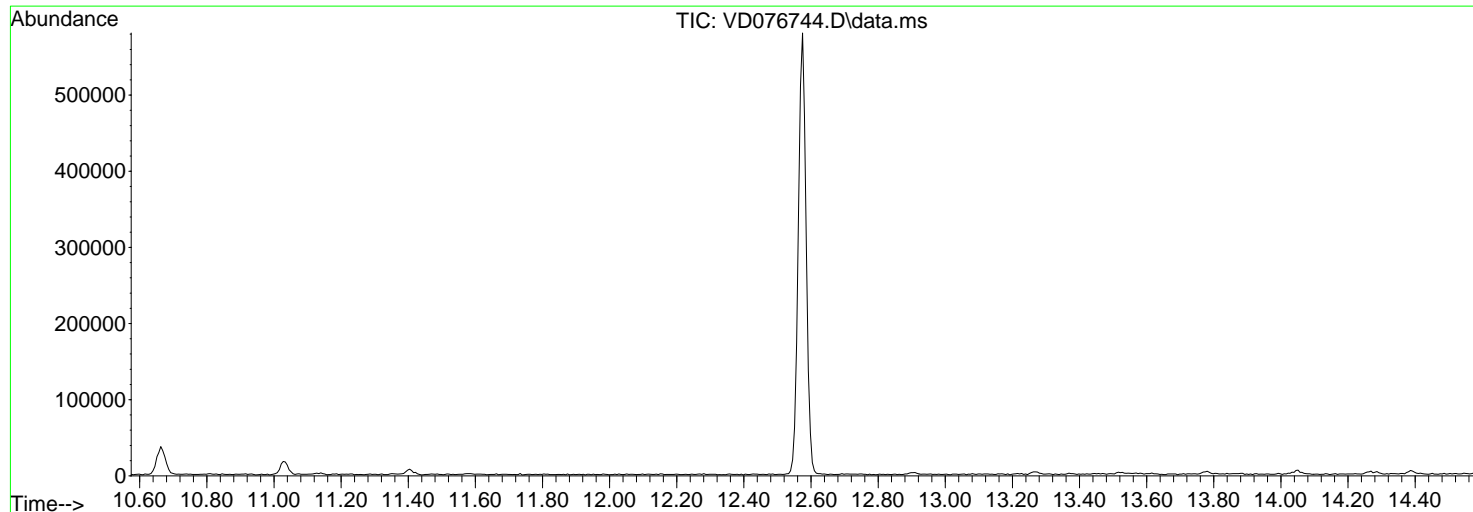

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	18263	PASS
75	95	30	60	50.9	50085	PASS
95	95	100	100	100.0	98403	PASS
96	95	5	9	6.5	6377	PASS
173	174	0.00	2	1.2	998	PASS
174	95	50	100	85.9	84491	PASS
175	174	5	9	6.9	5850	PASS
176	174	95	101	97.0	81995	PASS
177	176	5	9	6.9	5624	PASS