


Dichlorodifluoromethane

Response Ratio

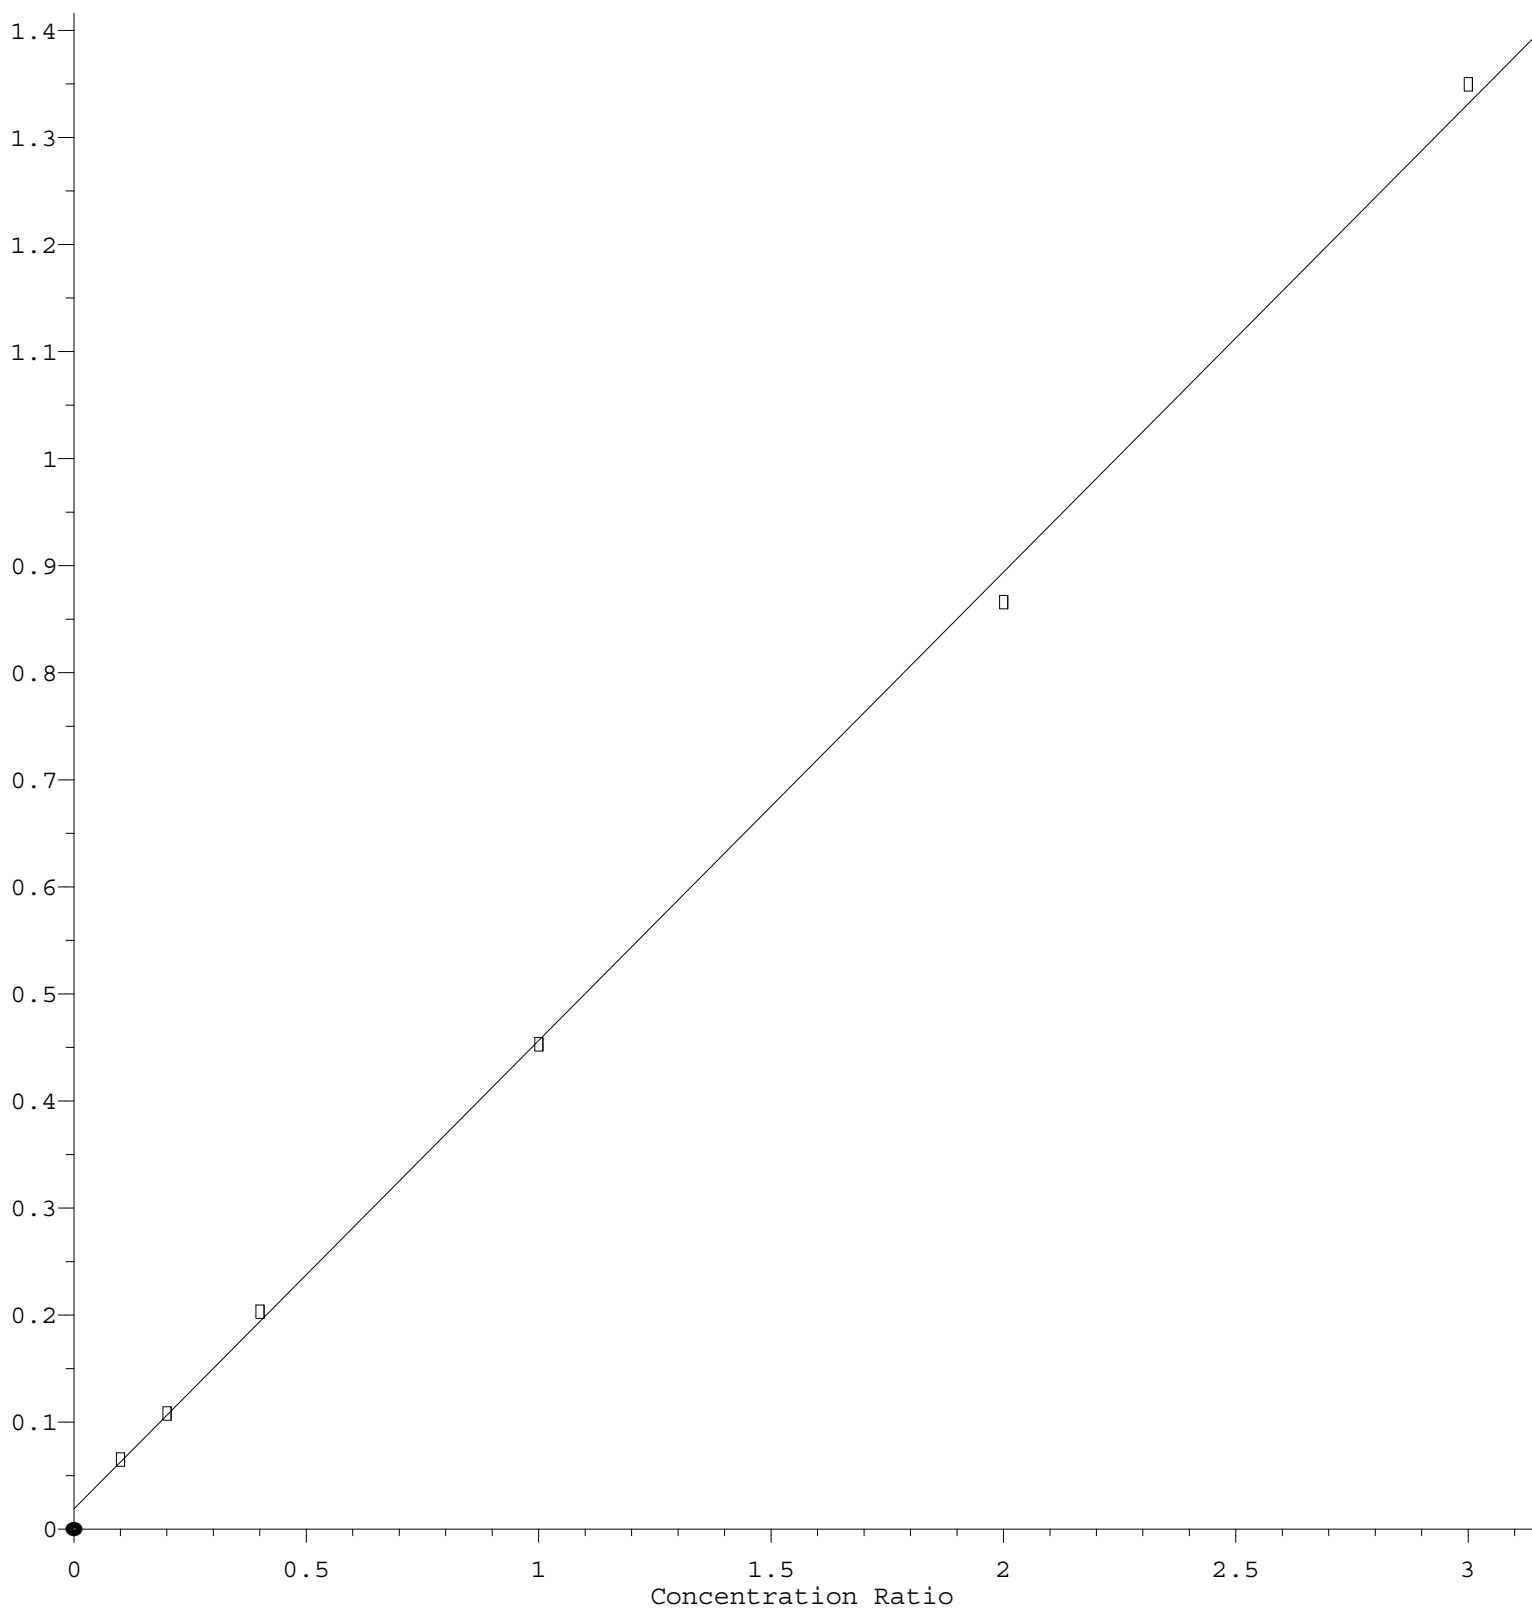

$$\text{Response} = 4.374\text{e-}001 * \text{Amt} + 1.900\text{e-}002$$


Coef of Det (r^2) = 0.999054 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D071822S.M

Calibration Table Last Updated: Wed Jul 20 15:29:08 2022

Chloromethane

Response Ratio

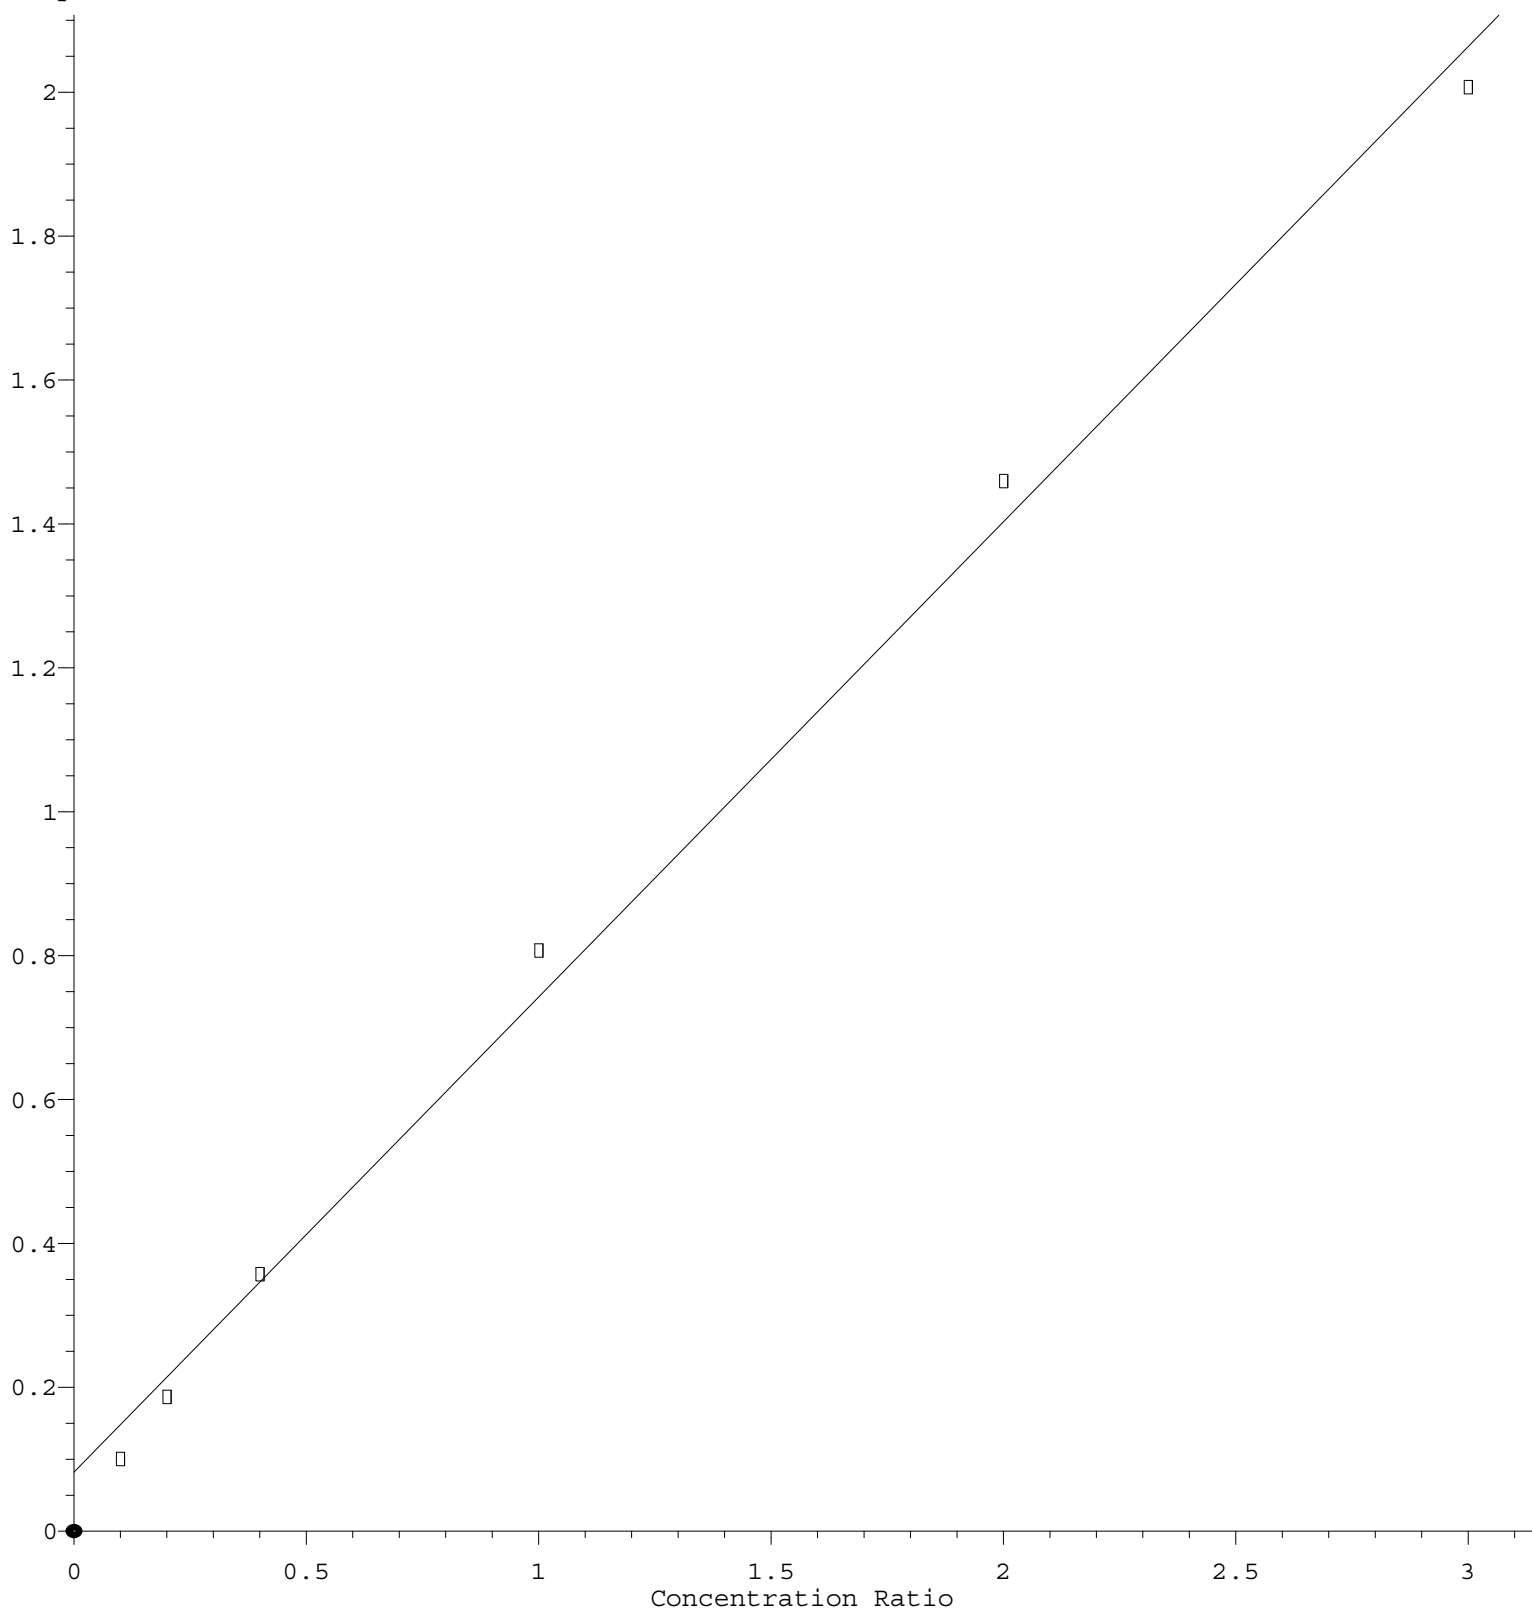


$$\text{Response} = 6.608\text{e-}001 * \text{Amt} + 8.174\text{e-}002$$

Coef of Det (r^2) = 0.995362 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D071822S.M

Calibration Table Last Updated: Wed Jul 20 15:29:08 2022


Tert butyl alcohol

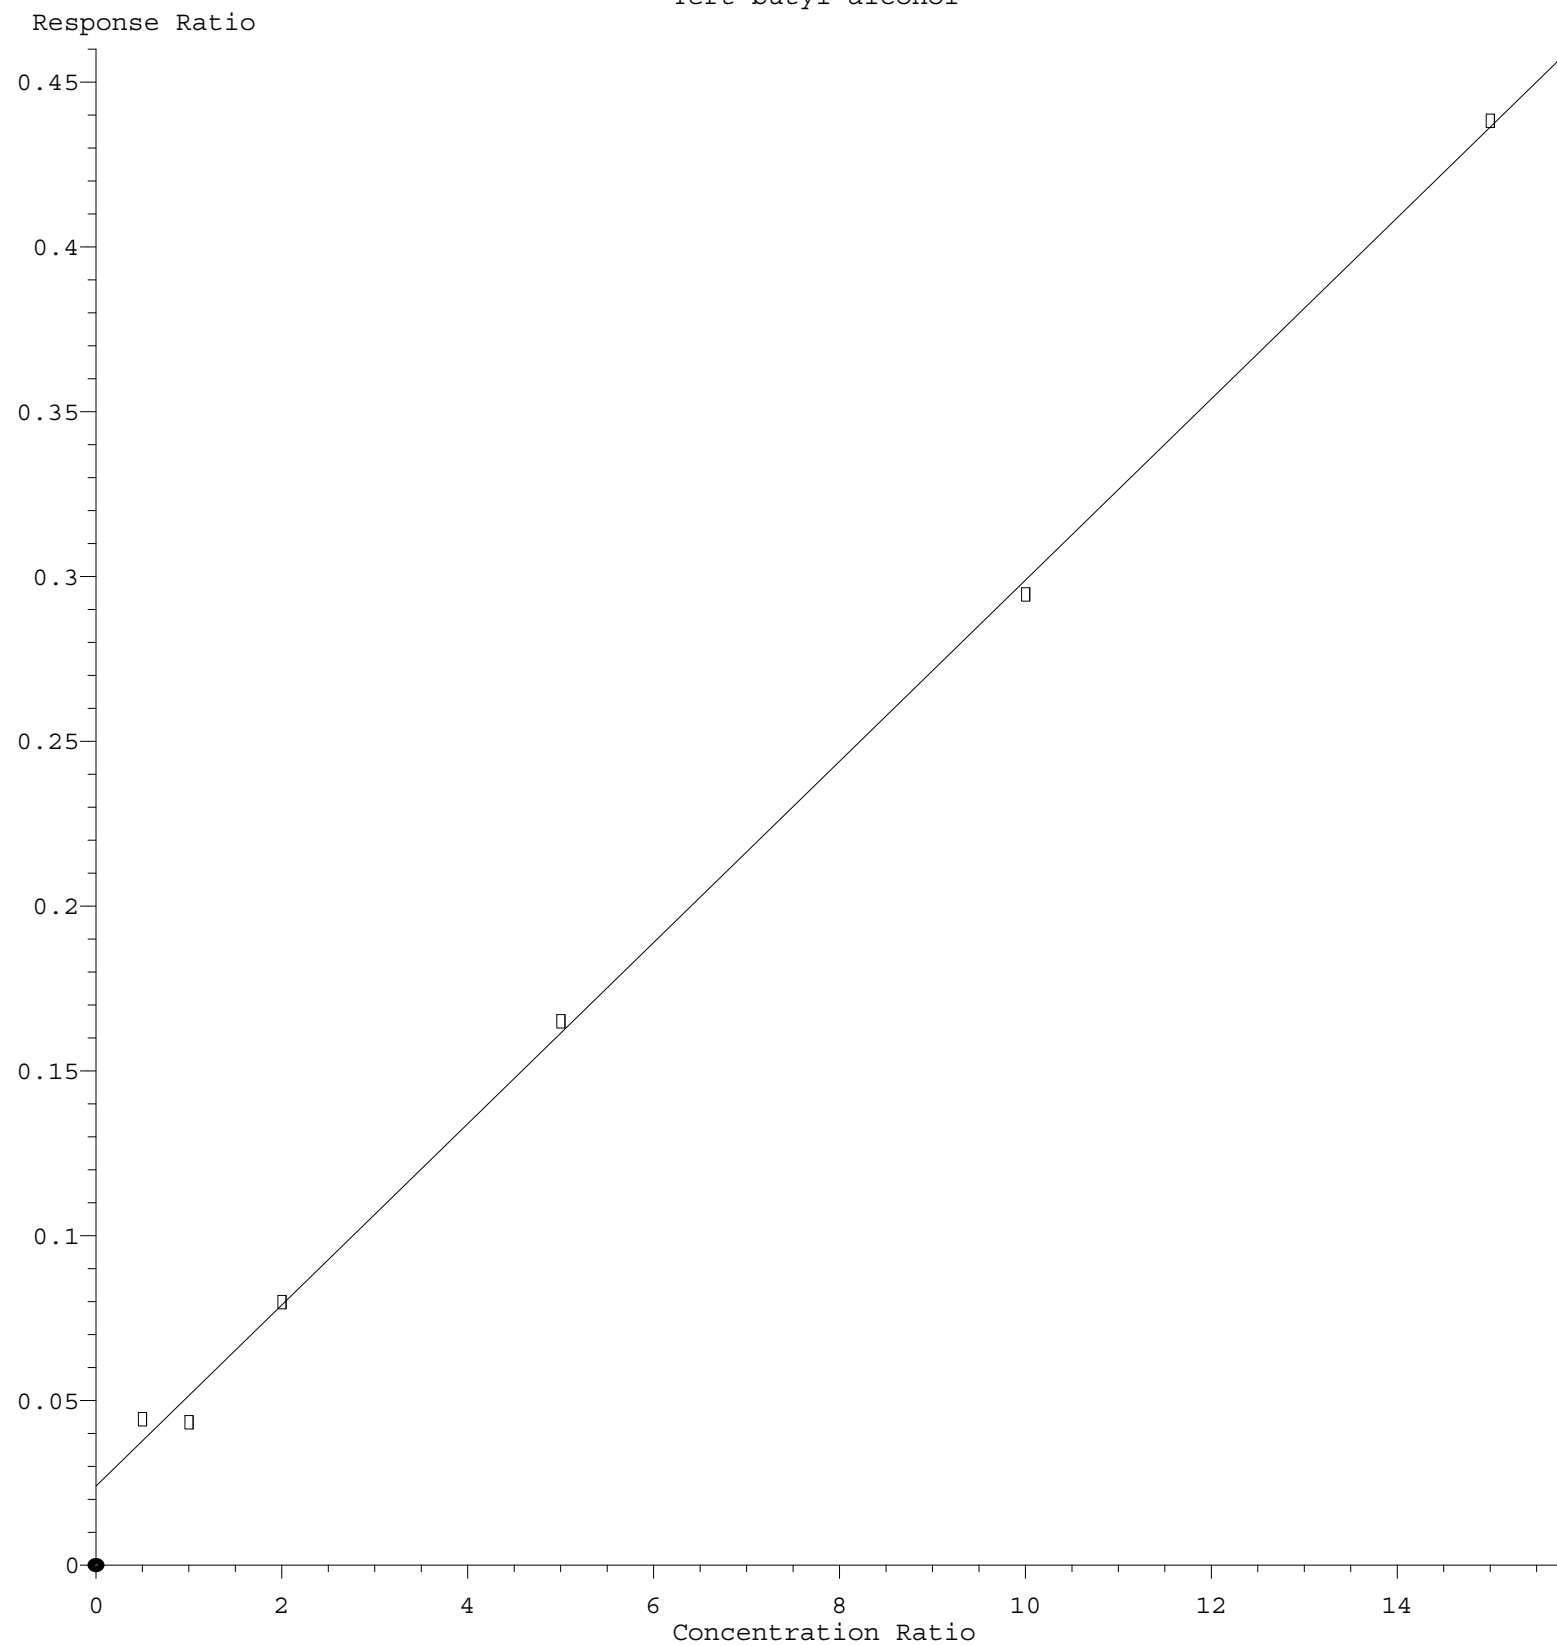

Response = $2.748e-002 * Amt + 2.413e-002$
 Coef of Det (r^2) = 0.998854 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D071822S.M
 Calibration Table Last Updated: Wed Jul 20 15:29:08 2022

Methylene Chloride

Response Ratio

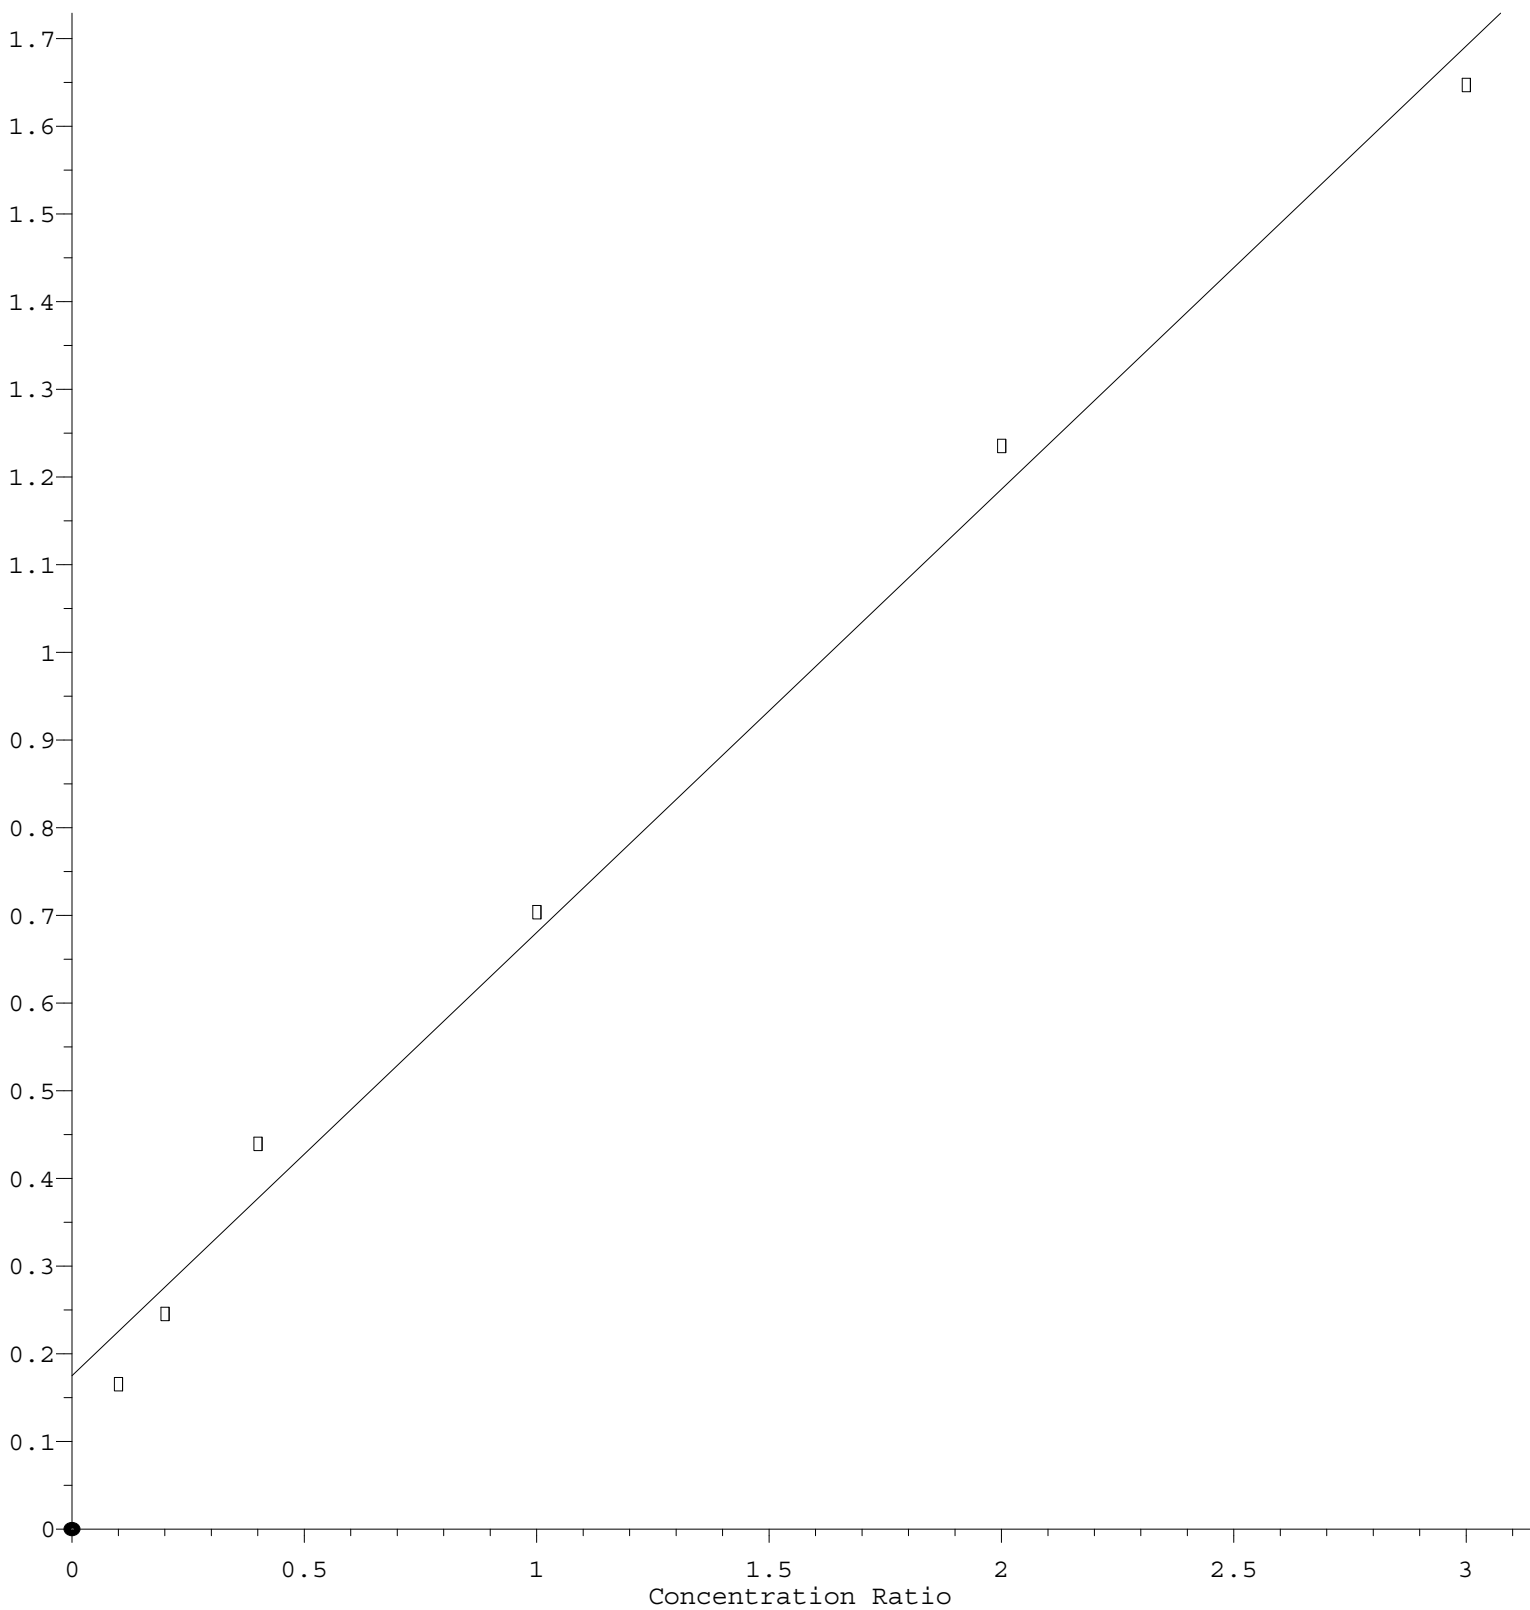

$$\text{Response} = 5.058\text{e-}001 * \text{Amt} + 1.746\text{e-}001$$

Coef of Det (r^2) = 0.992287 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D071822S.M

Calibration Table Last Updated: Wed Jul 20 15:29:08 2022