
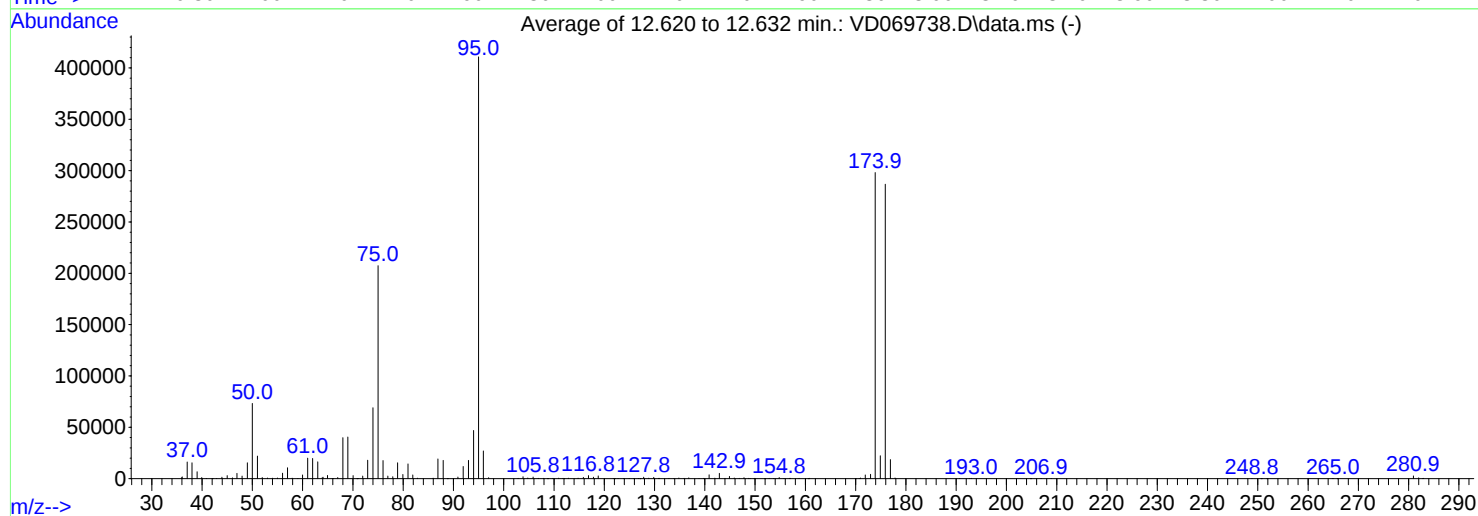


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD071921\
Data File : VD069738.D
Acq On : 19 Jul 2021 08:26
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D071321S.M
Title : SW846 8260
Last Update : Wed Jul 14 06:00:31 2021

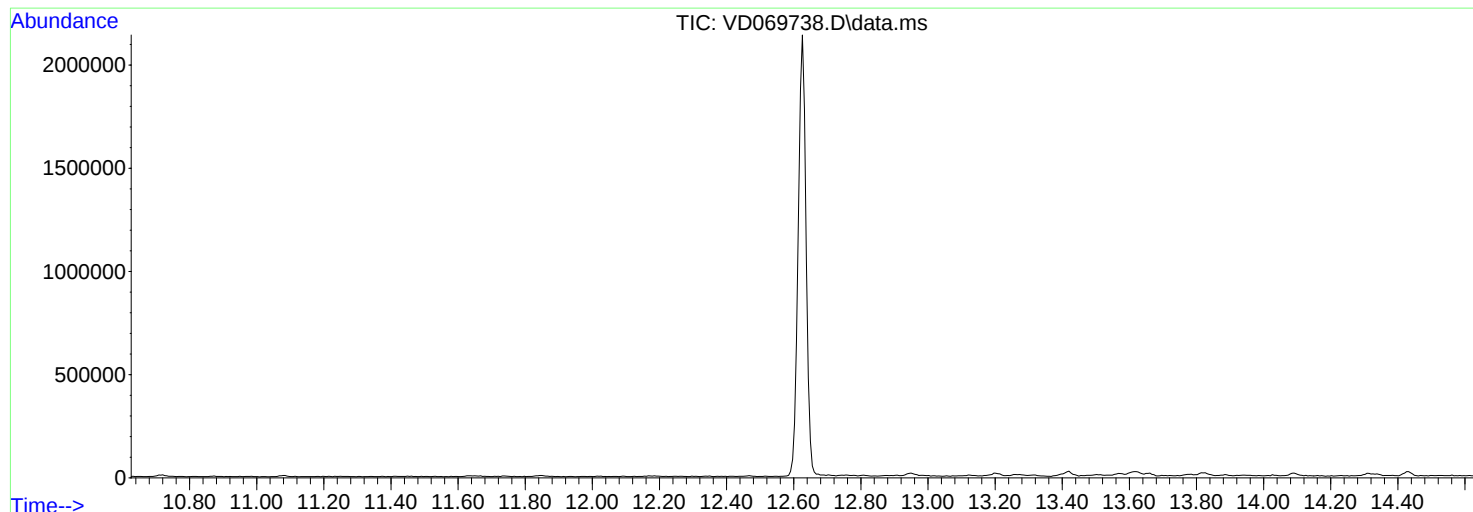

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.8	73205	PASS
75	95	30	60	50.5	207339	PASS
95	95	100	100	100.0	410773	PASS
96	95	5	9	6.6	27038	PASS
173	174	0.00	2	1.4	4160	PASS
174	95	50	100	72.6	298091	PASS
175	174	5	9	7.5	22355	PASS
176	174	95	101	96.2	286699	PASS
177	176	5	9	6.5	18512	PASS