
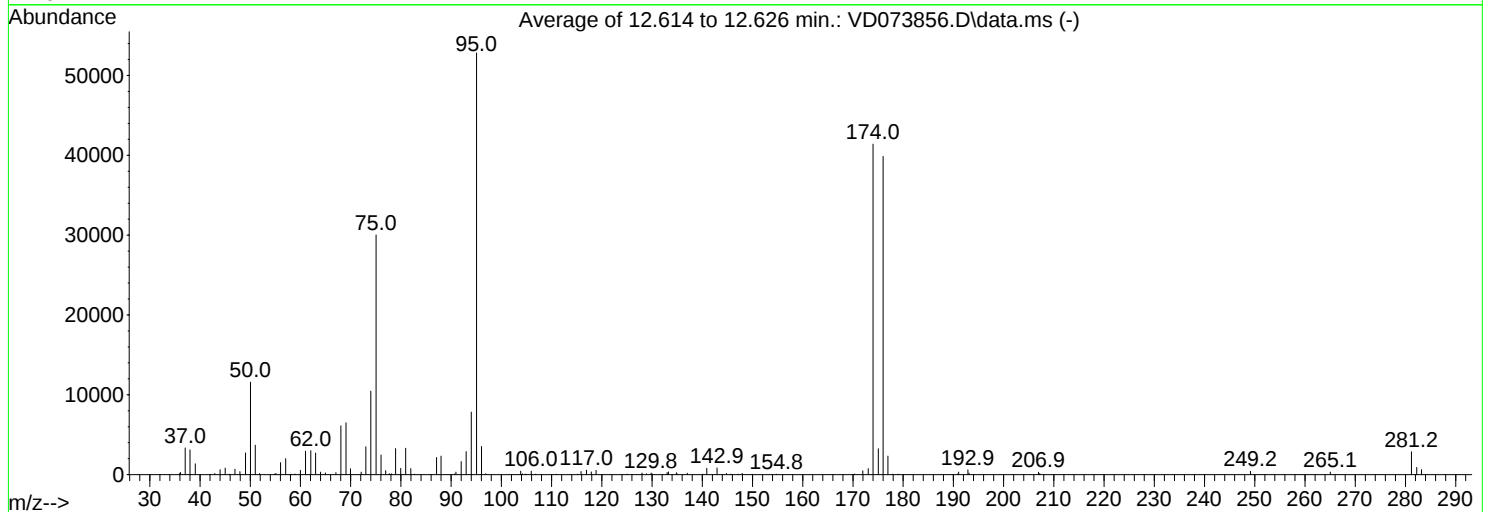


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD071922\
Data File : VD073856.D
Acq On : 19 Jul 2022 09:46
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D071822S.M
Title : SW846 8260
Last Update : Tue Jul 19 01:56:16 2022

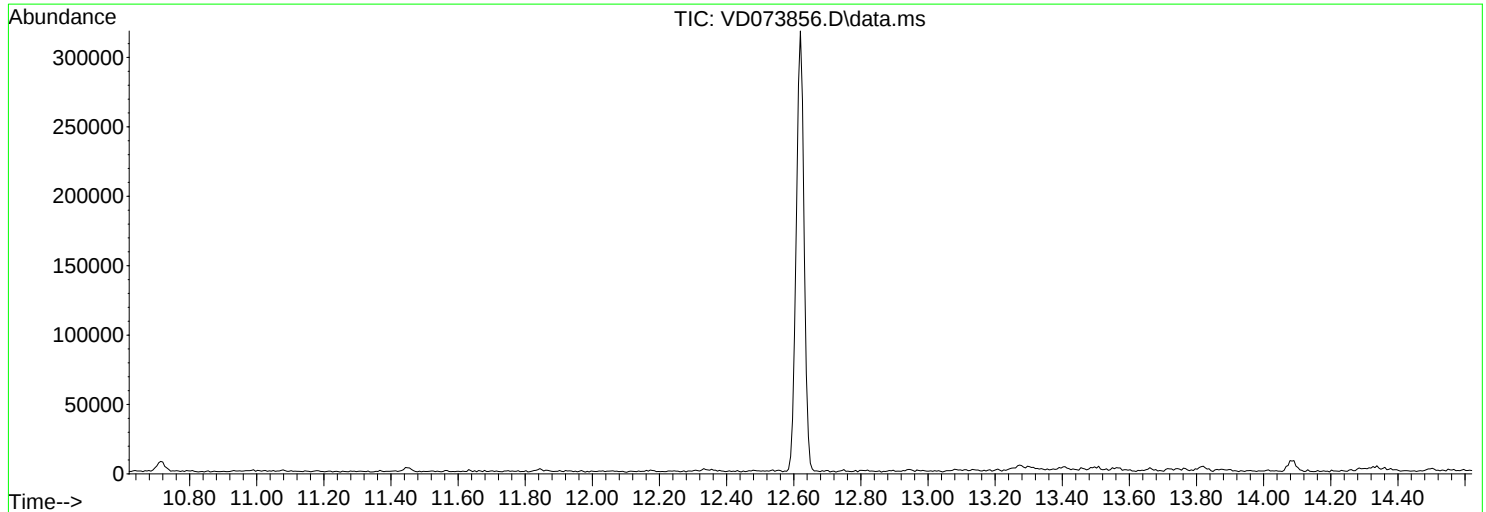

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	11578	PASS
75	95	30	60	56.8	30029	PASS
95	95	100	100	100.0	52832	PASS
96	95	5	9	6.7	3523	PASS
173	174	0.00	2	1.8	756	PASS
174	95	50	100	78.4	41400	PASS
175	174	5	9	7.8	3246	PASS
176	174	95	101	96.3	39864	PASS
177	176	5	9	5.8	2322	PASS