

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD072321\
 Data File : VD069830.D
 Acq On : 23 Jul 2021 15:50
 Operator : VA/SY
 Sample : M3117-02
 Misc : 5.02G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 NJ-CLEAN-2

Quant Time: Jul 24 01:35:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D072221S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 23 04:51:13 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	91678	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	153550	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	190754	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.567	152	92730	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	76916	72.949	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	145.900%
35) Dibromofluoromethane	7.914	113	55670	57.512	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	115.020%
50) Toluene-d8	10.338	98	203774	54.595	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	109.180%
62) 4-Bromofluorobenzene	12.626	95	84003	67.342	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	134.680%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD072321\
Data File : VD069830.D
Acq On : 23 Jul 2021 15:50
Operator : VA/SY
Sample : M3117-02
Misc : 5.02G/5.00ml/MSVOA_D/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
NJ-CLEAN-2

Quant Time: Jul 24 01:35:02 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D072221S.M
Quant Title : SW846 8260
QLast Update : Fri Jul 23 04:51:13 2021
Response via : Initial Calibration




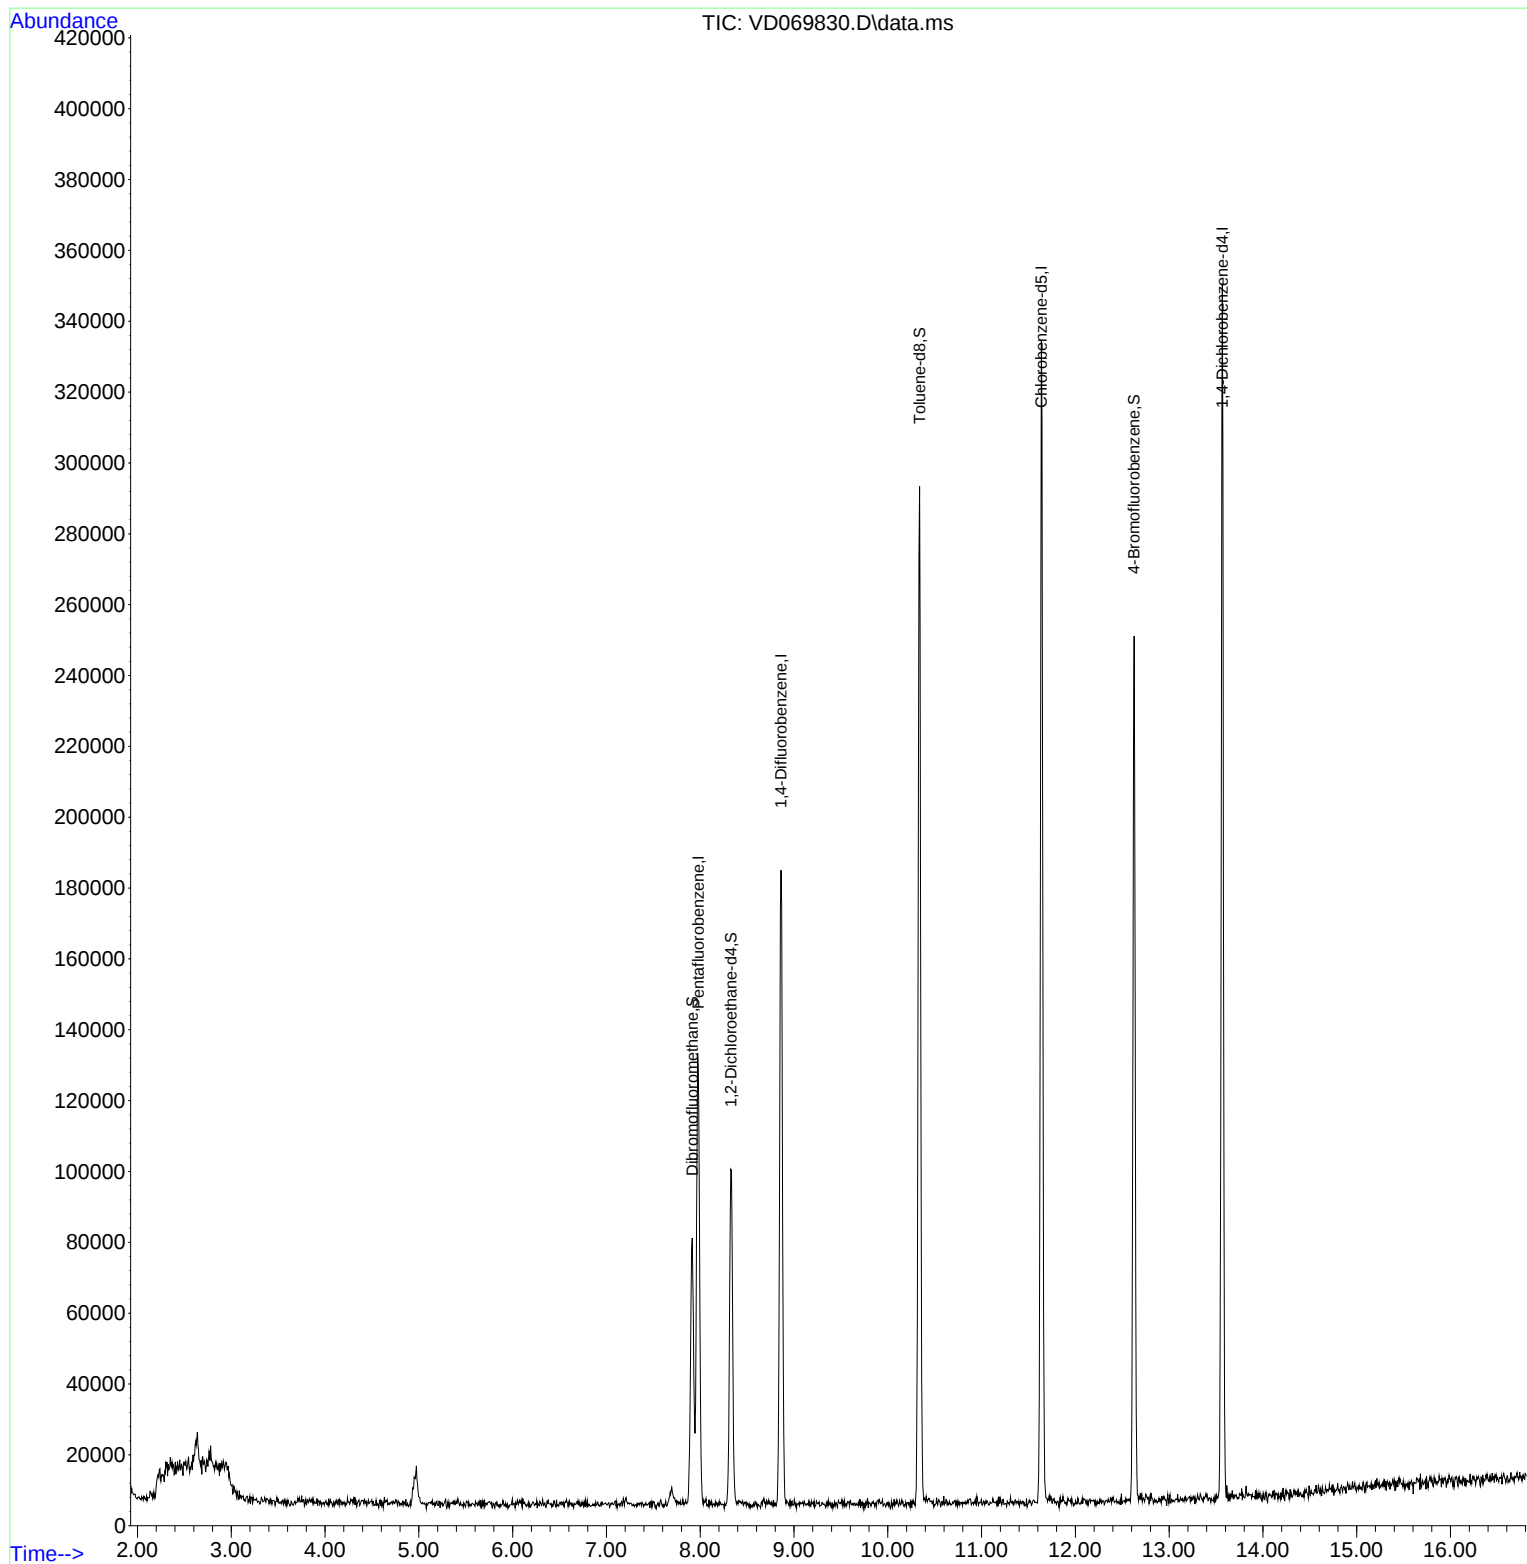


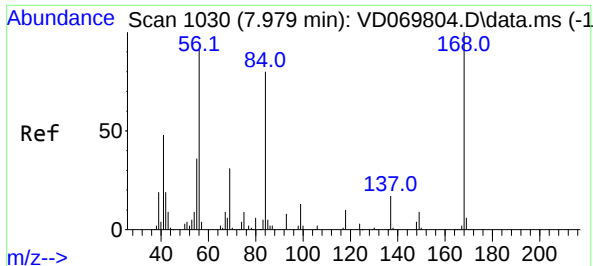

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. 0.000 min
Lab File: VD069830.D
Acq: 23 Jul 2021 15:50




Instrument :
MSVOA_D
ClientSampleId :
NJ-CLEAN-2

Tgt Ion:168 Resp: 91678
Ion Ratio Lower Upper
168 100
99 61.2 51.1 76.7

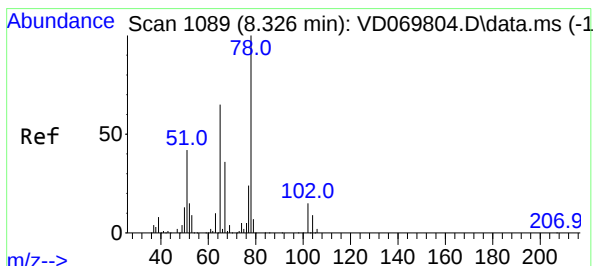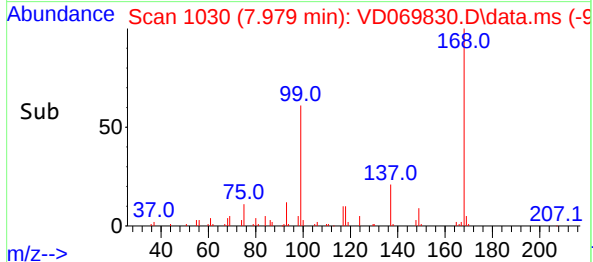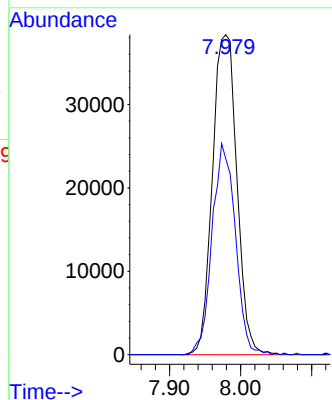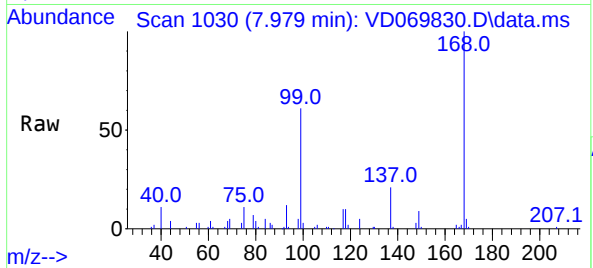

#33
1,2-Dichloroethane-d4
Concen: 72.949 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. 0.000 min
Lab File: VD069830.D
Acq: 23 Jul 2021 15:50

Tgt Ion: 65 Resp: 76916
Ion Ratio Lower Upper
65 100
67 54.8 0.0 111.2

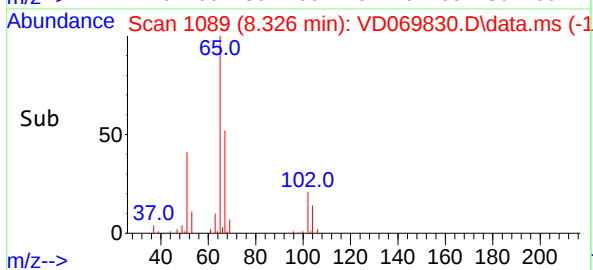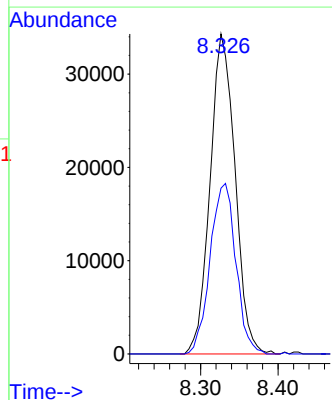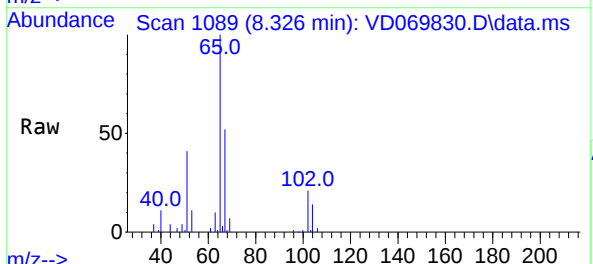







#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. 0.000 min
Lab File: VD069830.D
Acq: 23 Jul 2021 15:50

Instrument :
MSVOA_D
ClientSampleId :
NJ-CLEAN-2




Tgt Ion:114 Resp: 153550
Ion Ratio Lower Upper
114 100
63 20.1 0.0 41.6
88 13.2 0.0 31.4

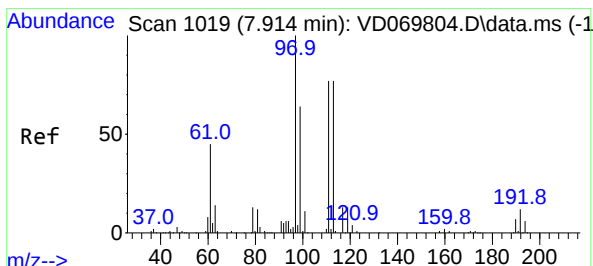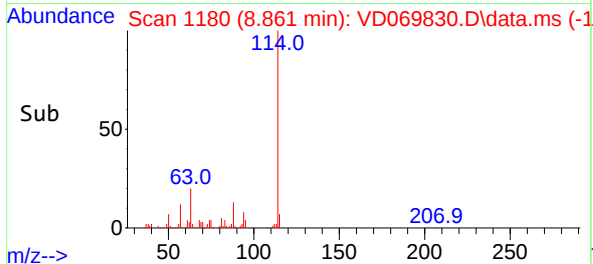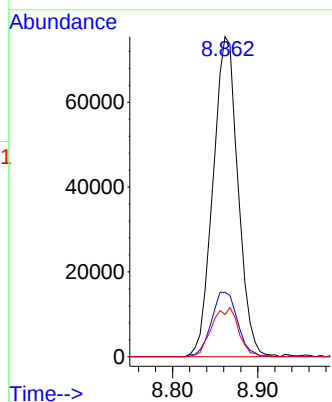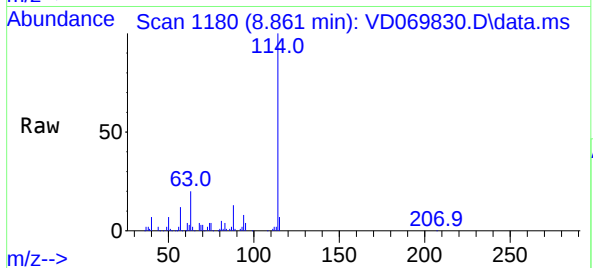

#35

Dibromofluoromethane
Concen: 57.512 ug/l
RT: 7.914 min Scan# 1019
Delta R.T. 0.000 min
Lab File: VD069830.D
Acq: 23 Jul 2021 15:50

Tgt Ion:113 Resp: 55670
Ion Ratio Lower Upper
113 100
111 103.4 80.5 120.7
192 15.5 12.6 19.0


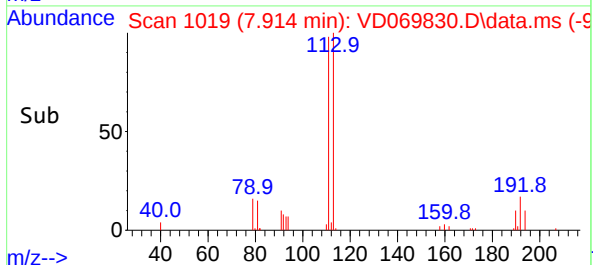
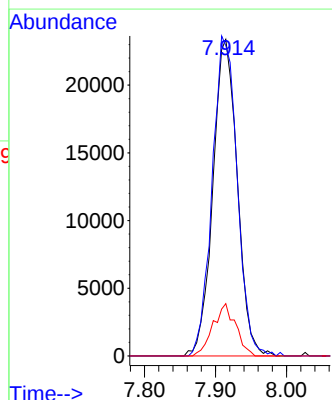
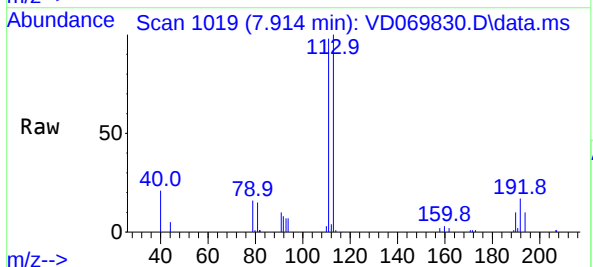




#50
Toluene-d8
Concen: 54.595 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. 0.000 min
Lab File: VD069830.D
Acq: 23 Jul 2021 15:50




Instrument :
MSVOA_D
ClientSampleId :
NJ-CLEAN-2


Tgt Ion: 98 Resp: 203774
Ion Ratio Lower Upper
98 100
100 64.1 51.9 77.9

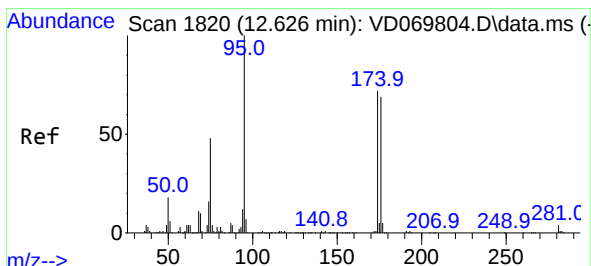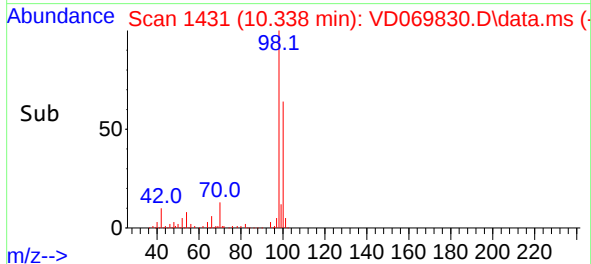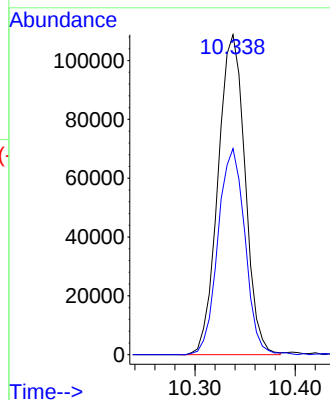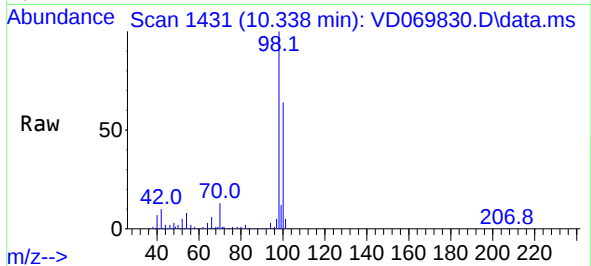

#62
4-Bromofluorobenzene
Concen: 67.342 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. 0.000 min
Lab File: VD069830.D
Acq: 23 Jul 2021 15:50

Tgt Ion: 95 Resp: 84003
Ion Ratio Lower Upper
95 100
174 74.2 0.0 142.6
176 72.2 0.0 134.2

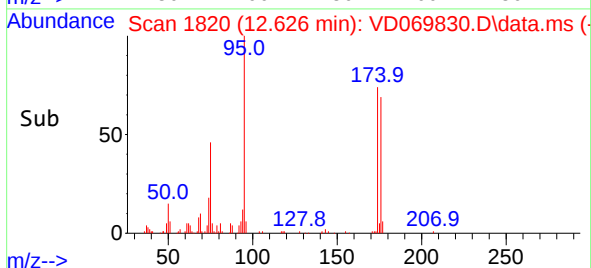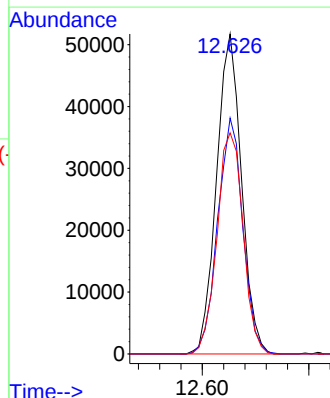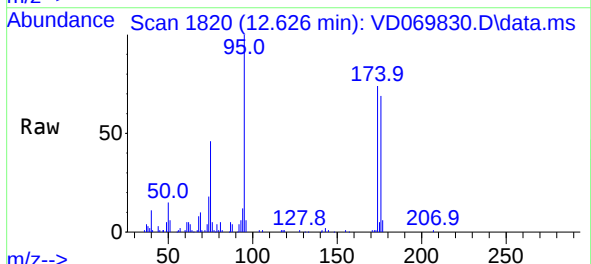




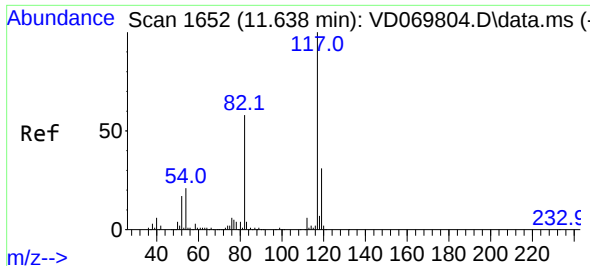


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 1652
Delta R.T. 0.000 min
Lab File: VD069830.D
Acq: 23 Jul 2021 15:50

Instrument :
MSVOA_D
ClientSampleId :
NJ-CLEAN-2

Tgt Ion:117 Resp: 190754

Ion	Ratio	Lower	Upper
117	100		
82	60.4	46.3	69.5
119	34.8	24.7	37.1

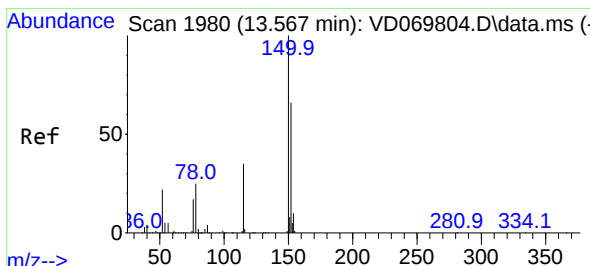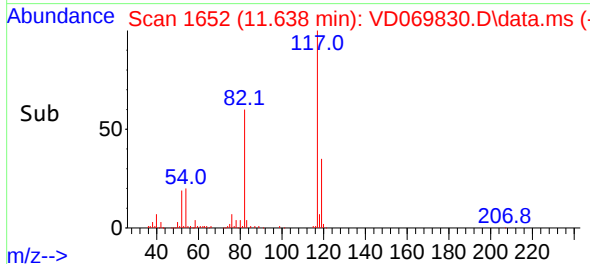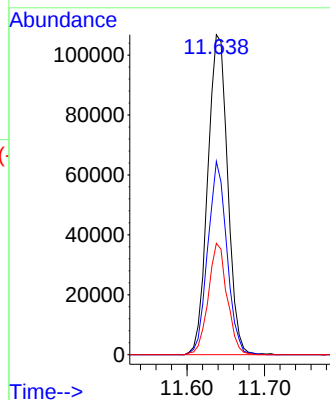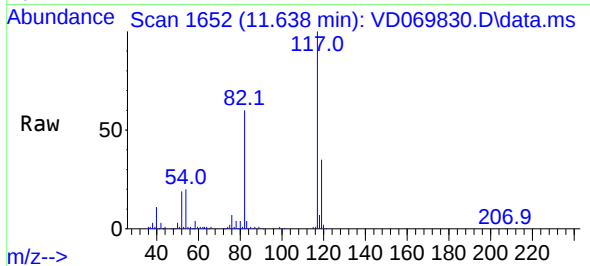

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.567 min Scan# 1980
Delta R.T. 0.000 min
Lab File: VD069830.D
Acq: 23 Jul 2021 15:50

Tgt Ion:152 Resp: 92730

Ion	Ratio	Lower	Upper
152	100		
115	59.8	31.1	93.3
150	152.5	0.0	343.0

