


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD072321\
Data File : VD069820.D
Acq On : 23 Jul 2021 09:29
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D072221S.M
Title : SW846 8260
Last Update : Fri Jul 23 04:51:13 2021

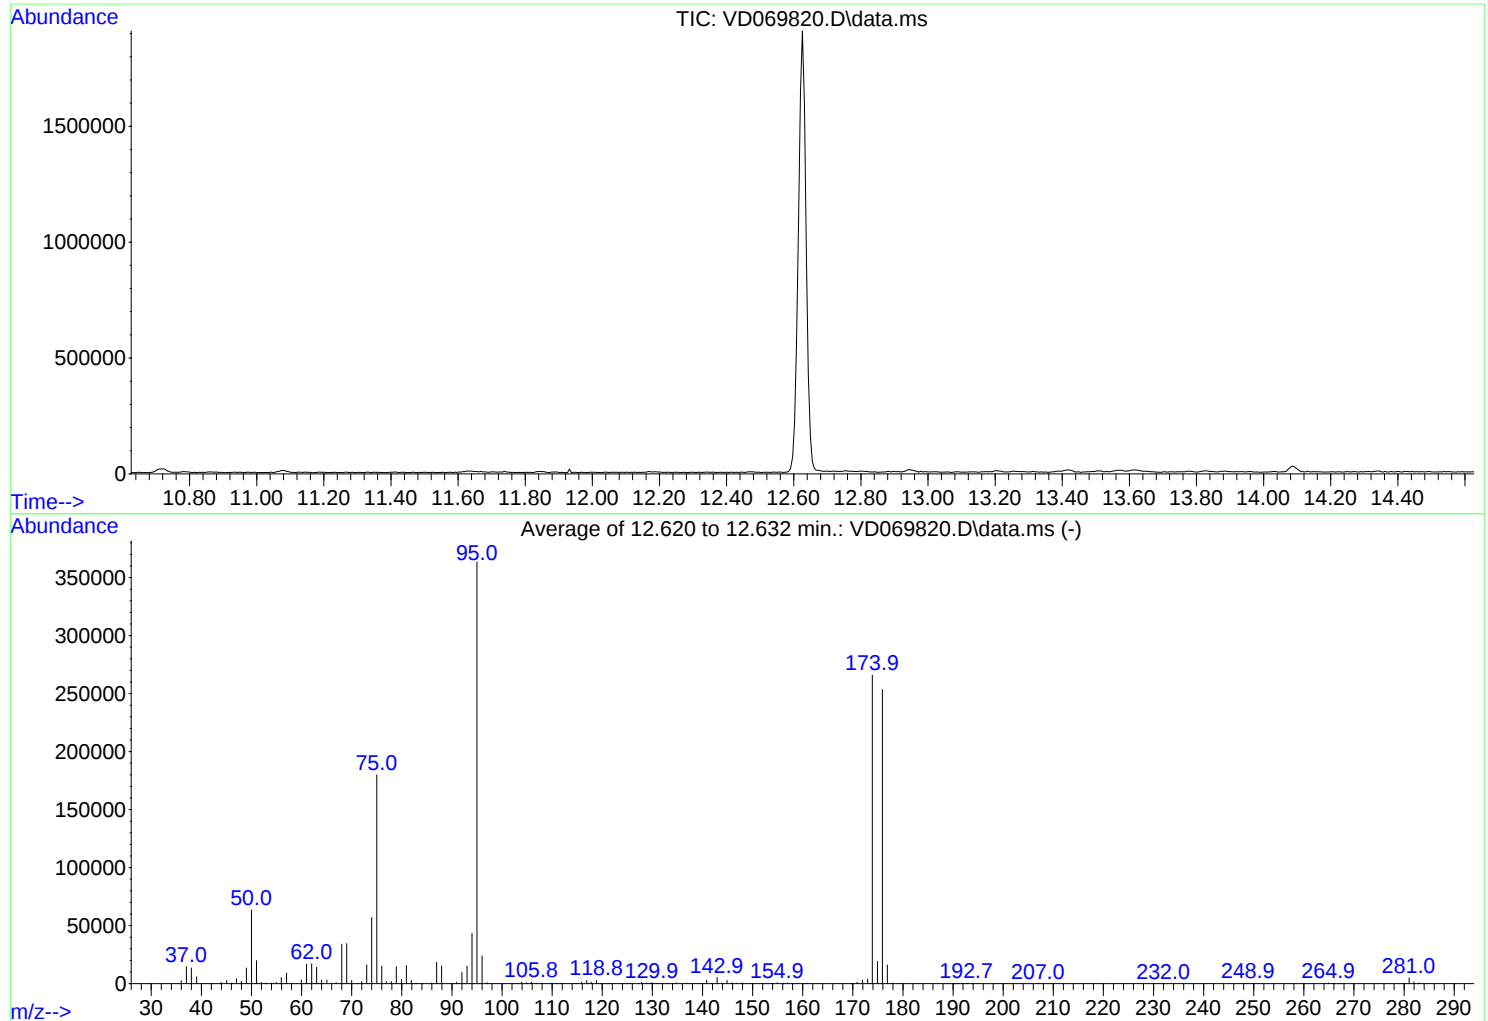

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1808

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	63437	PASS
75	95	30	60	49.5	179925	PASS
95	95	100	100	100.0	363563	PASS
96	95	5	9	6.6	24016	PASS
173	174	0.00	2	1.4	3839	PASS
174	95	50	100	73.2	265963	PASS
175	174	5	9	7.2	19139	PASS
176	174	95	101	95.3	253547	PASS
177	176	5	9	6.4	16113	PASS