


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD072418\
Data File : VD059573.D
Acq On : 24 Jul 2018 15:35
Operator : VA/AP
Sample : BFB
Misc : 5.00g/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D072418S.M
Title : SW846 8260
Last Update : Wed Jul 25 07:10:33 2018

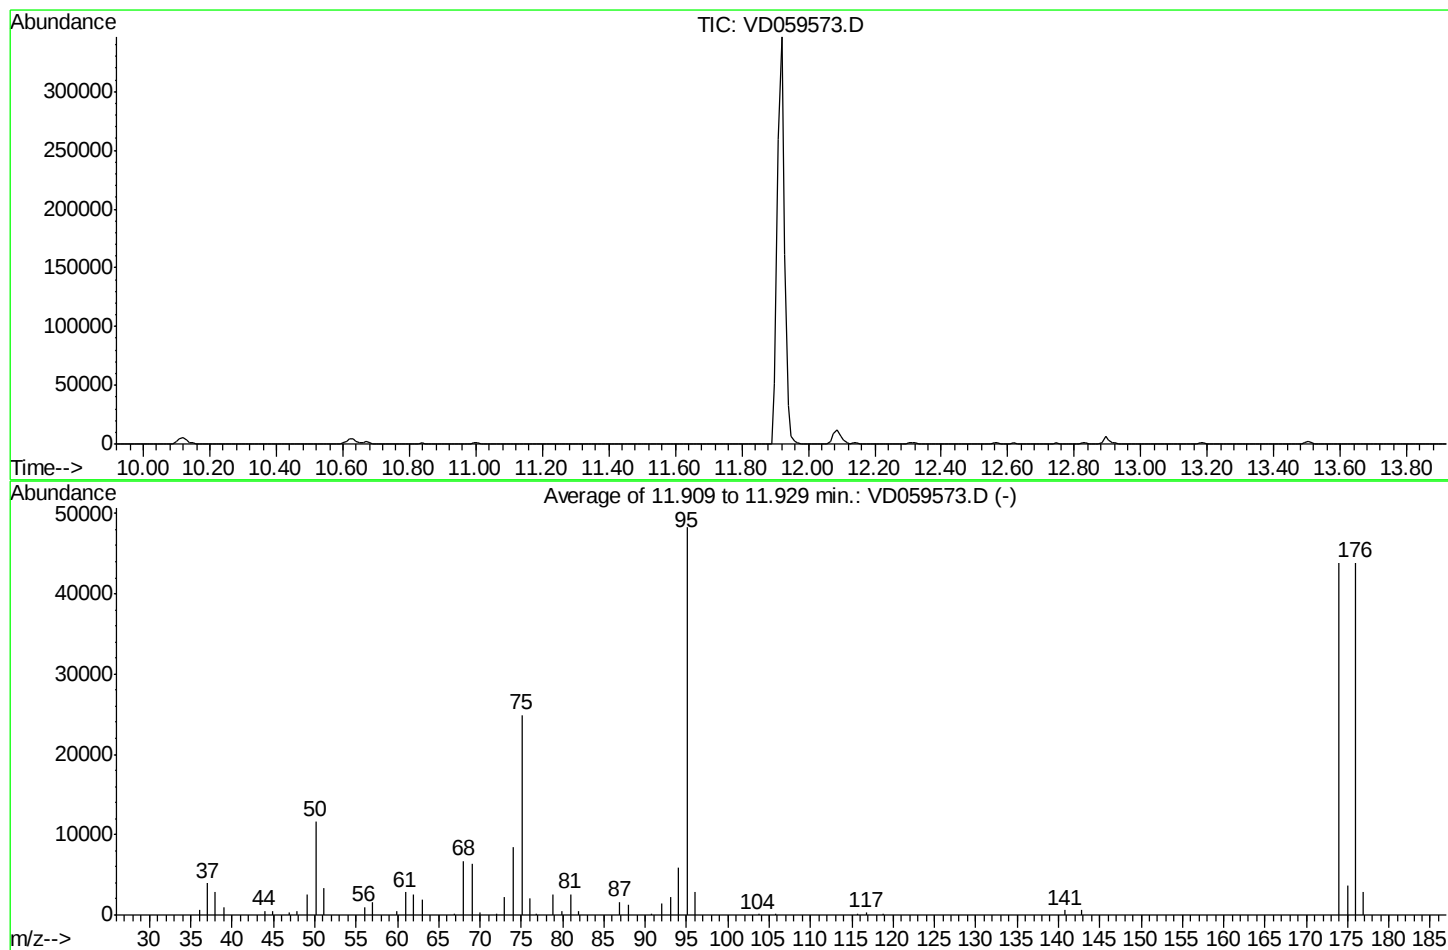

AutoFind: Scans 1188, 1189, 1190; Background Corrected with Scan 1183

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.1	11627	PASS
75	95	30	60	51.6	24909	PASS
95	95	100	100	100.0	48269	PASS
96	95	5	9	6.0	2899	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	90.9	43872	PASS
175	174	5	9	8.3	3636	PASS
176	174	95	101	100.1	43909	PASS
177	176	5	9	6.4	2830	PASS