

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD072420\
 Data File : VD066045.D
 Acq On : 24 Jul 2020 14:17
 Operator : VA/SY
 Sample : L3383-17
 Misc : 8.01G/5.00ml/MSVOA D/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 CRT-008

Quant Time: Jul 25 00:18:01 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D072120S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 21 12:34:13 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.99	168	309015	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.87	114	473498	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	501285	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	268069	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.33	65	121186	48.20	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.40%	
35) Dibromofluoromethane	7.92	113	140494	48.92	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.84%	
50) Toluene-d8	10.34	98	576303	53.87	ug/l	0.00
Spiked Amount 50.000			Recovery	=	107.74%	
62) 4-Bromofluorobenzene	12.64	95	224584	60.54	ug/l	0.00
Spiked Amount 50.000			Recovery	=	121.08%	
Target Compounds						
20) Methylene Chloride	4.96	84	44499	13.657	ug/l	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD072420\
Data File : VD066045.D
Acq On : 24 Jul 2020 14:17
Operator : VA/SY
Sample : L3383-17
Misc : 8.01G/5.00ml/MSVOA D/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
CRT-008

Quant Time: Jul 25 00:18:01 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D072120S.M
Quant Title : SW846 8260
QLast Update : Tue Jul 21 12:34:13 2020
Response via : Initial Calibration

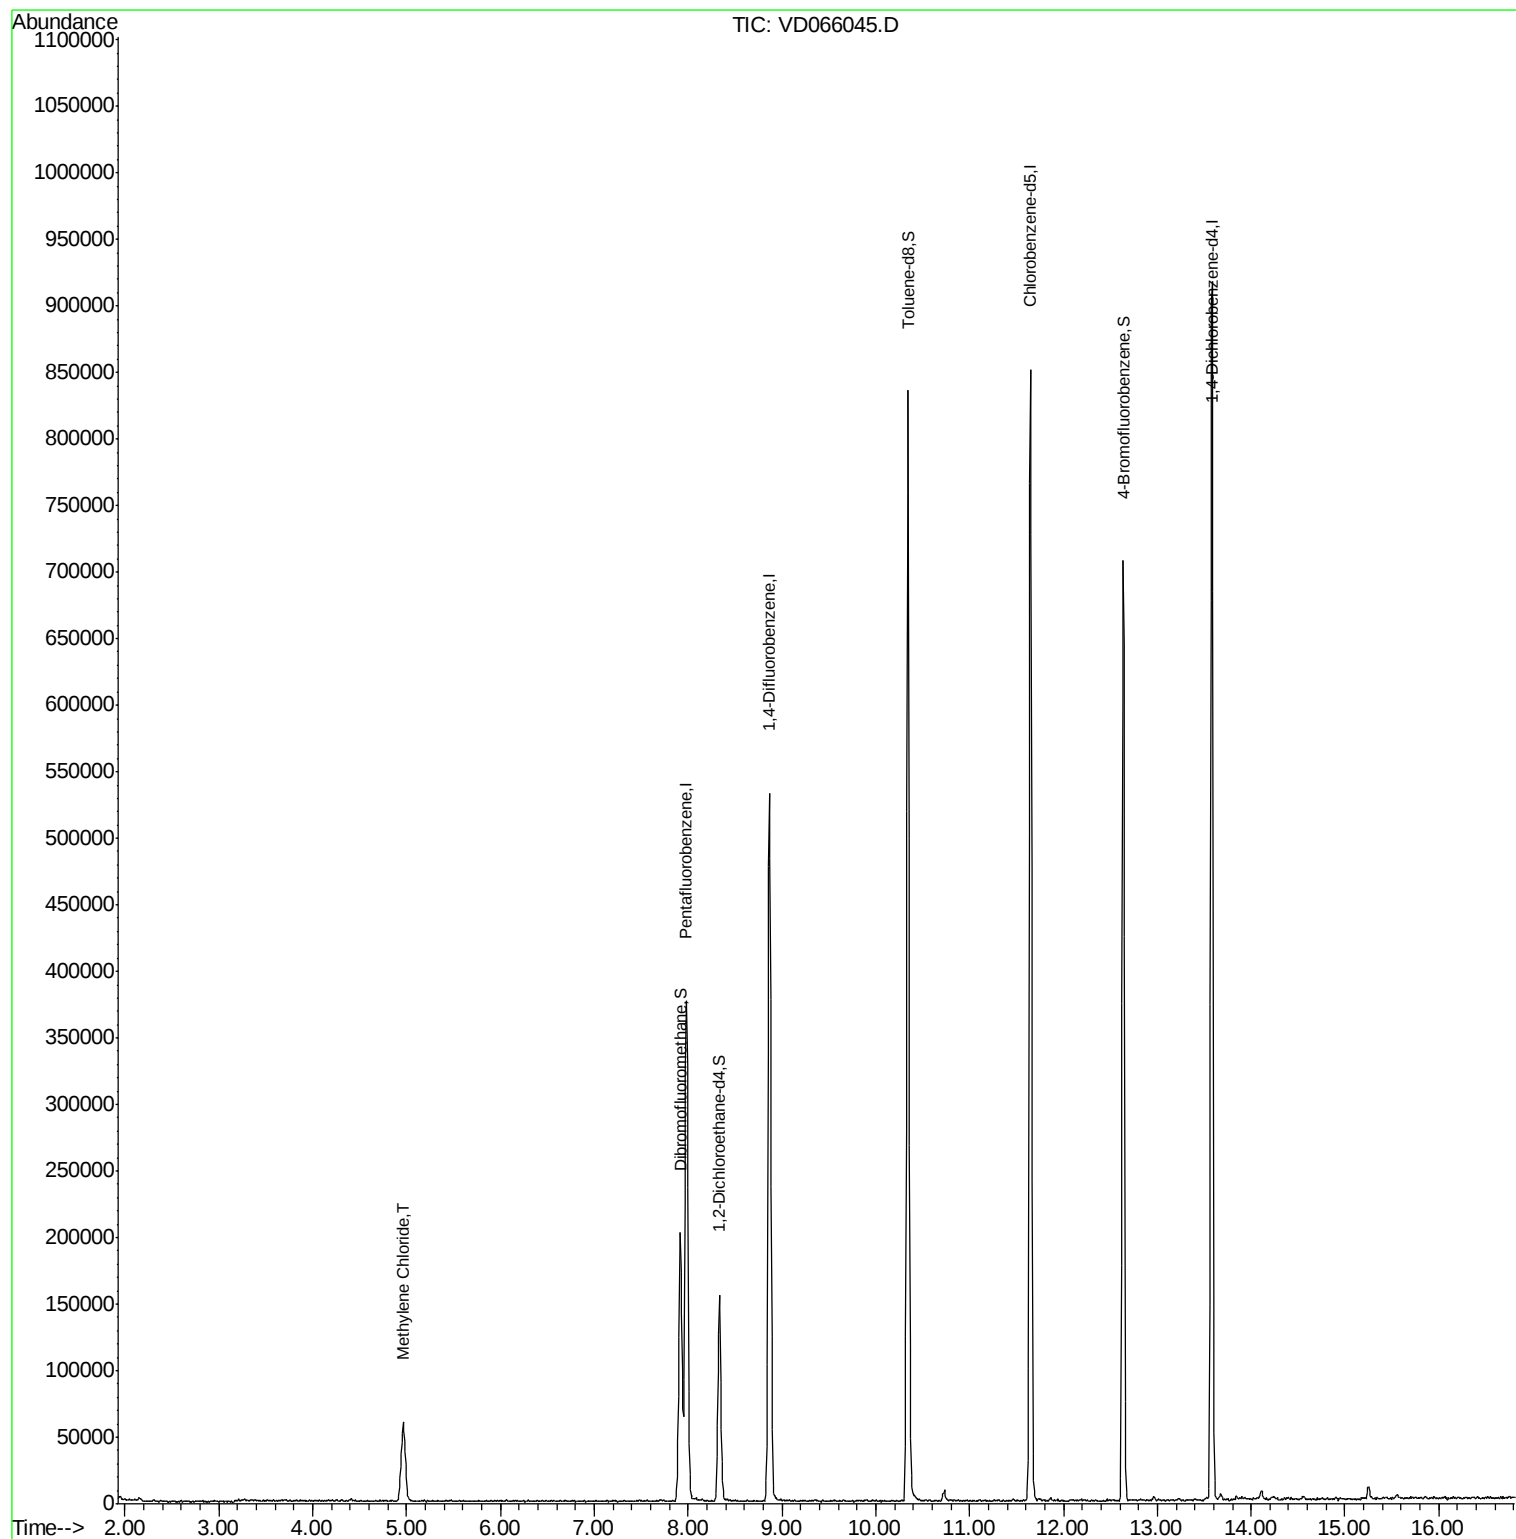

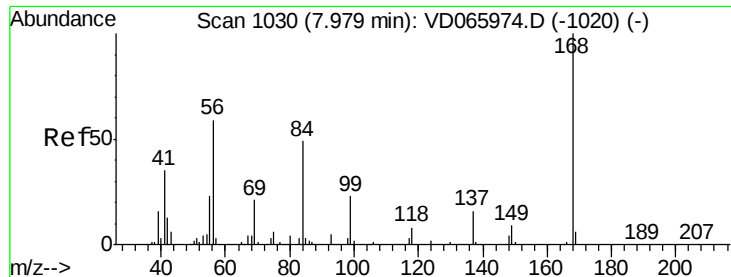

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.99 min Scan# 1031

Delta R.T. 0.01 min

Lab File: VD066045.D

Acq: 24 Jul 2020 14:17

Instrument :

MSVOA_D

ClientSampleId :


CRT-008

Tot Ion:168 Resp: 309015

Ion Ratio Lower Upper

168 100

99 50.3 40.8 61.2

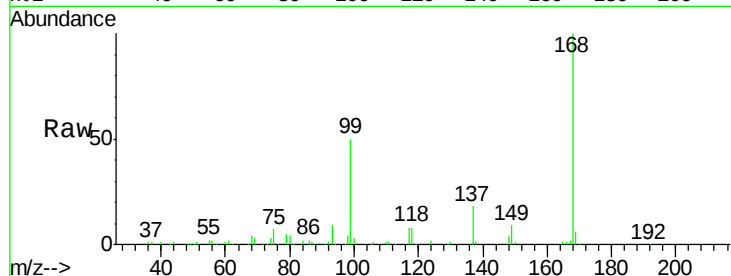

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

7.99



150000

100000

50000

0

Time-->

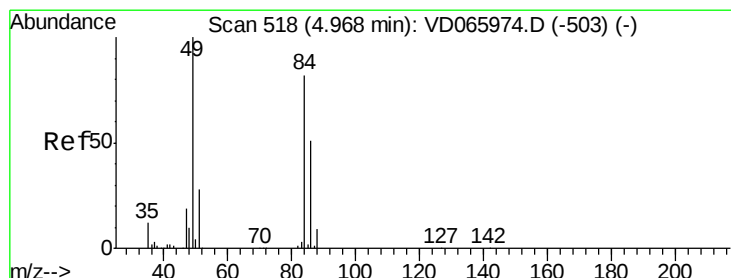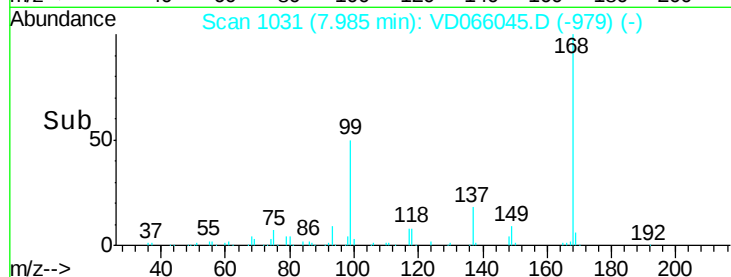

#20

Methylene Chloride

Concen: 13.657 ug/l

RT: 4.96 min Scan# 517

Delta R.T. -0.01 min

Lab File: VD066045.D

Acq: 24 Jul 2020 14:17

Tgt Ion: 84 Resp: 44499


Ion Ratio Lower Upper

84 100

49 131.6 97.7 146.5

51 37.8 27.4 41.2

86 59.7 49.4 74.2

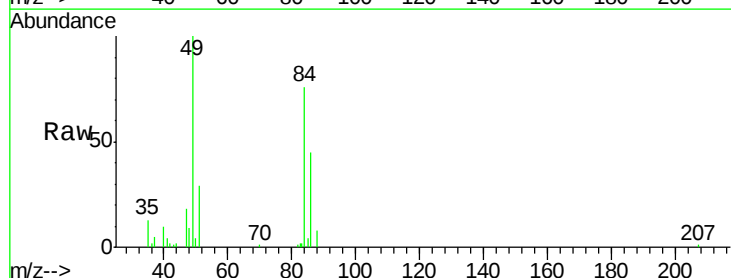

Abundance Ion 83.90 (83.60 to 84.60): VDC

Ion 48.90 (48.60 to 49.60): VDC

Ion 50.90 (50.60 to 51.60): VDC

Ion 85.90 (85.60 to 86.60): VDC

4.96

25000

20000


15000


10000

5000

0

Time-->




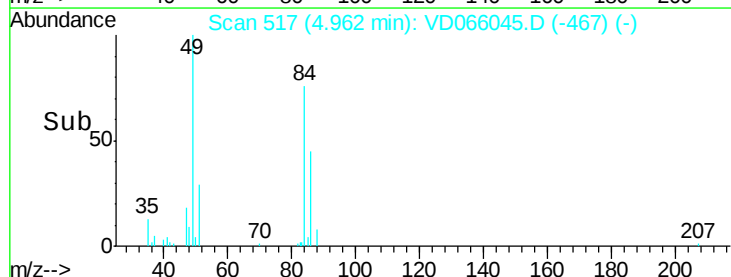


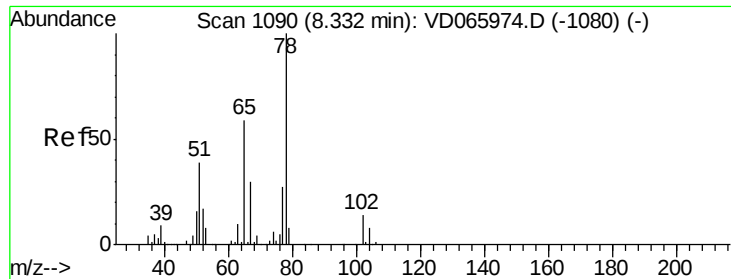

#33
 1,2-Dichloroethane-d4
 Concen: 48.196 ug/l
 RT: 8.33 min Scan# 1090
 Delta R.T. 0.00 min
 Lab File: VD066045.D
 Acq: 24 Jul 2020 14:17




Instrument :
 MSVOA_D
 ClientSampleId :
 CRT-008

Tot Ion: 65 Resp: 121186
 Ion Ratio Lower Upper
 65 100
 67 50.9 0.0 105.0

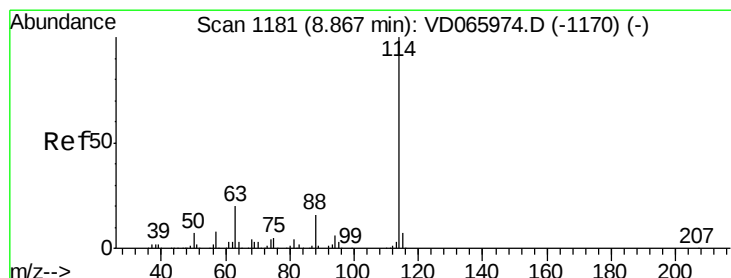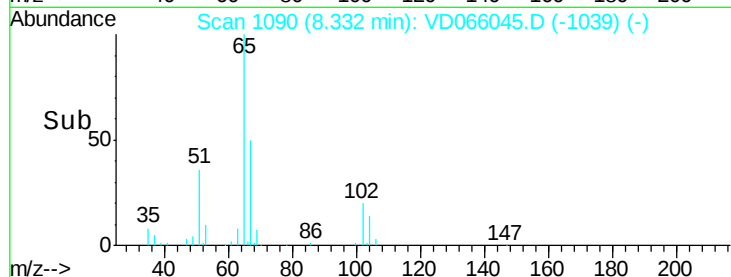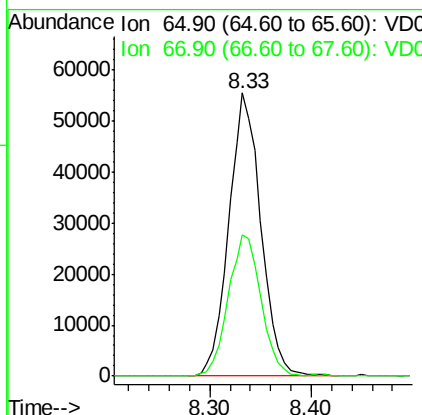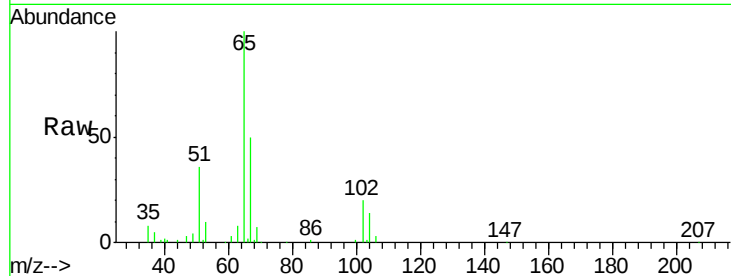

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.87 min Scan# 1181
 Delta R.T. 0.00 min
 Lab File: VD066045.D
 Acq: 24 Jul 2020 14:17

Tgt Ion: 114 Resp: 473498
 Ion Ratio Lower Upper
 114 100
 63 20.0 0.0 39.6
 88 15.4 0.0 31.2


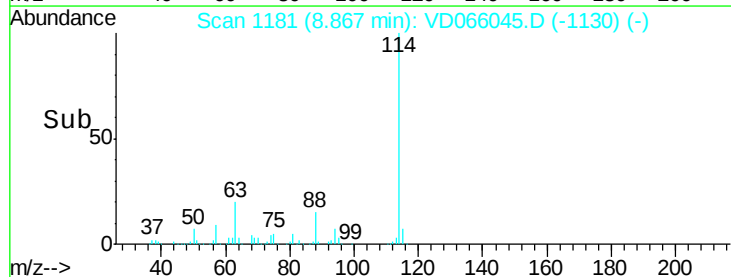
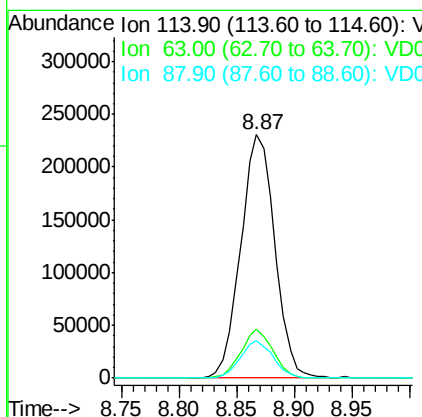
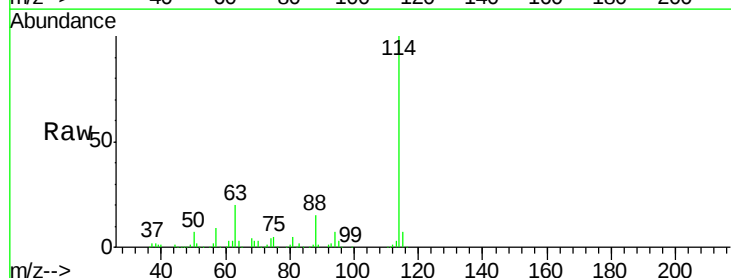




#35
 Dibromofluoromethane
 Concen: 48.920 ug/l
 RT: 7.92 min Scan# 1020
 Delta R.T. 0.00 min
 Lab File: VD066045.D
 Acq: 24 Jul 2020 14:17




Instrument :
 MSVOA_D
 ClientSampleId :
 CRT-008


Tot Ion	Ratio	Lower	Upper
113	100		
111	105.4	83.2	124.8
192	23.6	18.7	28.1

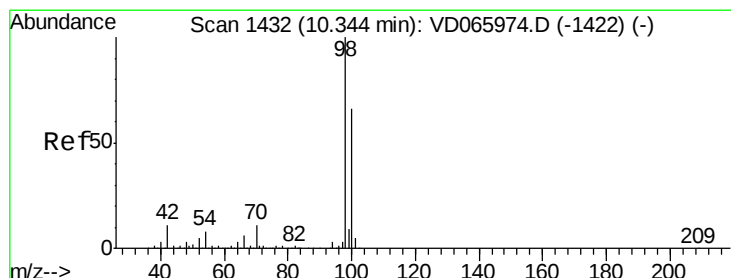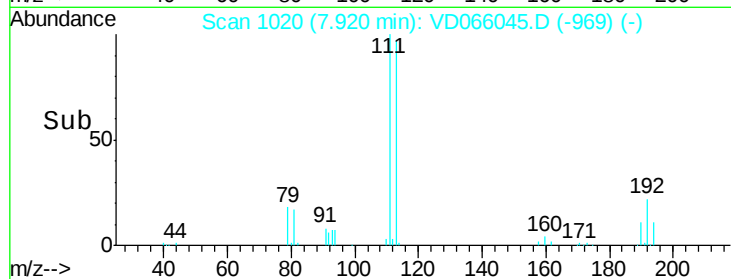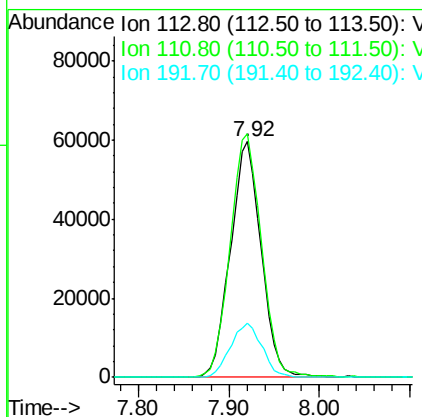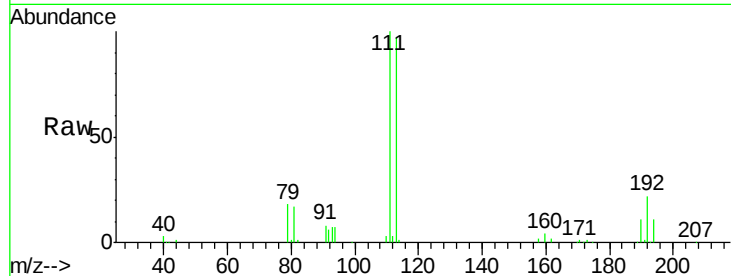

#50
 Toluene-d8
 Concen: 53.867 ug/l
 RT: 10.34 min Scan# 1432
 Delta R.T. 0.00 min
 Lab File: VD066045.D
 Acq: 24 Jul 2020 14:17

Tgt Ion	Ratio	Lower	Upper
98	100		
100	65.2	52.7	79.1


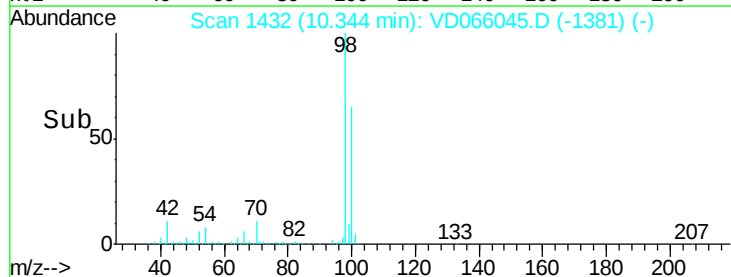
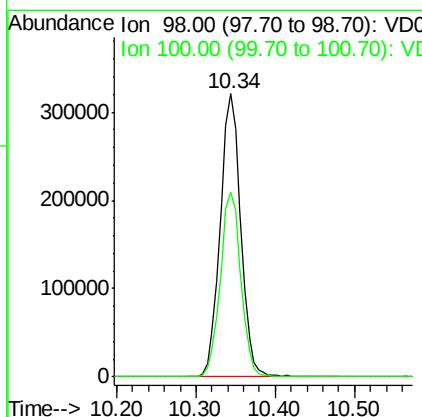
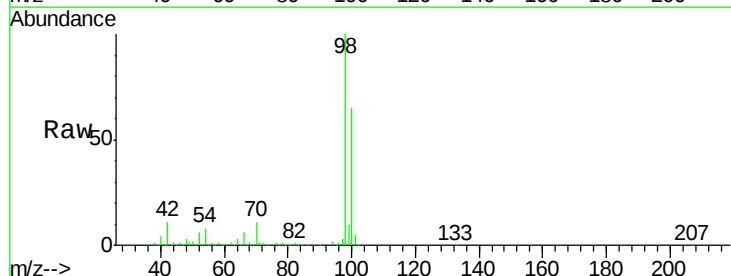


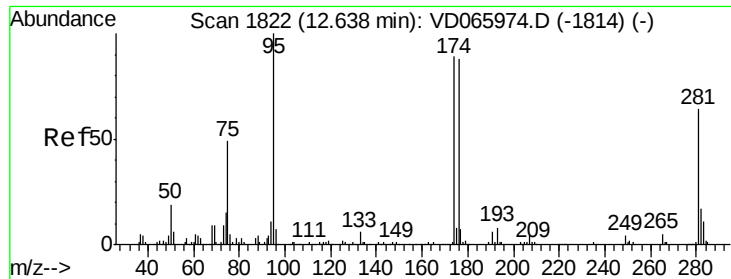

#62
4-Bromofluorobenzene
Concen: 60.541 ug/l
RT: 12.64 min Scan# 1822
Delta R.T. 0.00 min
Lab File: VD066045.D
Acq: 24 Jul 2020 14:17




Instrument :
MSVOA_D
ClientSampleId :
CRT-008


Tot Ion: 95 Resp: 224584
Ion Ratio Lower Upper
95 100
174 93.4 0.0 178.8
176 90.8 0.0 172.6

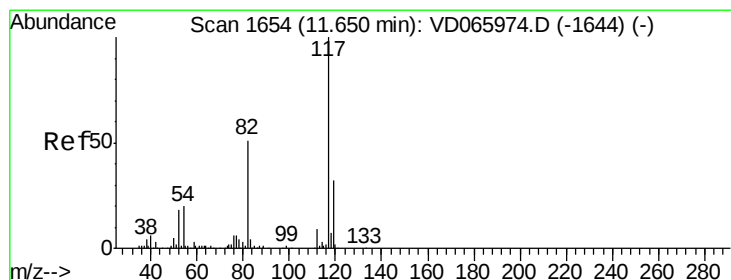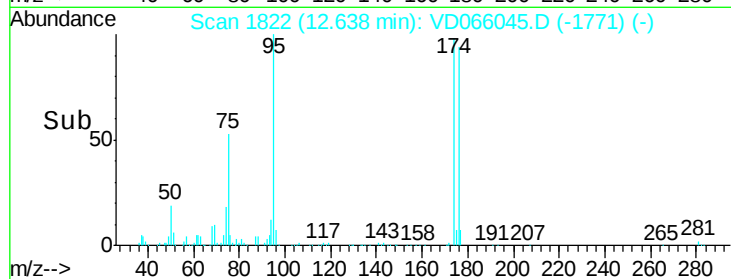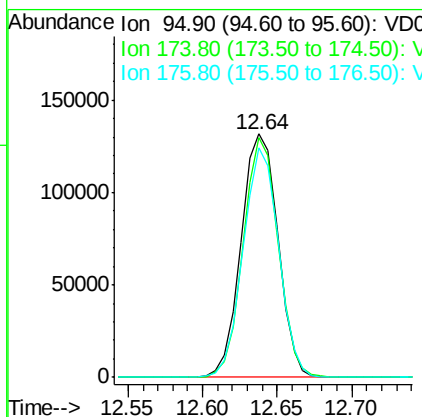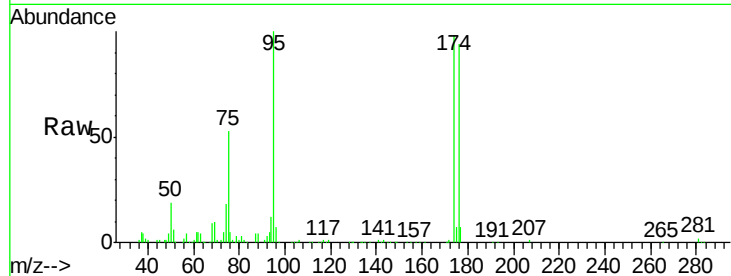

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.65 min Scan# 1654
Delta R.T. 0.00 min
Lab File: VD066045.D
Acq: 24 Jul 2020 14:17

Tgt Ion: 117 Resp: 501285
Ion Ratio Lower Upper
117 100
82 51.4 41.1 61.7
119 30.5 25.9 38.9

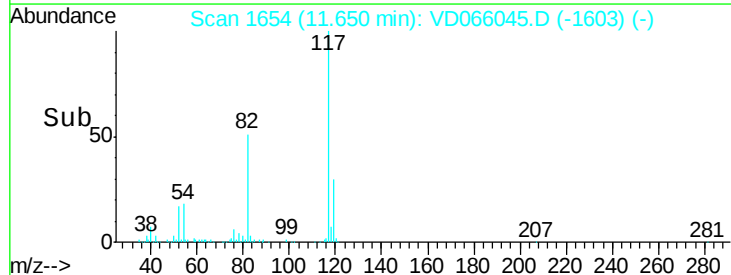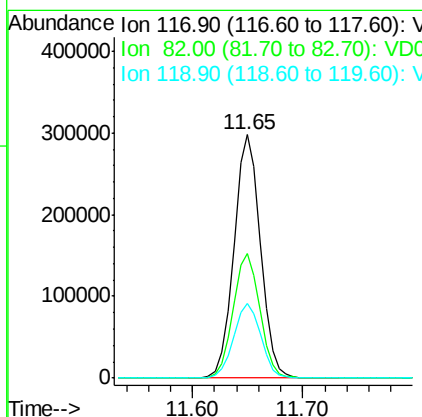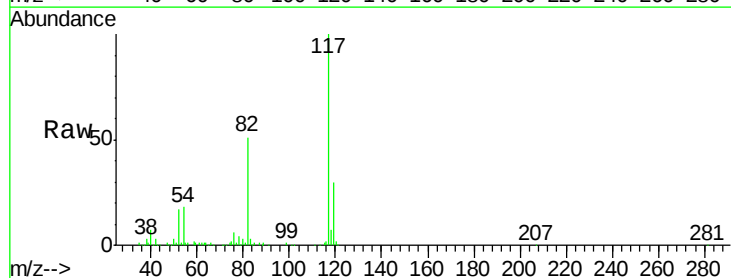

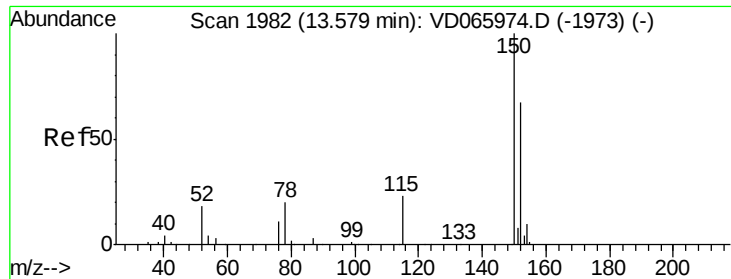

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.58 min Scan# 1983

Delta R.T. 0.01 min

Lab File: VD066045.D

Acq: 24 Jul 2020 14:17

Instrument :

MSVOA_D

ClientSampleId :

CRT-008


Tot Ion:152 Resp: 268069

Ion Ratio Lower Upper

152 100

115 54.9 27.9 83.7

150 153.4 0.0 348.2

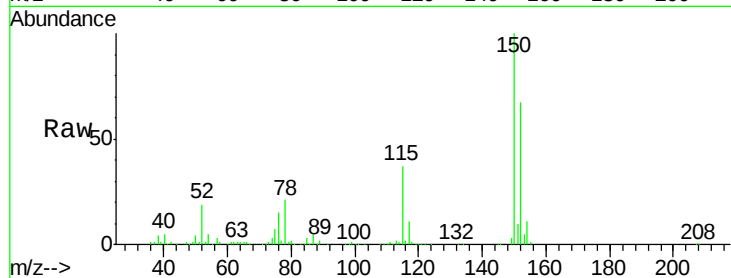

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

