

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD072420\
 Data File : VD066053.D
 Acq On : 24 Jul 2020 17:56
 Operator : VA/SY
 Sample : L3372-02
 Misc : 8.42G/5.00ml/MSVOA D/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 FK-BPM-04-011-ABCD

Quant Time: Jul 25 00:47:10 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D072120S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 21 12:34:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.98	168	292565	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.87	114	450315	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	483755	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	260095	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.33	65	118470	49.77	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.54%	
35) Dibromofluoromethane	7.91	113	138302	50.64	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.28%	
50) Toluene-d8	10.34	98	549045	53.96	ug/l	0.00
Spiked Amount	50.000		Recovery	=	107.92%	
62) 4-Bromofluorobenzene	12.64	95	222836	63.16	ug/l	0.00
Spiked Amount	50.000		Recovery	=	126.32%	


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD072420\
Data File : VD066053.D
Acq On : 24 Jul 2020 17:56
Operator : VA/SY
Sample : L3372-02
Misc : 8.42G/5.00ml/MSVOA D/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
FK-BPM-04-011-ABCD

Quant Time: Jul 25 00:47:10 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D072120S.M
Quant Title : SW846 8260
QLast Update : Tue Jul 21 12:34:13 2020
Response via : Initial Calibration

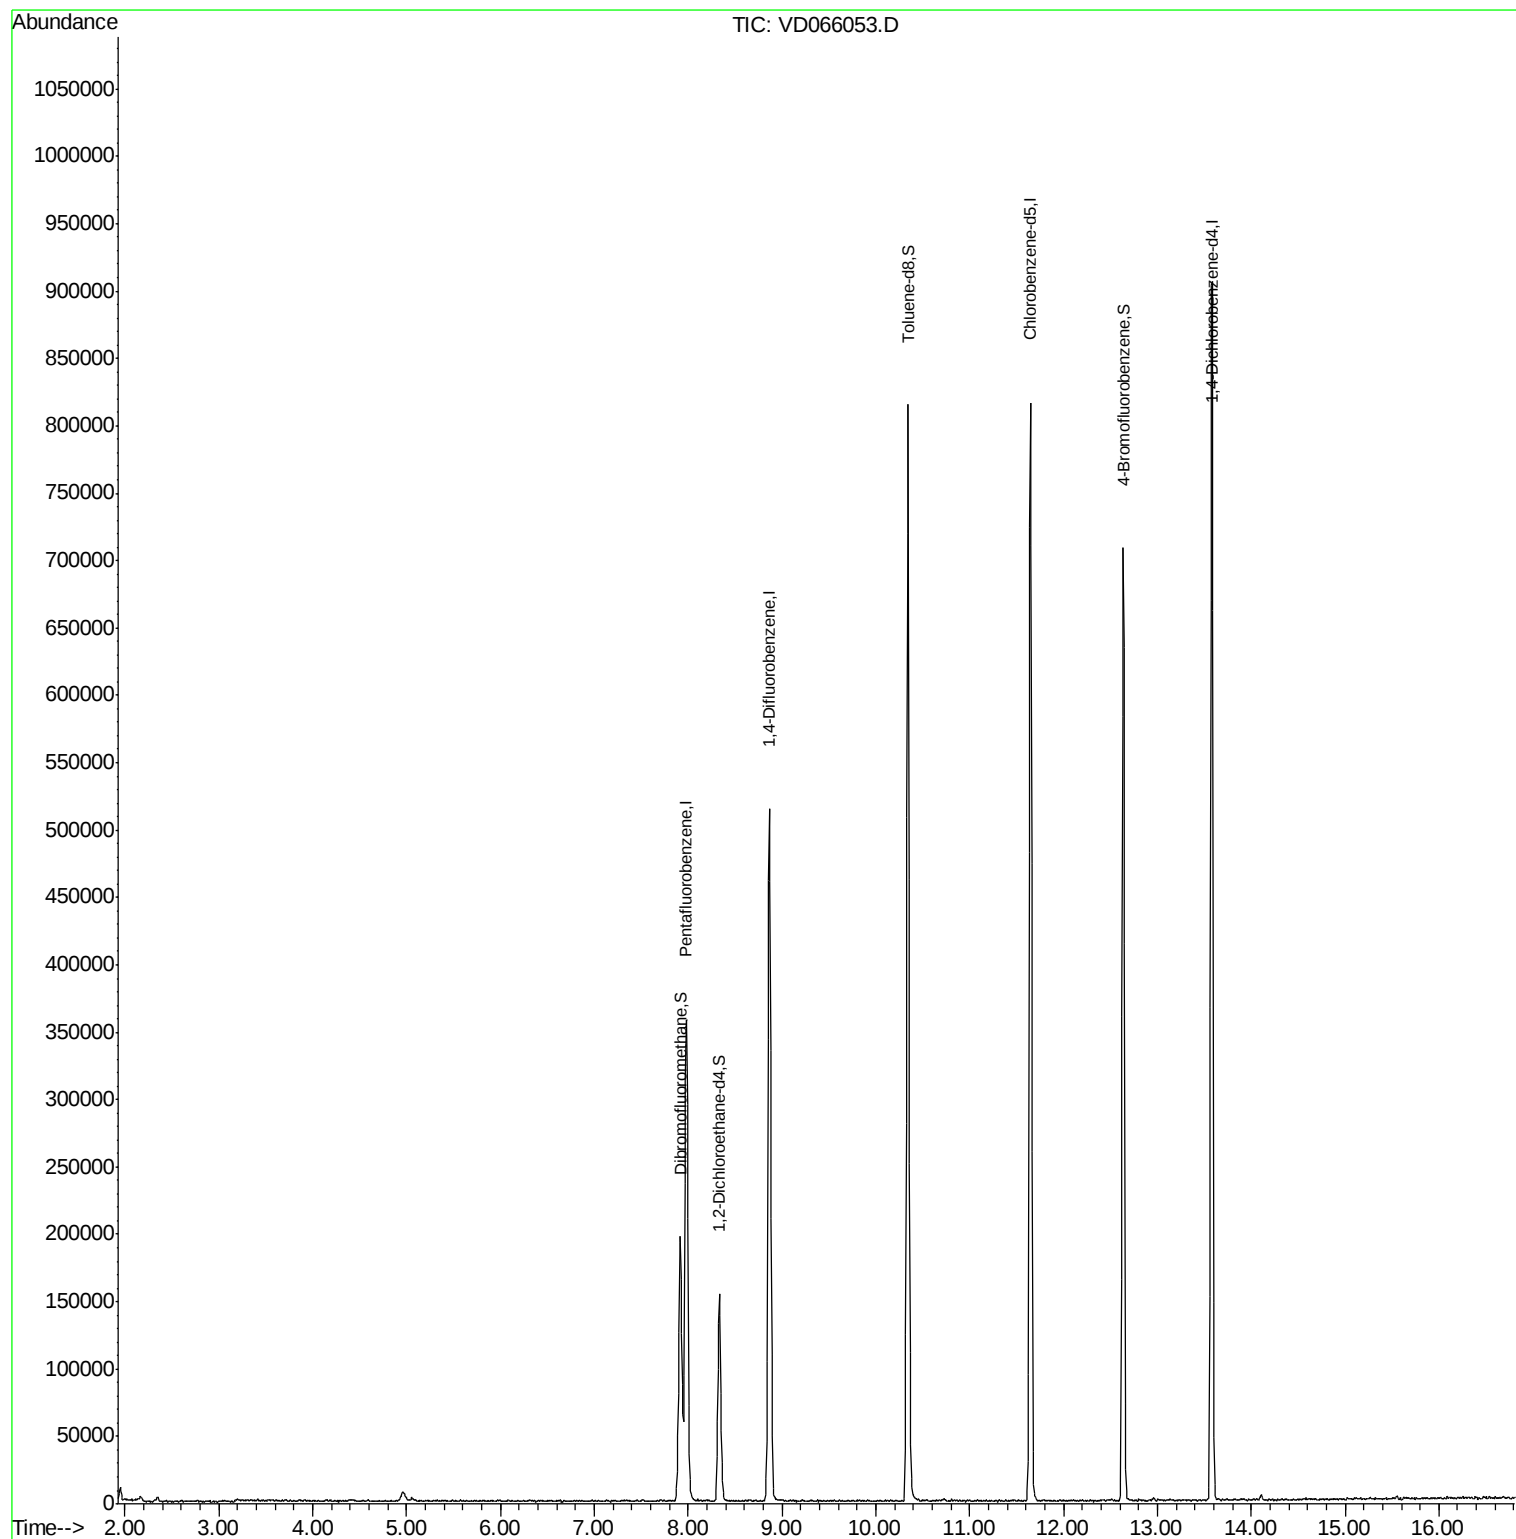



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.98 min Scan# 1030

Delta R.T. -0.00 min

Lab File: VD066053.D

Acq: 24 Jul 2020 17:56

Instrument :

MSVOA_D

ClientSampleId :


FK-BPM-04-011-ABCD

Tot Ion:168 Resp: 292565

Ion Ratio Lower Upper

168 100

99 50.5 40.8 61.2

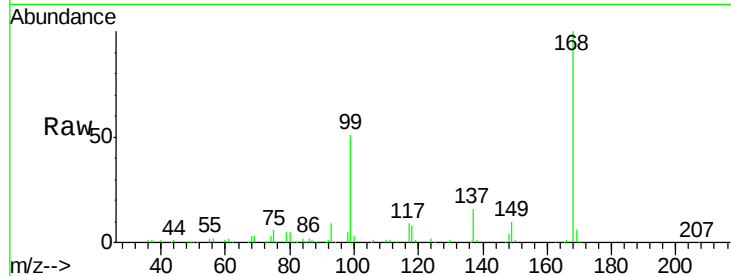

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

7.98



150000

100000

50000

0

Time-->

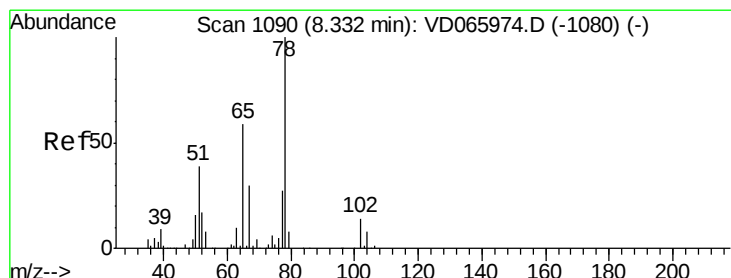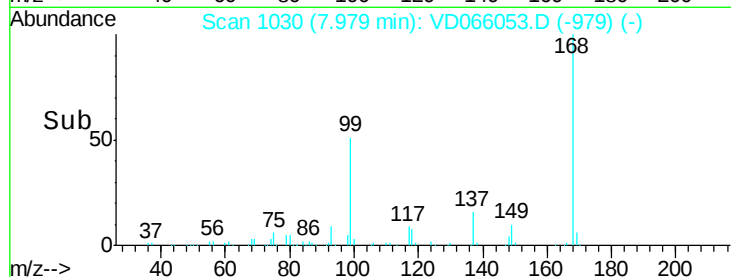

#33

1,2-Dichloroethane-d4

Concen: 49.765 ug/l

RT: 8.33 min Scan# 1090

Delta R.T. -0.00 min

Lab File: VD066053.D


Acq: 24 Jul 2020 17:56

Tgt Ion: 65 Resp: 118470

Ion Ratio Lower Upper

65 100

67 51.7 0.0 105.0

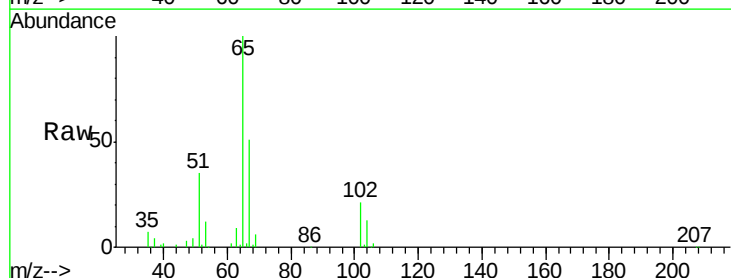

Abundance Ion 64.90 (64.60 to 65.60): VDC

Ion 66.90 (66.60 to 67.60): VDC

8.33

60000

50000

40000


30000


20000

10000

0

Time-->

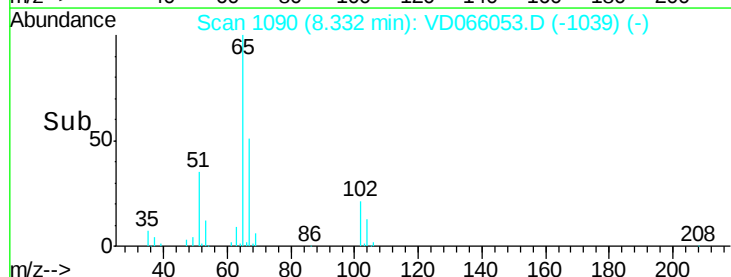


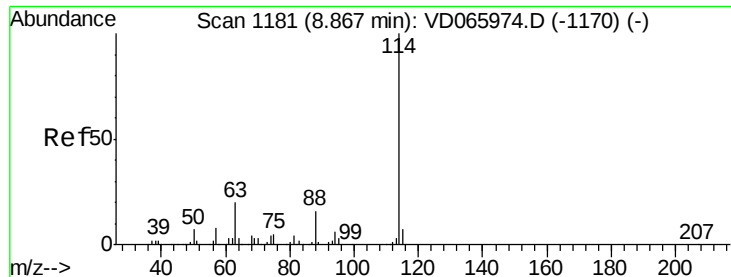




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.87 min Scan# 1181
 Delta R.T. -0.00 min
 Lab File: VD066053.D
 Acq: 24 Jul 2020 17:56

Instrument :
 MSVOA_D
 ClientSampleId :
 FK-BPM-04-011-ABCD

Tot Ion	Ratio	Lower	Upper
114	100		
63	17.8	0.0	39.6
88	15.0	0.0	31.2

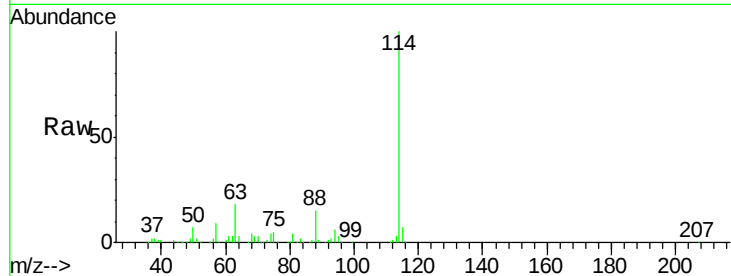


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): V
 Ion 87.90 (87.60 to 88.60): V

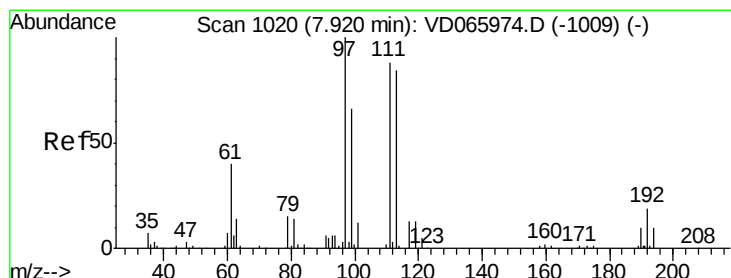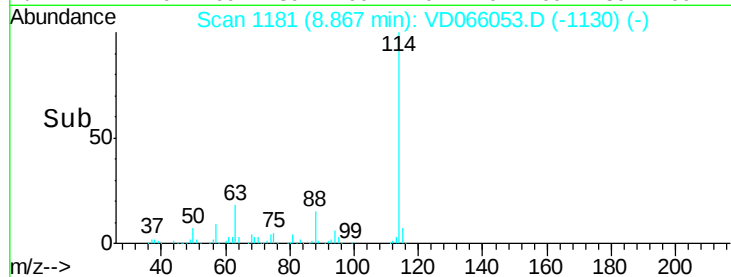
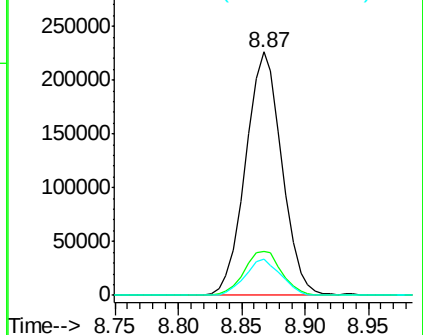



#35
 Dibromofluoromethane
 Concen: 50.636 ug/l
 RT: 7.91 min Scan# 1019
 Delta R.T. -0.01 min
 Lab File: VD066053.D
 Acq: 24 Jul 2020 17:56

Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.1	83.2	124.8
192	23.3	18.7	28.1

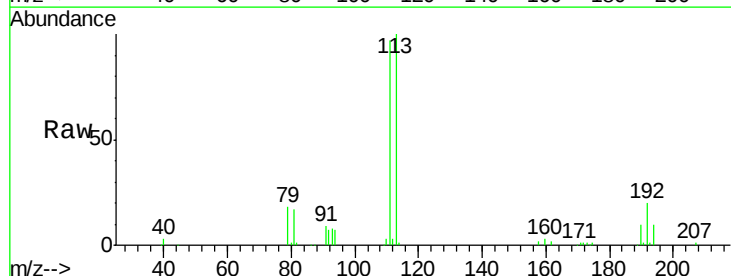

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V



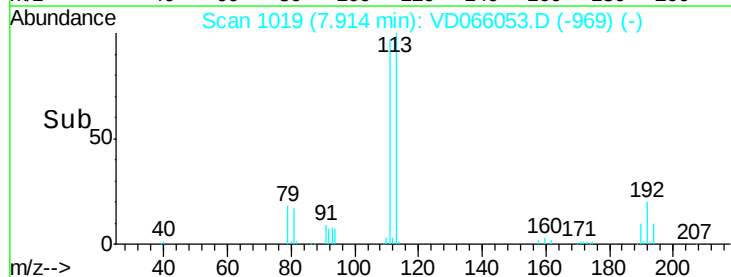
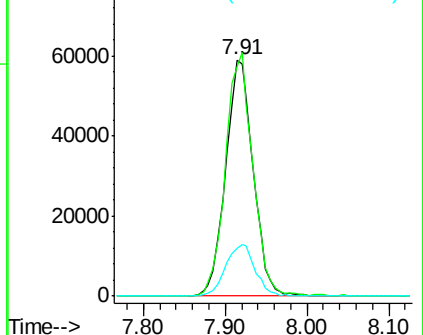


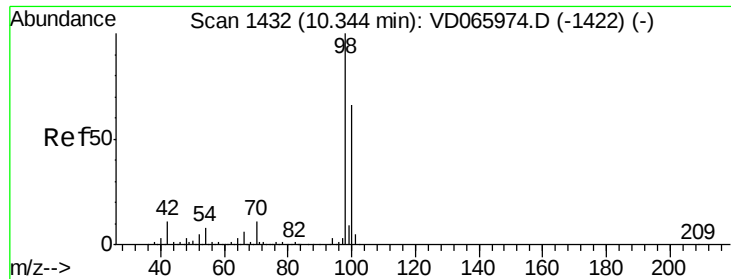

#50
Toluene-d8
Concen: 53.961 ug/l
RT: 10.34 min Scan# 1432
Delta R.T. -0.00 min
Lab File: VD066053.D
Acq: 24 Jul 2020 17:56




Instrument :
MSVOA_D
ClientSampleId :
FK-BPM-04-011-ABCD


Tot Ion: 98 Resp: 549045
Ion Ratio Lower Upper
98 100
100 66.3 52.7 79.1

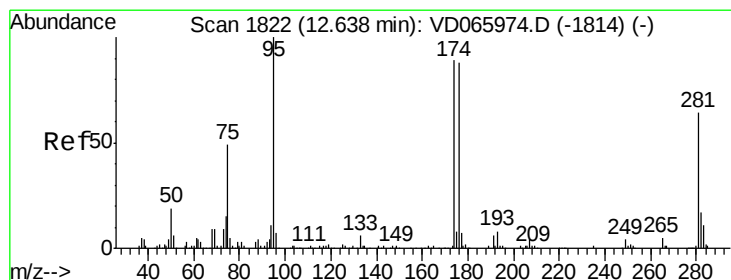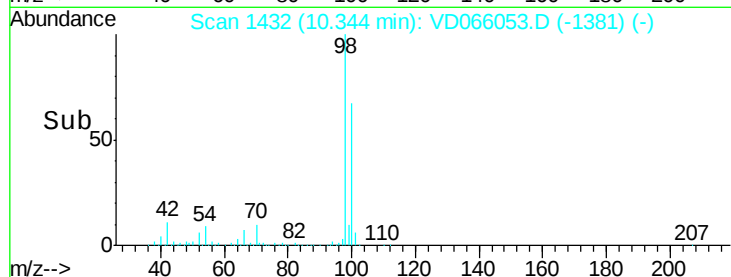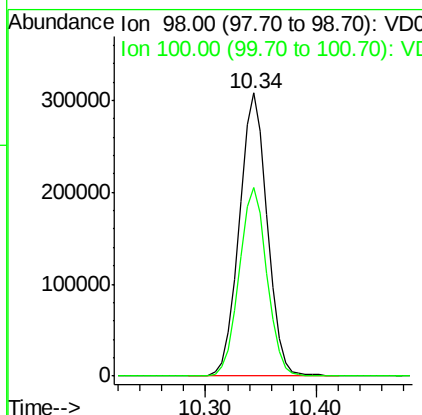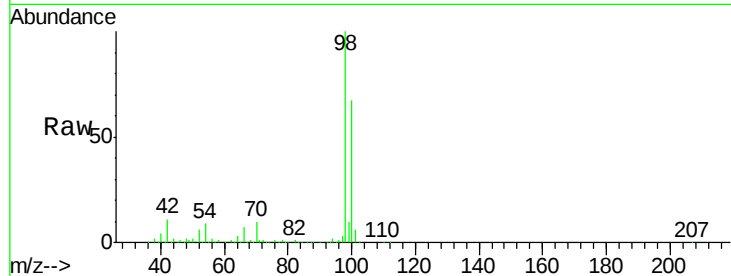

#62
4-Bromofluorobenzene
Concen: 63.162 ug/l
RT: 12.64 min Scan# 1822
Delta R.T. -0.00 min
Lab File: VD066053.D
Acq: 24 Jul 2020 17:56

Tgt Ion: 95 Resp: 222836
Ion Ratio Lower Upper
95 100
174 93.1 0.0 178.8
176 88.0 0.0 172.6


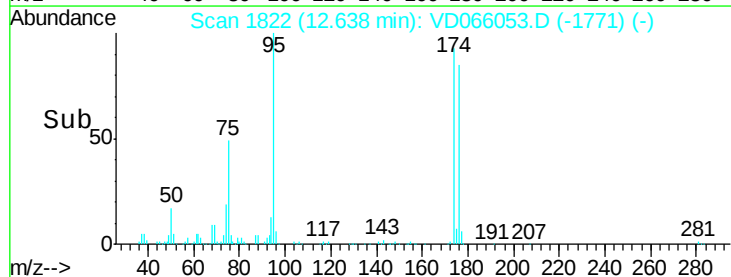
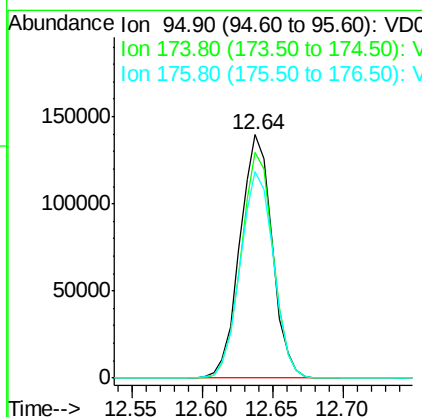
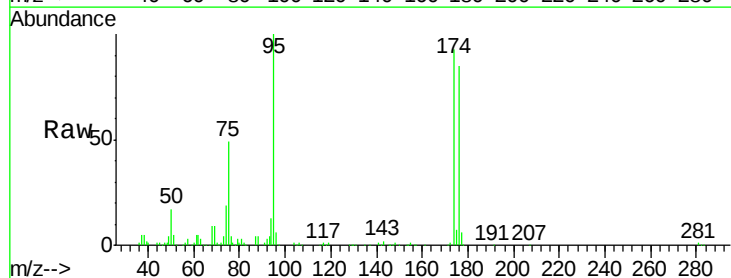


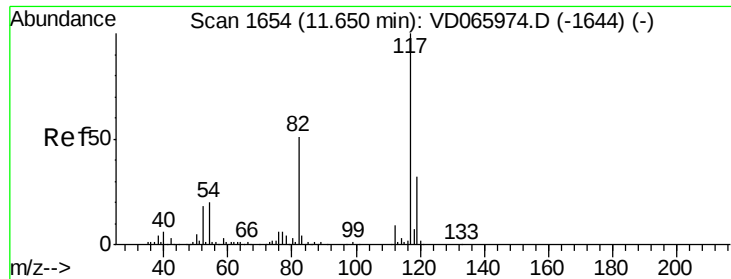

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.65 min Scan# 1654
Delta R.T. -0.00 min
Lab File: VD066053.D
Acq: 24 Jul 2020 17:56

Instrument :
MSVOA_D
ClientSampleId :
FK-BPM-04-011-ABCD

Tot Ion:117 Resp: 483755
Ion Ratio Lower Upper
117 100
82 53.8 41.1 61.7
119 32.7 25.9 38.9

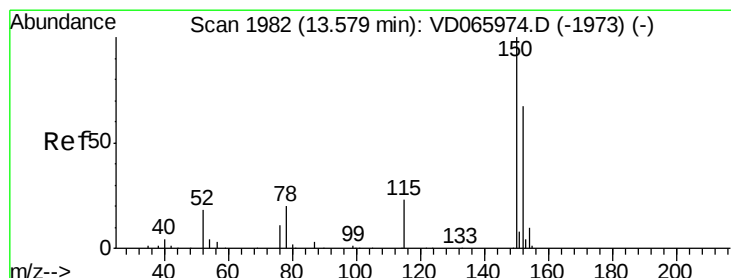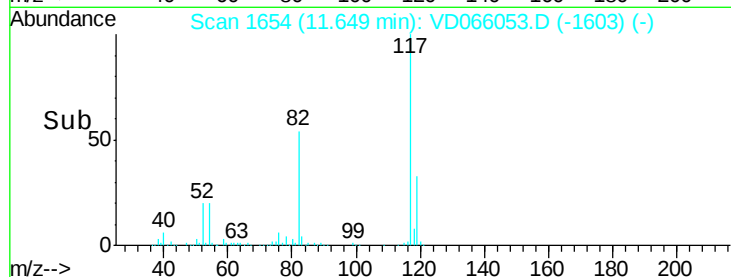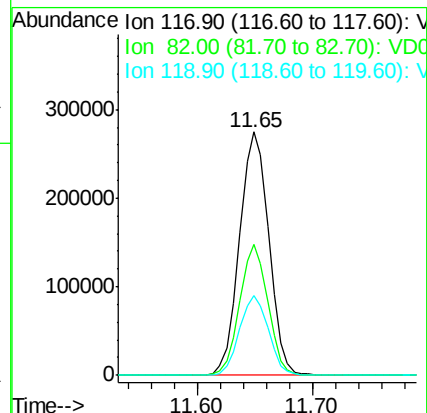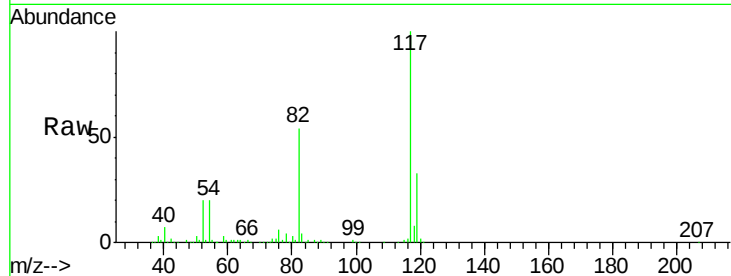

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.58 min Scan# 1982
Delta R.T. -0.00 min
Lab File: VD066053.D
Acq: 24 Jul 2020 17:56

Tgt Ion:152 Resp: 260095
Ion Ratio Lower Upper
152 100
115 56.1 27.9 83.7
150 156.5 0.0 348.2

