


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD072618\
Data File : VD059602.D
Acq On : 26 Jul 2018 12:36
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D072418S.M
Title : SW846 8260
Last Update : Wed Jul 25 07:10:33 2018

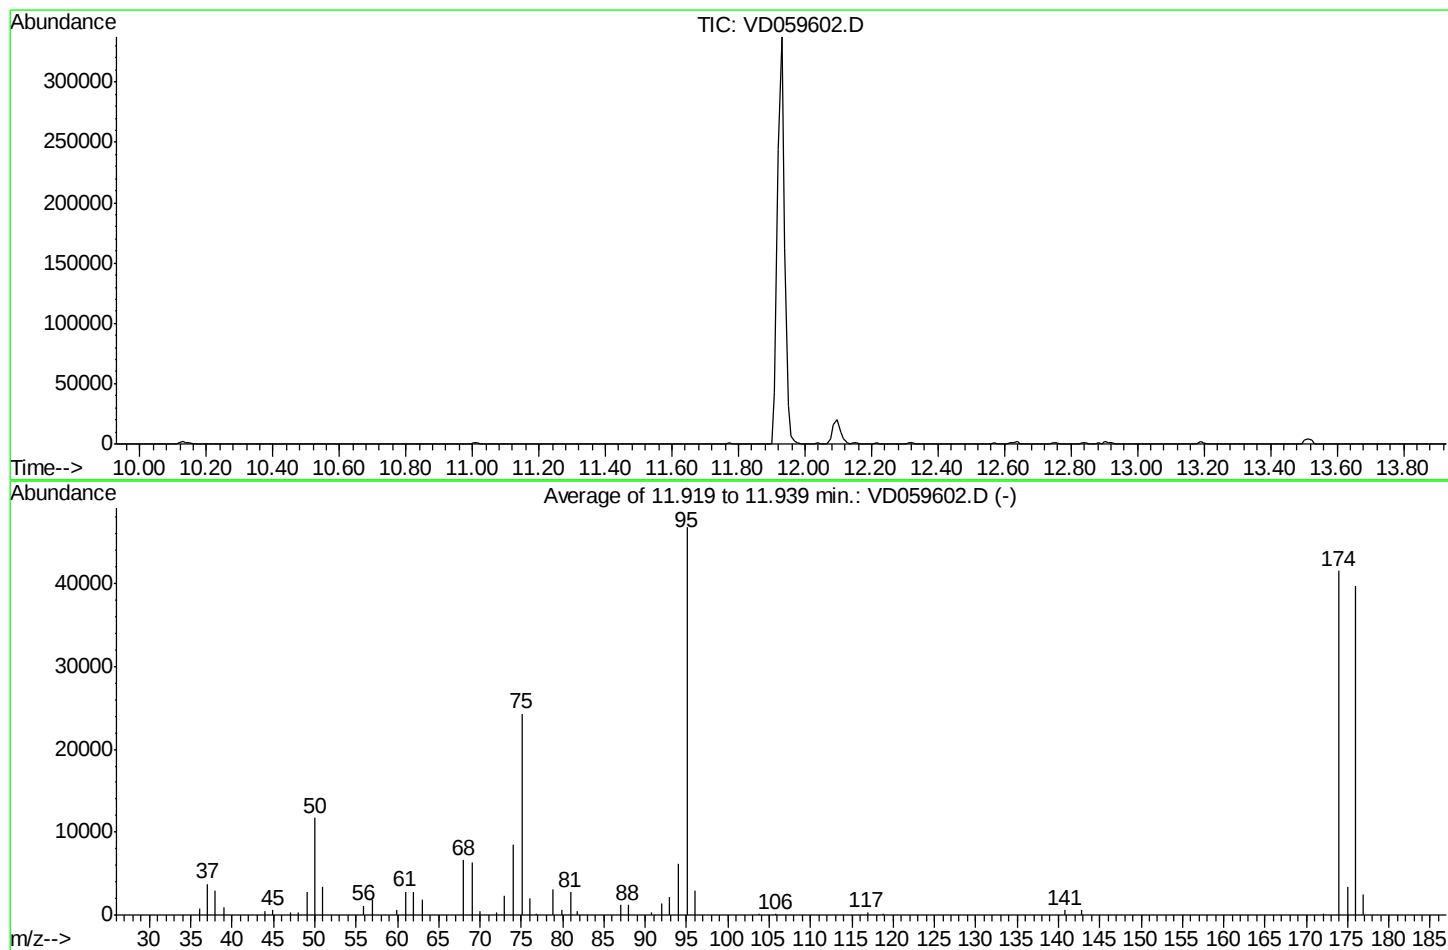

AutoFind: Scans 1189, 1190, 1191; Background Corrected with Scan 1184

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.0	11677	PASS
75	95	30	60	51.9	24289	PASS
95	95	100	100	100.0	46792	PASS
96	95	5	9	6.2	2890	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	88.8	41536	PASS
175	174	5	9	8.2	3423	PASS
176	174	95	101	95.8	39786	PASS
177	176	5	9	6.2	2470	PASS