

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD072623\
 Data File : VD076807.D
 Acq On : 26 Jul 2023 15:50
 Operator : KP/SY
 Sample : 03769-02
 Misc : 5.03G/5.0ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 B-P4B

Quant Time: Jul 27 04:23:58 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D071423S.M
 Quant Title : SW846 8260
 QLast Update : Mon Jul 17 08:07:52 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.875	168	214865	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.775	114	427315	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	388452	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	166895	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	110115	51.453	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	102.900%
35) Dibromofluoromethane	7.805	113	136525	50.842	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	101.680%
50) Toluene-d8	10.269	98	508551	52.940	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	105.880%
62) 4-Bromofluorobenzene	12.575	95	146123	47.021	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	94.040%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD072623\
Data File : VD076807.D
Acq On : 26 Jul 2023 15:50
Operator : KP/SY
Sample : 03769-02
Misc : 5.03G/5.0ml/MSVOA_D/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
B-P4B

Quant Time: Jul 27 04:23:58 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D071423S.M
Quant Title : SW846 8260
QLast Update : Mon Jul 17 08:07:52 2023
Response via : Initial Calibration




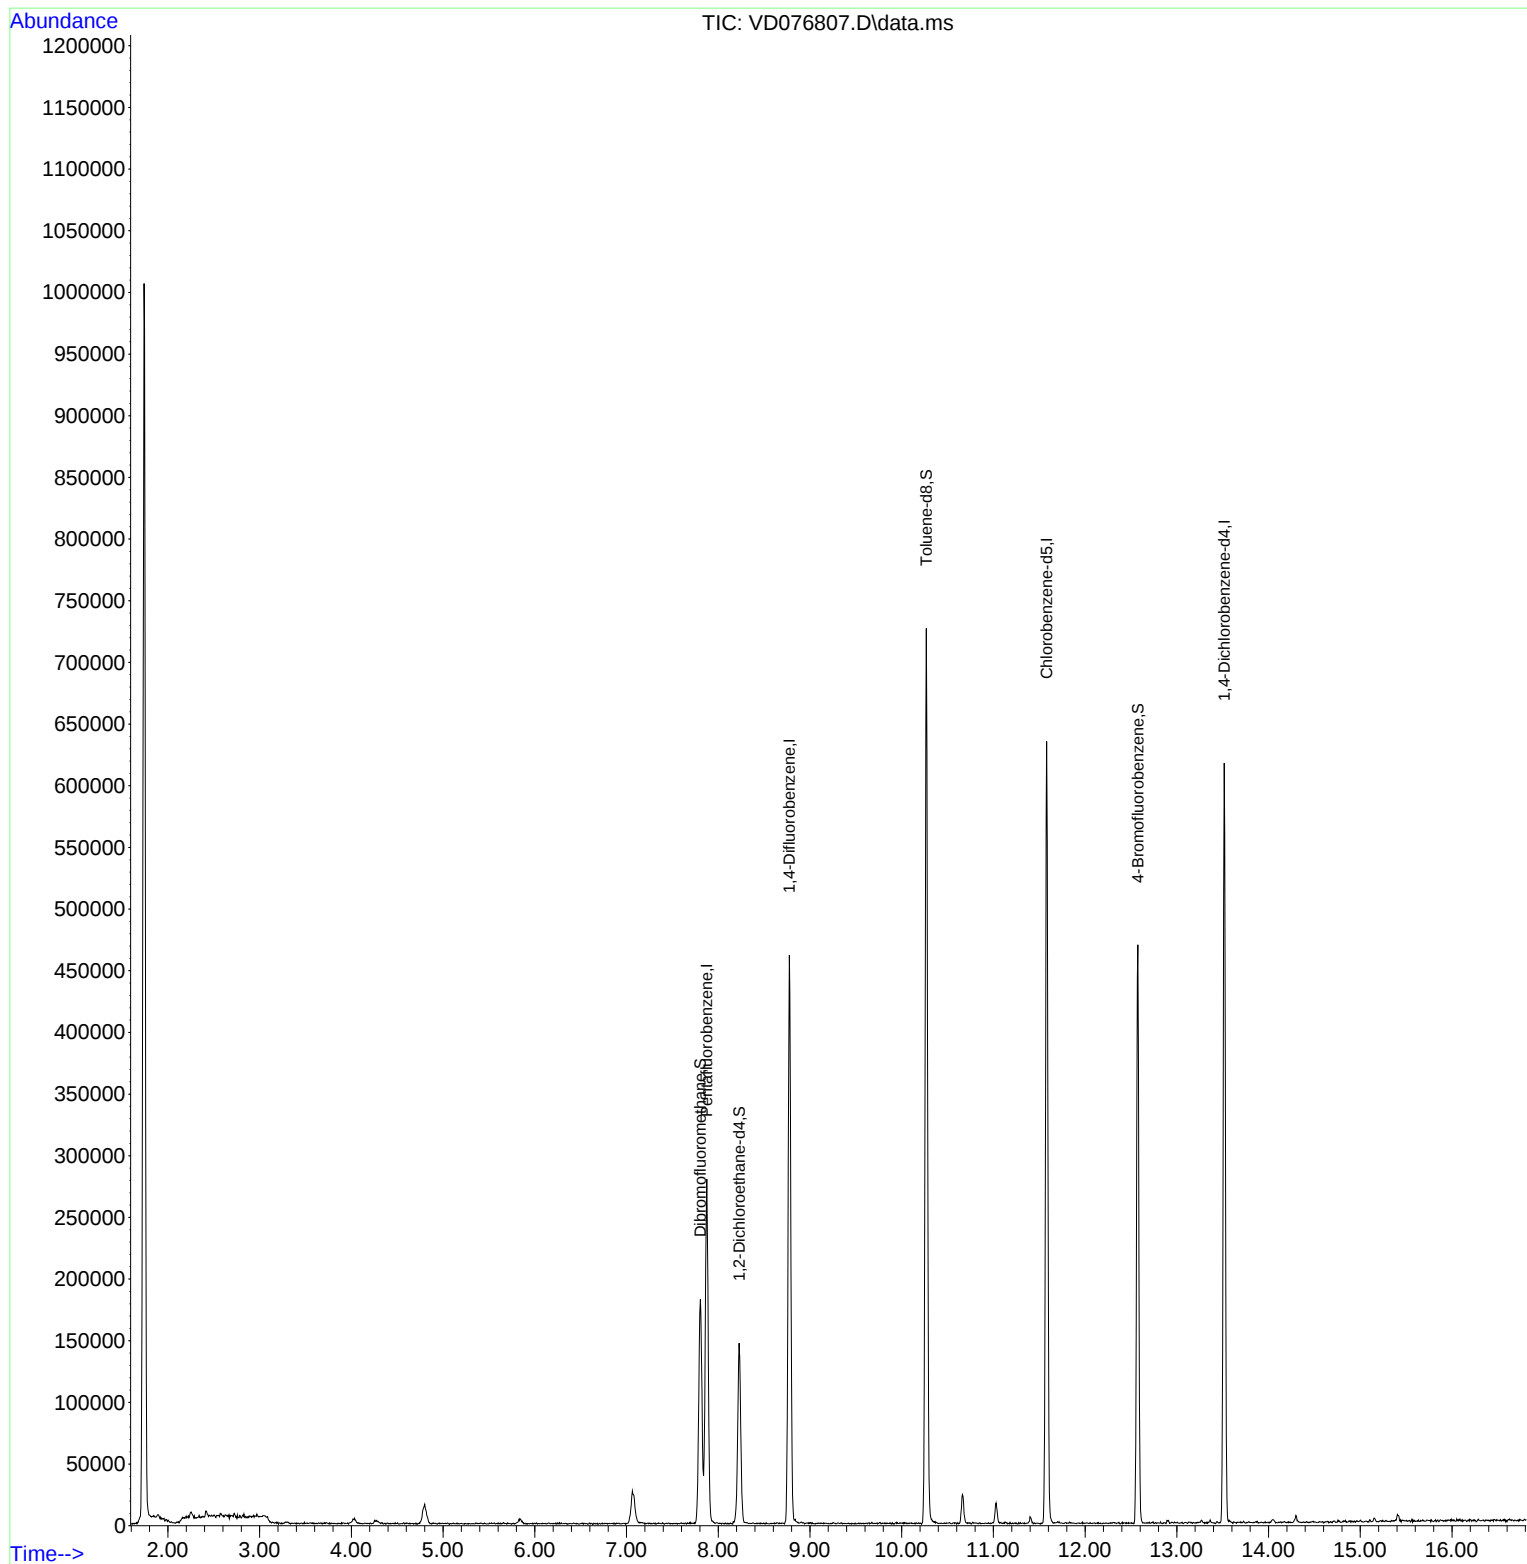


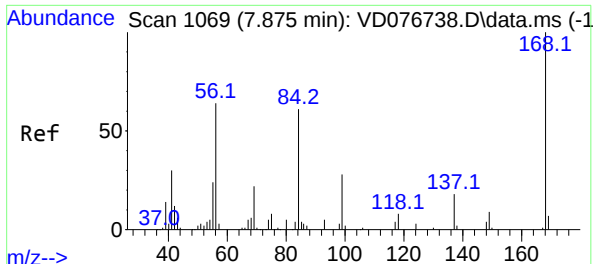

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1069
Delta R.T. 0.000 min
Lab File: VD076807.D
Acq: 26 Jul 2023 15:50




Instrument :
MSVOA_D
ClientSampleId :
B-P4B


Tgt Ion:168 Resp: 214865
Ion Ratio Lower Upper
168 100
99 50.8 36.7 55.1

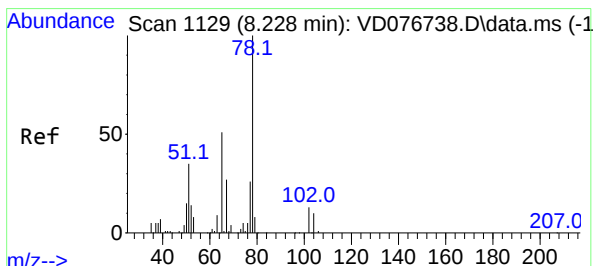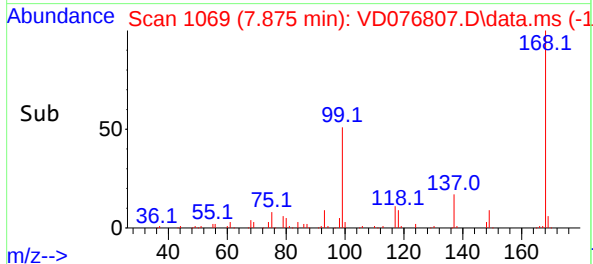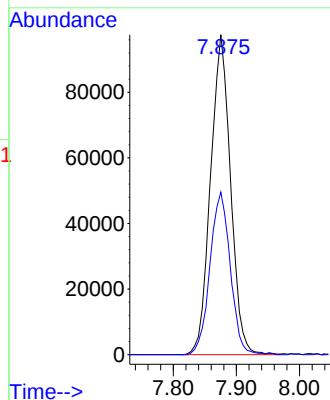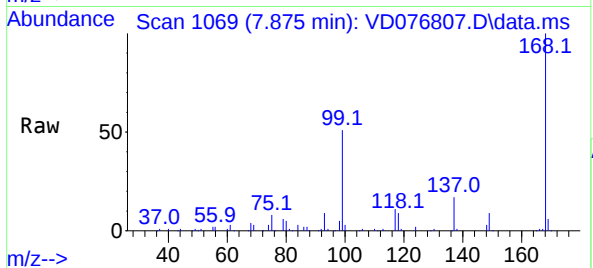

#33
1,2-Dichloroethane-d4
Concen: 51.453 ug/l
RT: 8.228 min Scan# 1129
Delta R.T. 0.000 min
Lab File: VD076807.D
Acq: 26 Jul 2023 15:50

Tgt Ion: 65 Resp: 110115
Ion Ratio Lower Upper
65 100
67 54.7 0.0 115.0


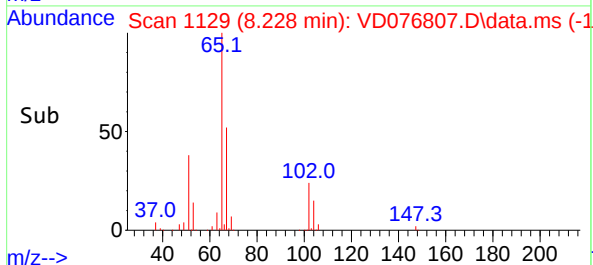
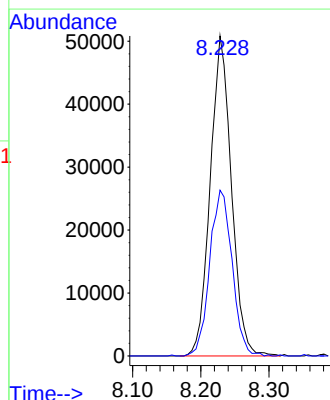
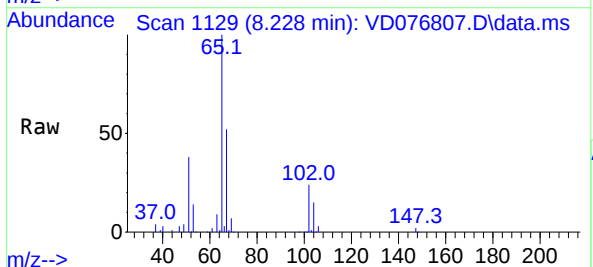


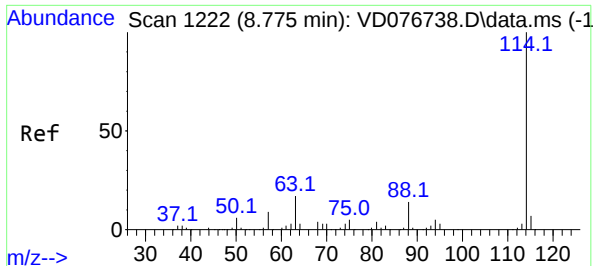

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.775 min Scan# 11
Delta R.T. 0.000 min
Lab File: VD076807.D
Acq: 26 Jul 2023 15:50




Instrument :
MSVOA_D
ClientSampleId :
B-P4B


Tgt Ion:114 Resp: 427315
Ion Ratio Lower Upper
114 100
63 17.9 0.0 33.4
88 14.0 0.0 26.2

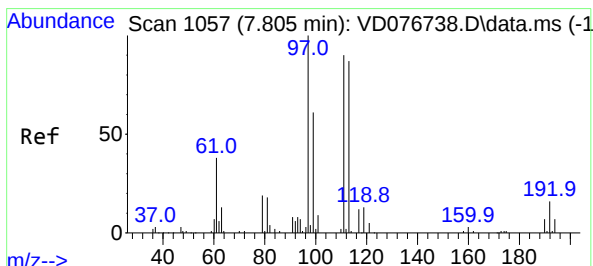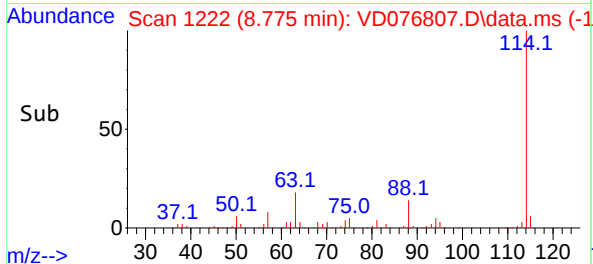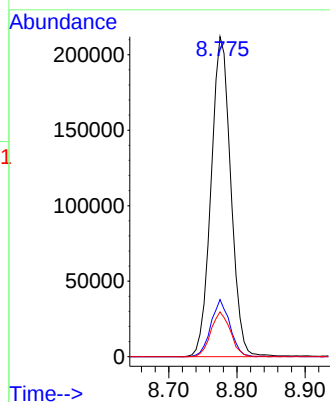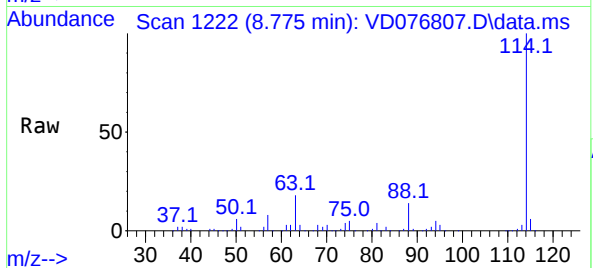

#35
Dibromofluoromethane
Concen: 50.842 ug/l
RT: 7.805 min Scan# 1057
Delta R.T. -0.000 min
Lab File: VD076807.D
Acq: 26 Jul 2023 15:50

Tgt Ion:113 Resp: 136525
Ion Ratio Lower Upper
113 100
111 101.8 84.7 127.1
192 18.1 16.8 25.2


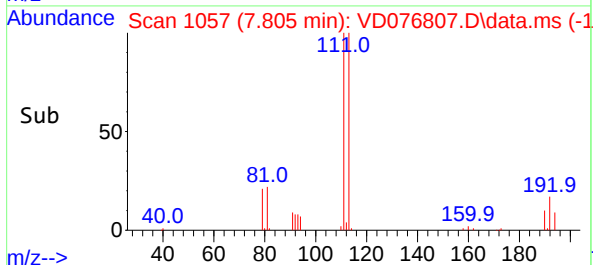
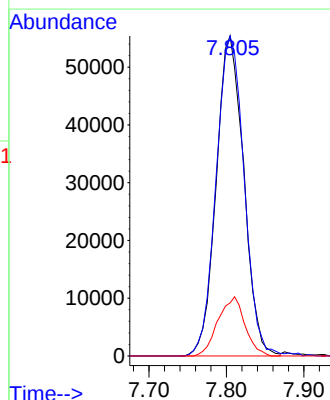
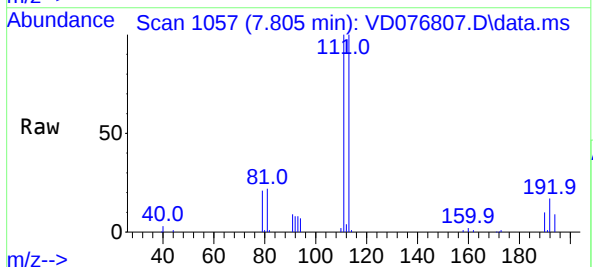


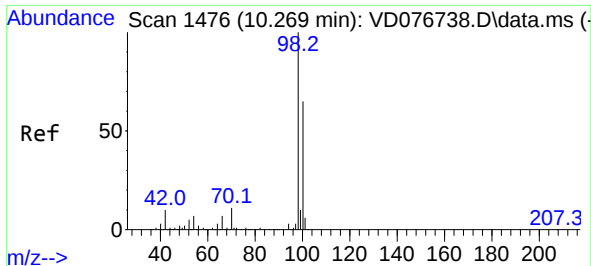

#50
Toluene-d8
Concen: 52.940 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VD076807.D
Acq: 26 Jul 2023 15:50




Instrument :
MSVOA_D
ClientSampleId :
B-P4B


Tgt Ion: 98 Resp: 508551
Ion Ratio Lower Upper
98 100
100 65.8 50.3 75.5

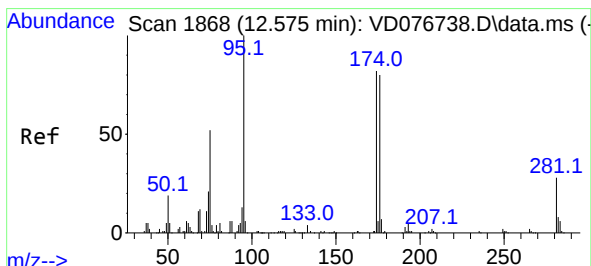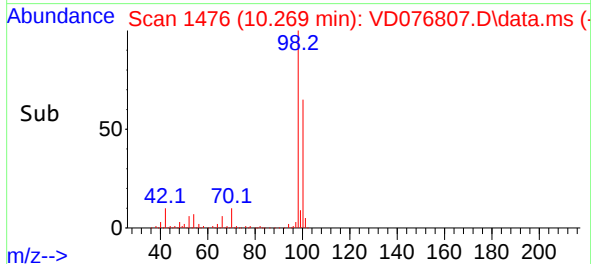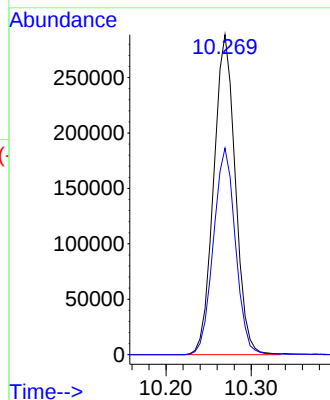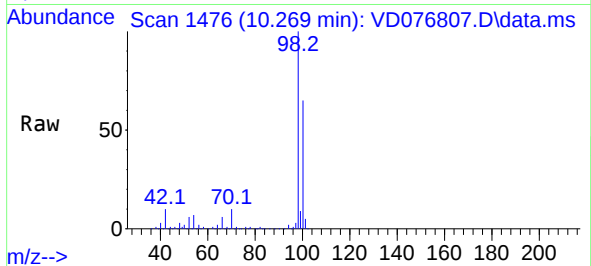

#62
4-Bromofluorobenzene
Concen: 47.021 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD076807.D
Acq: 26 Jul 2023 15:50

Tgt Ion: 95 Resp: 146123
Ion Ratio Lower Upper
95 100
174 88.7 0.0 201.8
176 84.2 0.0 191.8


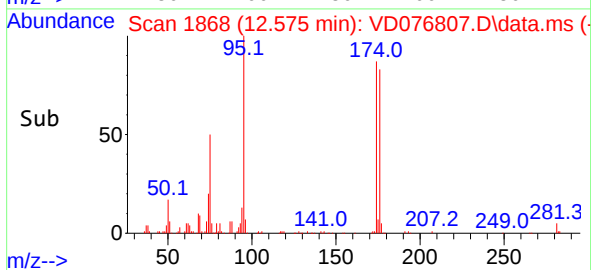
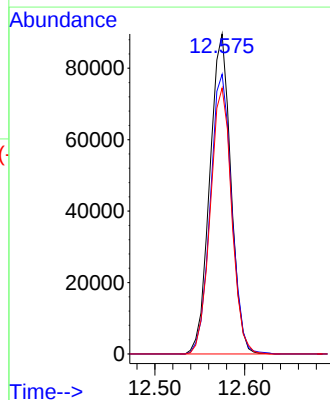
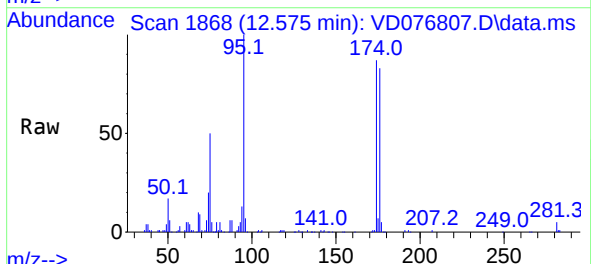


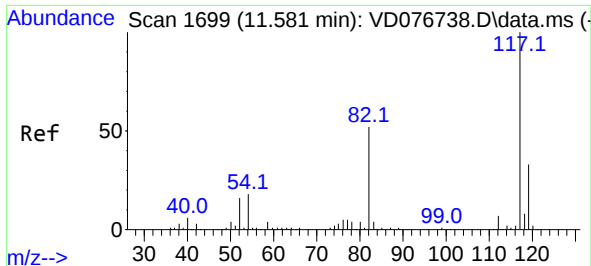

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 117
Delta R.T. 0.000 min
Lab File: VD076807.D
Acq: 26 Jul 2023 15:50

Instrument :
MSVOA_D
ClientSampleId :
B-P4B

Tgt Ion:117 Resp: 388452
Ion Ratio Lower Upper
117 100
82 53.9 38.3 57.5
119 31.4 25.0 37.4

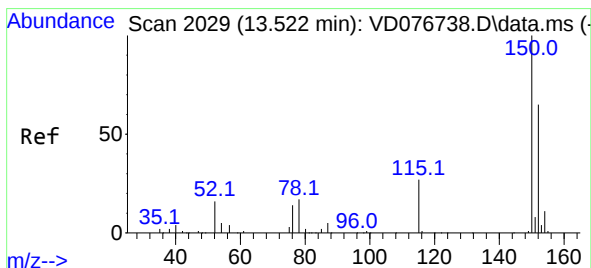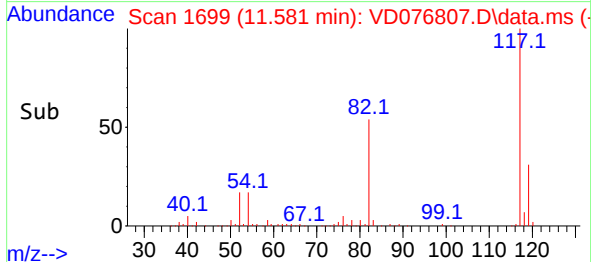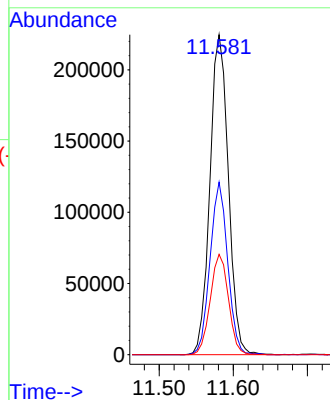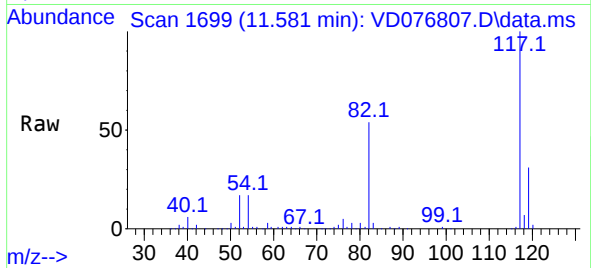

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. -0.006 min
Lab File: VD076807.D
Acq: 26 Jul 2023 15:50

Tgt Ion:152 Resp: 166895
Ion Ratio Lower Upper
152 100
115 58.2 27.1 81.3
150 156.7 0.0 353.6

