
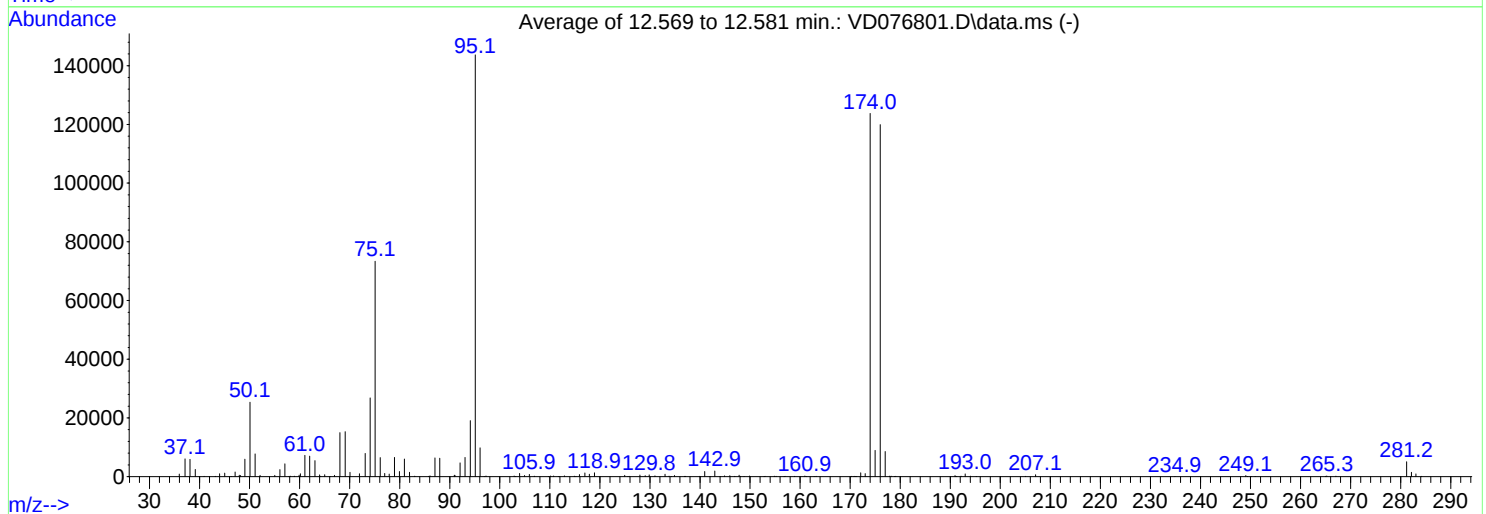


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD072623\
Data File : VD076801.D
Acq On : 26 Jul 2023 12:28
Operator : KP/SY
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D071423S.M
Title : SW846 8260
Last Update : Mon Jul 17 08:07:52 2023

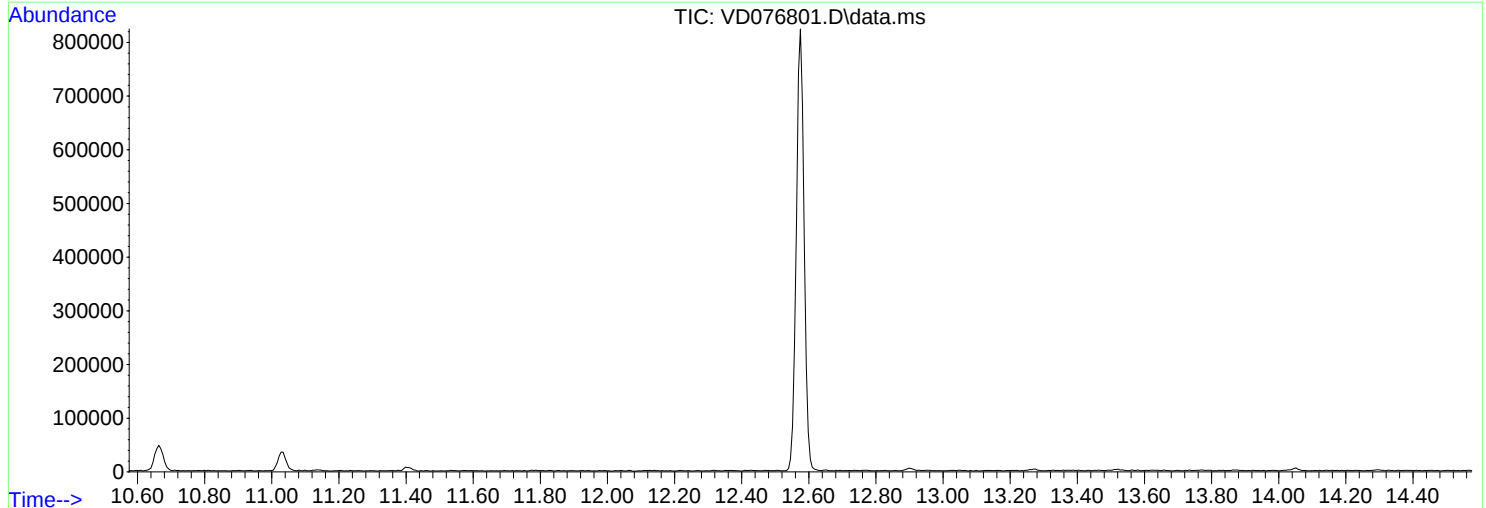

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	25360	PASS
75	95	30	60	51.1	73373	PASS
95	95	100	100	100.0	143701	PASS
96	95	5	9	6.8	9842	PASS
173	174	0.00	2	0.8	1041	PASS
174	95	50	100	86.1	123712	PASS
175	174	5	9	7.2	8949	PASS
176	174	95	101	96.9	119901	PASS
177	176	5	9	7.2	8575	PASS