


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD072820\
Data File : VD066071.D
Acq On : 28 Jul 2020 09:22
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D072120S.M
Title : SW846 8260
Last Update : Tue Jul 21 12:34:13 2020

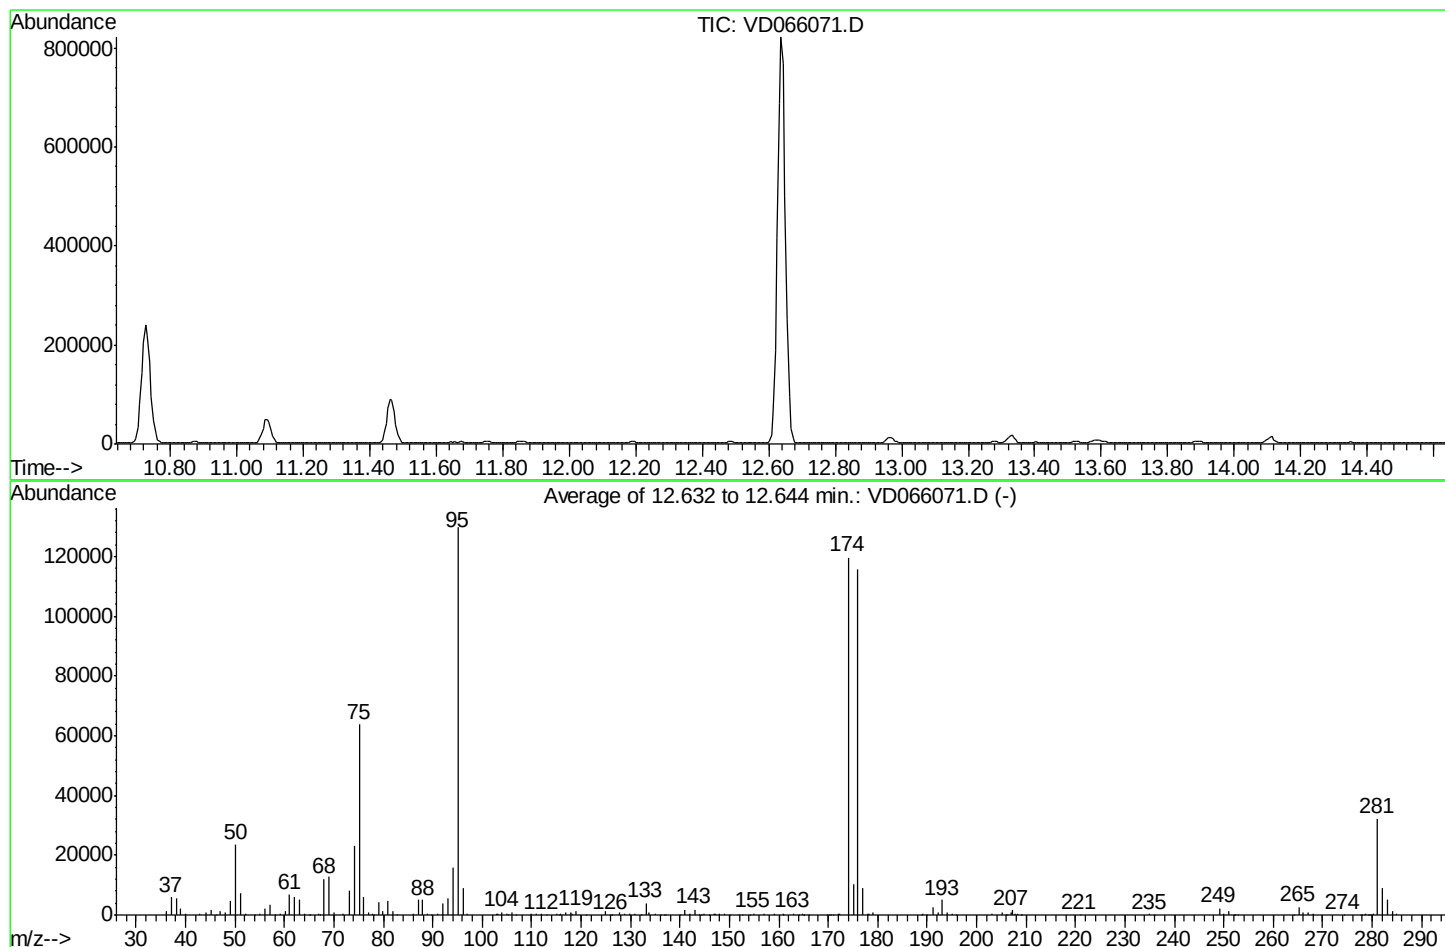

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	23397	PASS
75	95	30	60	49.1	63757	PASS
95	95	100	100	100.0	129800	PASS
96	95	5	9	6.9	9013	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	92.2	119717	PASS
175	174	5	9	8.4	10106	PASS
176	174	95	101	96.6	115677	PASS
177	176	5	9	7.8	9023	PASS