

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD072823\
 Data File : VD076853.D
 Acq On : 28 Jul 2023 14:27
 Operator : KP/SY
 Sample : 03770-10
 Misc : 5.16G/5.0ml/MSVOA_D/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 HOWE-2-LP

Quant Time: Jul 28 23:04:13 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D071423S.M
 Quant Title : SW846 8260
 QLast Update : Mon Jul 17 08:07:52 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.875	168	183985	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.775	114	351846	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	329964	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	144800	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	93132	50.821	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	101.640%
35) Dibromofluoromethane	7.804	113	110577	50.012	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.020%
50) Toluene-d8	10.269	98	432010	54.618	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	109.240%
62) 4-Bromofluorobenzene	12.575	95	130660	51.063	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	102.120%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD072823\
Data File : VD076853.D
Acq On : 28 Jul 2023 14:27
Operator : KP/SY
Sample : 03770-10
Misc : 5.16G/5.0ml/MSVOA_D/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
HOWE-2-LP

Quant Time: Jul 28 23:04:13 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D071423S.M
Quant Title : SW846 8260
QLast Update : Mon Jul 17 08:07:52 2023
Response via : Initial Calibration




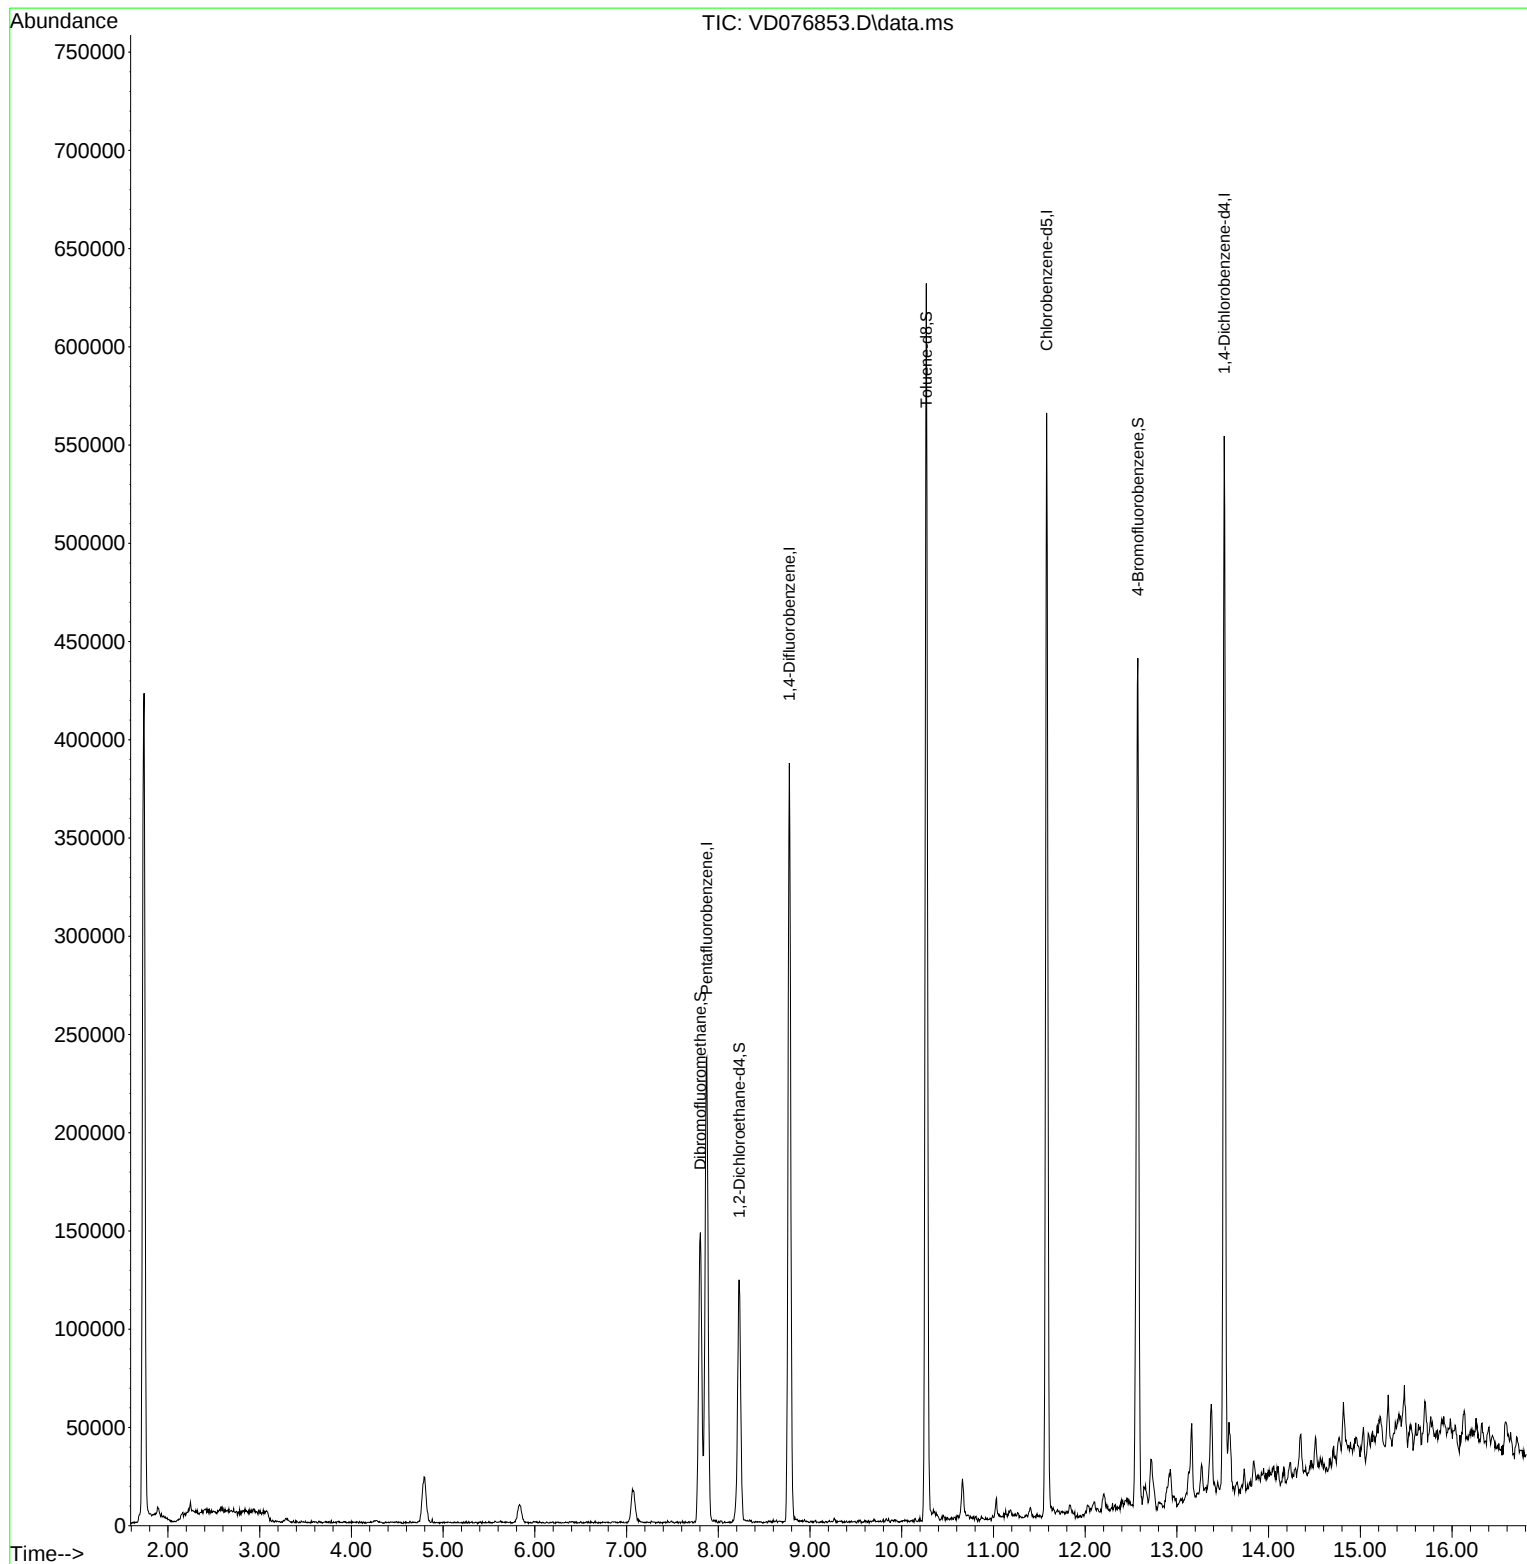


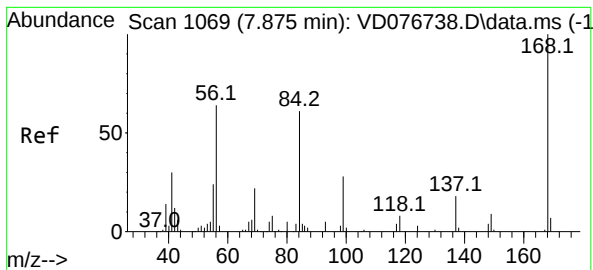

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1069
Delta R.T. 0.000 min
Lab File: VD076853.D
Acq: 28 Jul 2023 14:27




Instrument :
MSVOA_D
ClientSampleId :
HOWE-2-LP


Tgt Ion:168 Resp: 183985
Ion Ratio Lower Upper
168 100
99 53.0 36.7 55.1

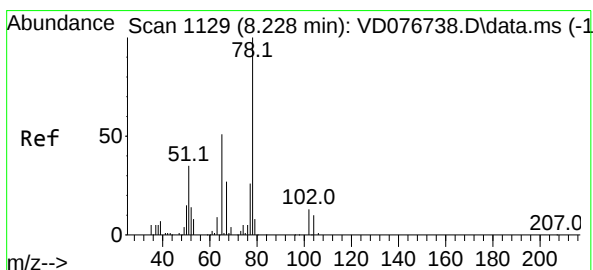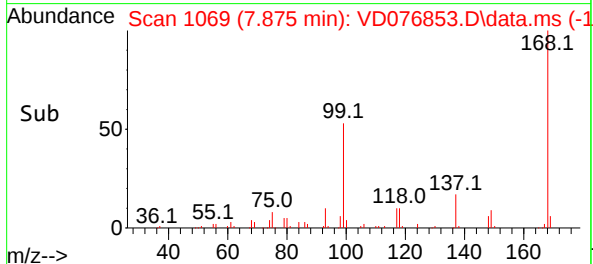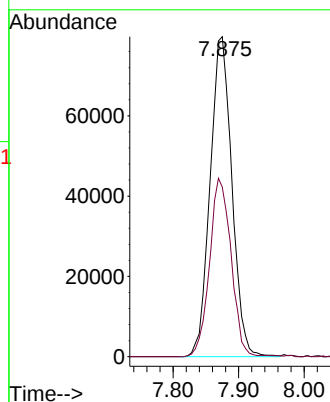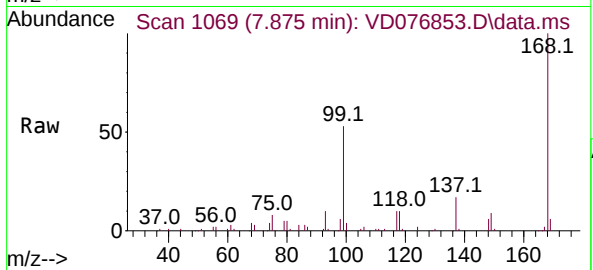

#33
1,2-Dichloroethane-d4
Concen: 50.821 ug/l
RT: 8.228 min Scan# 1129
Delta R.T. -0.000 min
Lab File: VD076853.D
Acq: 28 Jul 2023 14:27

Tgt Ion: 65 Resp: 93132
Ion Ratio Lower Upper
65 100
67 53.1 0.0 115.0

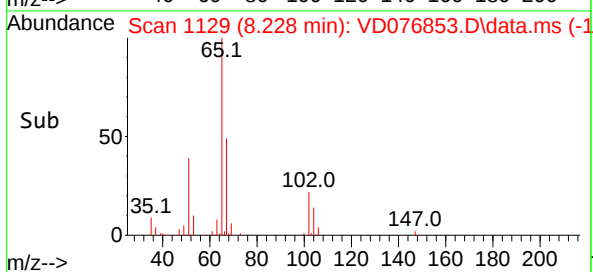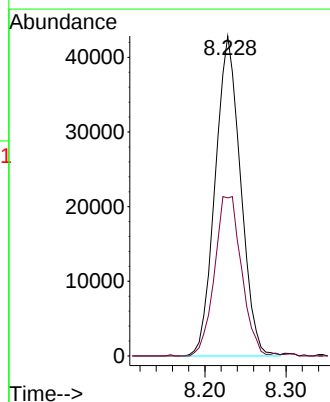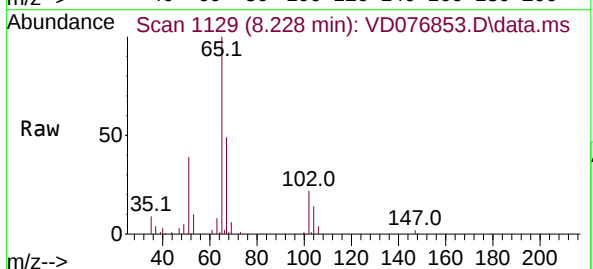

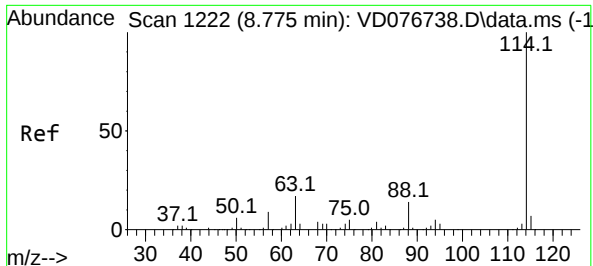

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.775 min Scan# 1

Delta R.T. -0.000 min

Lab File: VD076853.D

Acq: 28 Jul 2023 14:27

Instrument :

MSVOA_D

ClientSampleId :

HOWE-2-LP





Tgt Ion:114 Resp: 351846

Ion Ratio Lower Upper

114 100

63 16.8 0.0 33.4

88 13.8 0.0 26.2

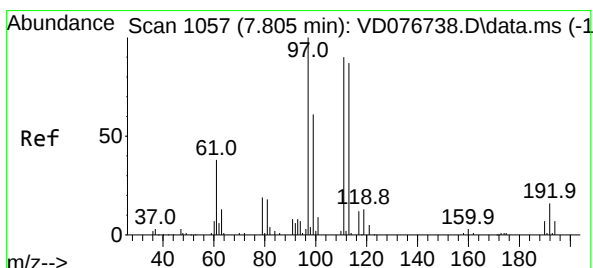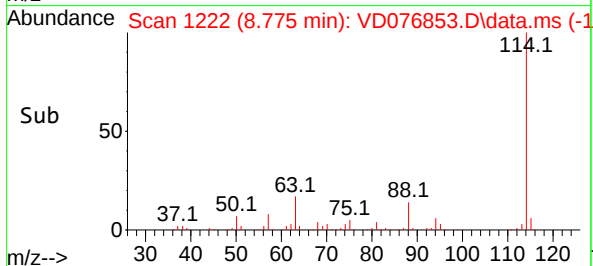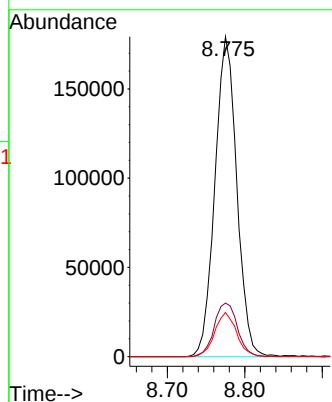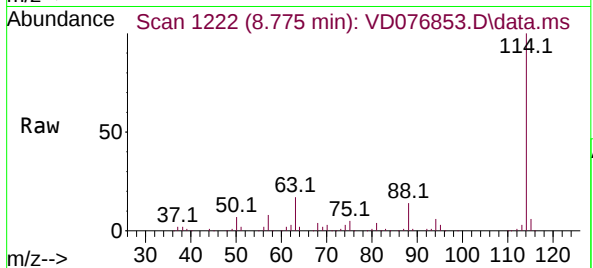

#35

Dibromofluoromethane

Concen: 50.012 ug/l

RT: 7.804 min Scan# 1057

Delta R.T. -0.001 min

Lab File: VD076853.D

Acq: 28 Jul 2023 14:27




Tgt Ion:113 Resp: 110577


Ion Ratio Lower Upper

113 100

111 100.0 84.7 127.1

192 17.6 16.8 25.2


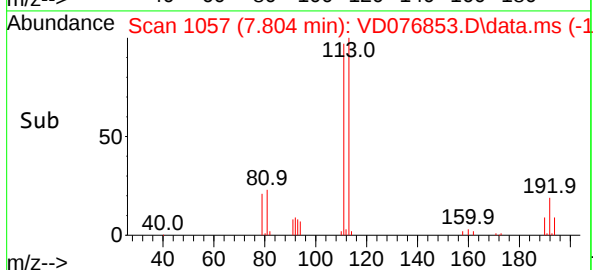
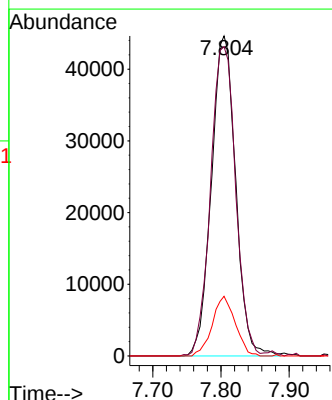
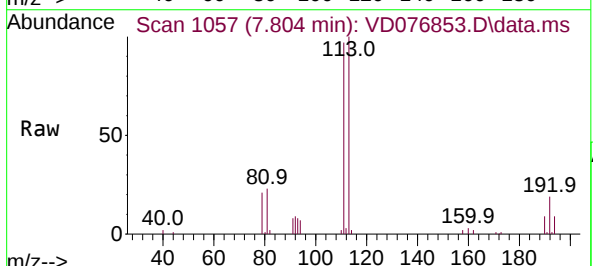


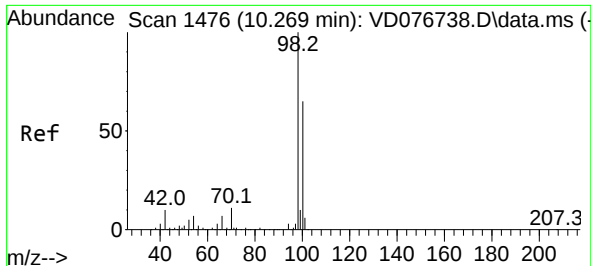

#50
Toluene-d8
Concen: 54.618 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VD076853.D
Acq: 28 Jul 2023 14:27




Instrument :
MSVOA_D
ClientSampleId :
HOWE-2-LP


Tgt Ion: 98 Resp: 432010
Ion Ratio Lower Upper
98 100
100 64.9 50.3 75.5

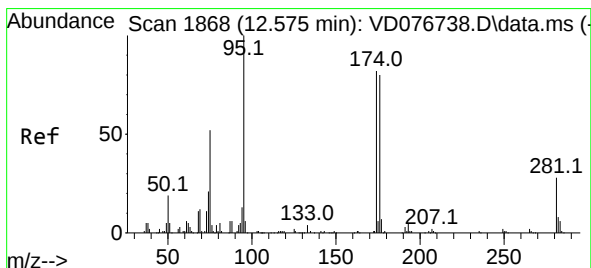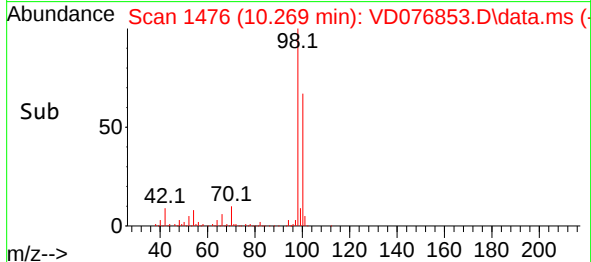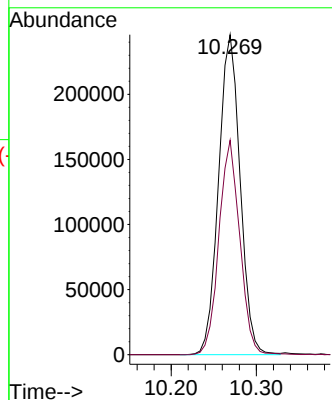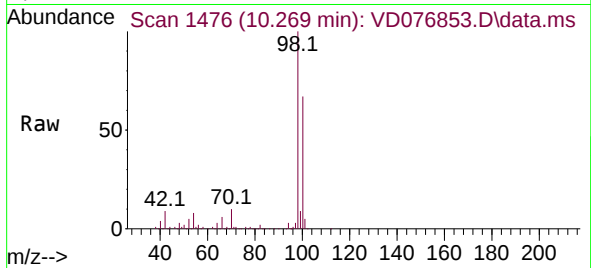

#62
4-Bromofluorobenzene
Concen: 51.063 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD076853.D
Acq: 28 Jul 2023 14:27

Tgt Ion: 95 Resp: 130660
Ion Ratio Lower Upper
95 100
174 85.0 0.0 201.8
176 83.1 0.0 191.8


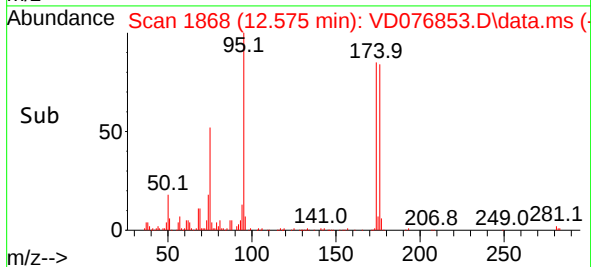
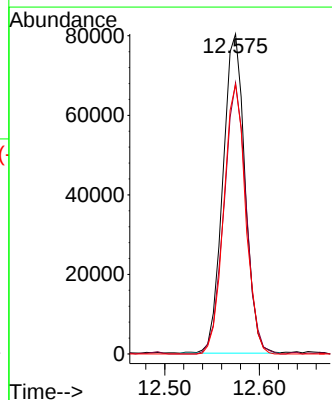
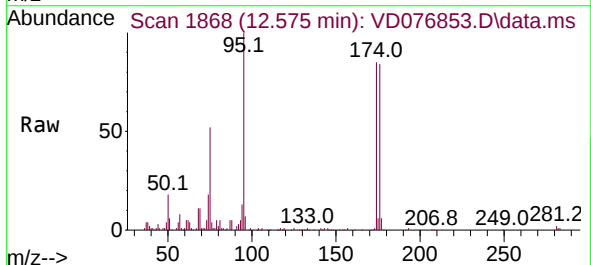


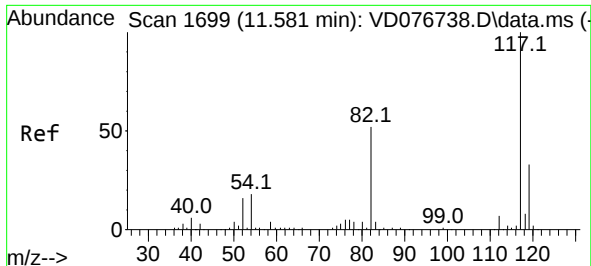

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 117
Delta R.T. -0.000 min
Lab File: VD076853.D
Acq: 28 Jul 2023 14:27

Instrument :
MSVOA_D
ClientSampleId :
HOWE-2-LP

Tgt Ion:117 Resp: 329964
Ion Ratio Lower Upper
117 100
82 51.7 38.3 57.5
119 32.1 25.0 37.4

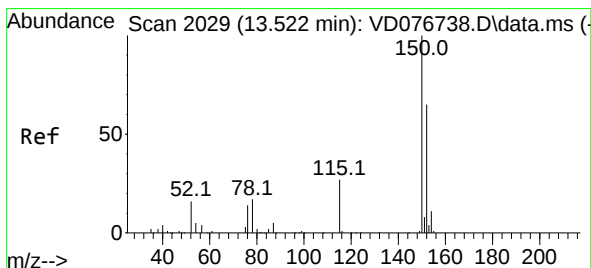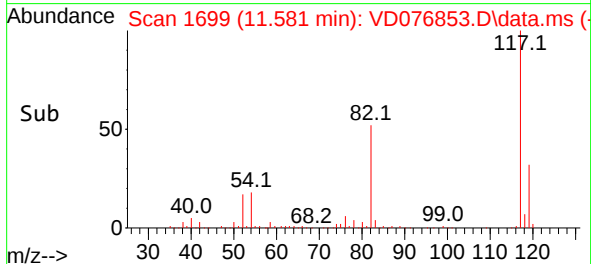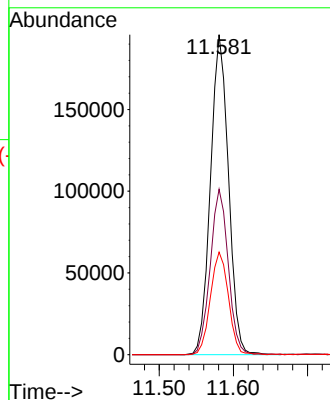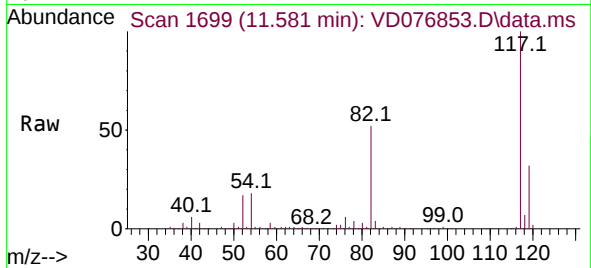

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. -0.006 min
Lab File: VD076853.D
Acq: 28 Jul 2023 14:27

Tgt Ion:152 Resp: 144800
Ion Ratio Lower Upper
152 100
115 60.4 27.1 81.3
150 156.6 0.0 353.6

