

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD072823\
 Data File : VD076856.D
 Acq On : 28 Jul 2023 15:53
 Operator : KP/SY
 Sample : 03810-03
 Misc : 5.00G/5.0ml/MSVOA_D/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 B-P16A

Quant Time: Jul 28 23:50:50 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D071423S.M
 Quant Title : SW846 8260
 QLast Update : Mon Jul 17 08:07:52 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.875	168	185788	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.775	114	349366	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	321181	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	137900	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	93406	50.476	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	100.960%
35) Dibromofluoromethane	7.804	113	109977	50.093	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.180%
50) Toluene-d8	10.269	98	423916	53.975	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	107.960%
62) 4-Bromofluorobenzene	12.575	95	119554	47.055	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	94.100%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD072823\
Data File : VD076856.D
Acq On : 28 Jul 2023 15:53
Operator : KP/SY
Sample : 03810-03
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
B-P16A

Quant Time: Jul 28 23:50:50 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D071423S.M
Quant Title : SW846 8260
QLast Update : Mon Jul 17 08:07:52 2023
Response via : Initial Calibration



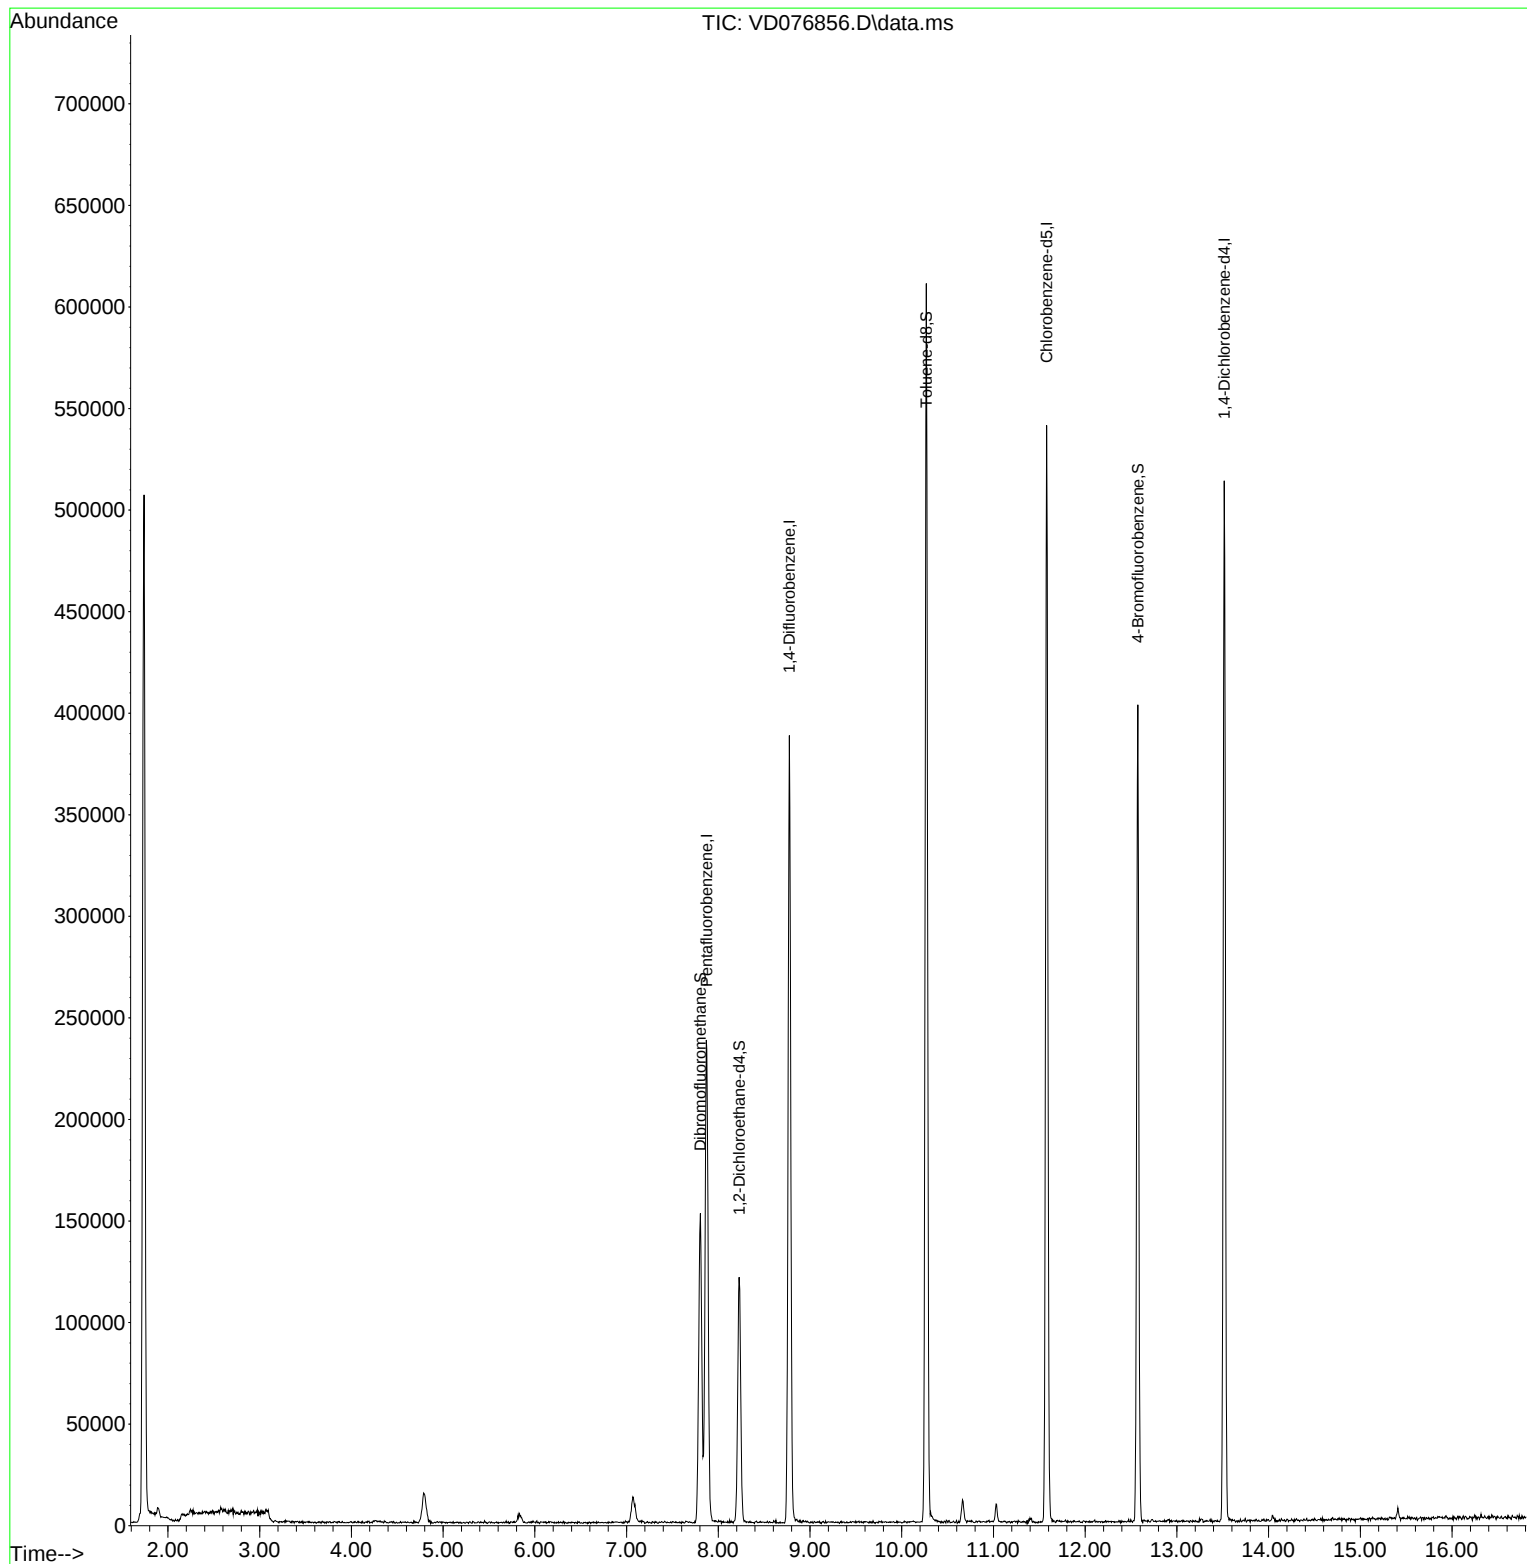


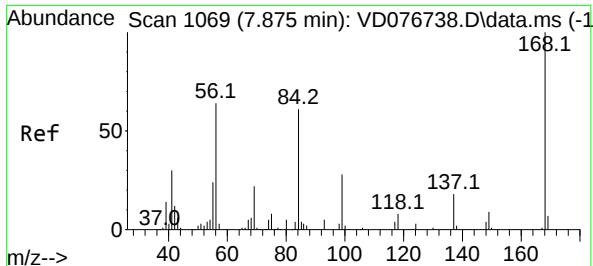

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1069
Delta R.T. 0.000 min
Lab File: VD076856.D
Acq: 28 Jul 2023 15:53




Instrument :
MSVOA_D
ClientSampleId :
B-P16A


Tgt Ion:168 Resp: 185788
Ion Ratio Lower Upper
168 100
99 51.8 36.7 55.1

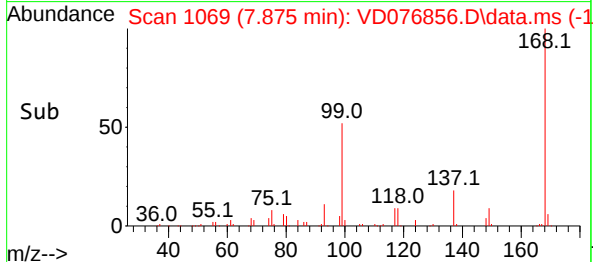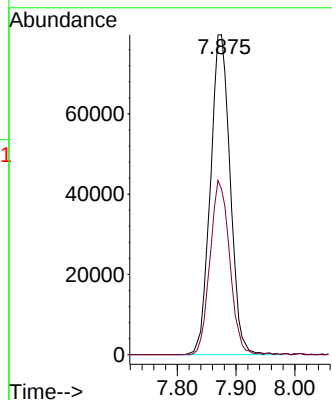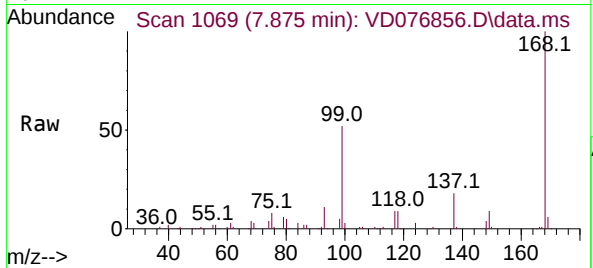

#33
1,2-Dichloroethane-d4
Concen: 50.476 ug/l
RT: 8.228 min Scan# 1129
Delta R.T. -0.000 min
Lab File: VD076856.D
Acq: 28 Jul 2023 15:53

Tgt Ion: 65 Resp: 93406
Ion Ratio Lower Upper
65 100
67 55.5 0.0 115.0

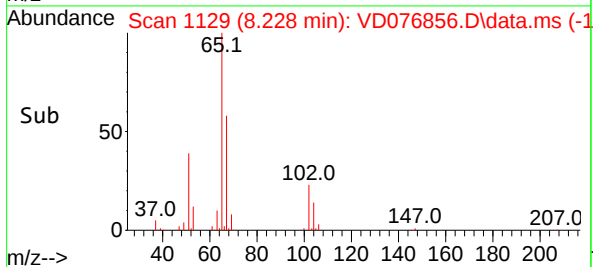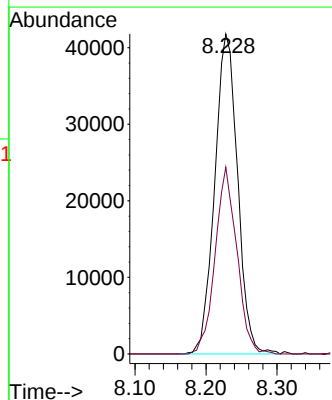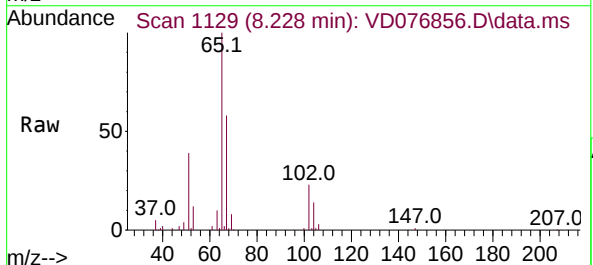

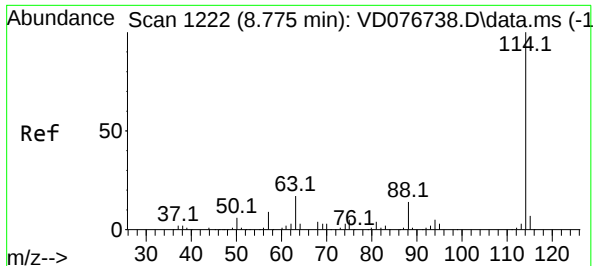

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.775 min Scan# 1

Delta R.T. -0.000 min

Lab File: VD076856.D

Acq: 28 Jul 2023 15:53

Instrument :

MSVOA_D

ClientSampleId :

B-P16A





Tgt Ion:114 Resp: 349366

Ion Ratio Lower Upper

114 100

63 18.1 0.0 33.4

88 13.5 0.0 26.2

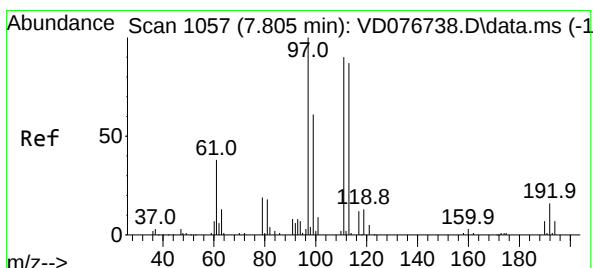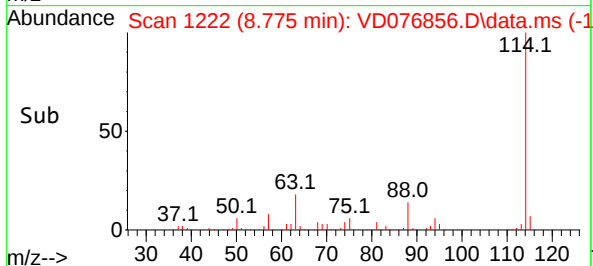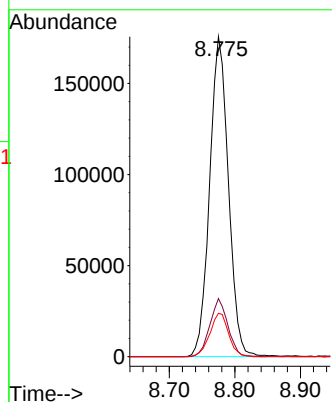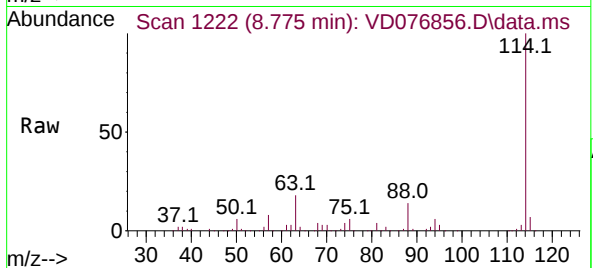

#35

Dibromofluoromethane

Concen: 50.093 ug/l

RT: 7.804 min Scan# 1057

Delta R.T. -0.001 min

Lab File: VD076856.D

Acq: 28 Jul 2023 15:53




Tgt Ion:113 Resp: 109977


Ion Ratio Lower Upper

113 100

111 103.8 84.7 127.1

192 17.6 16.8 25.2


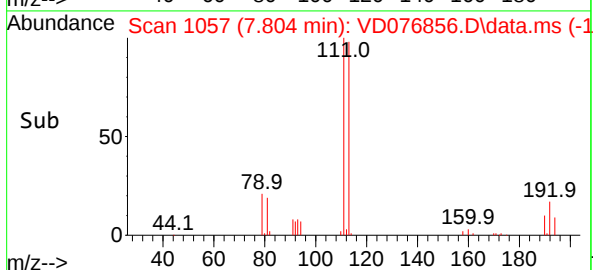
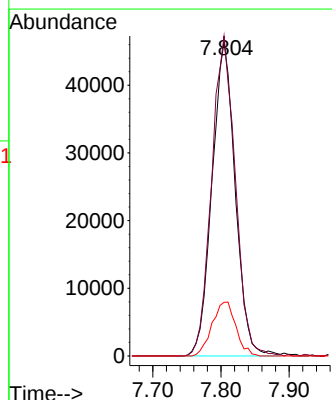
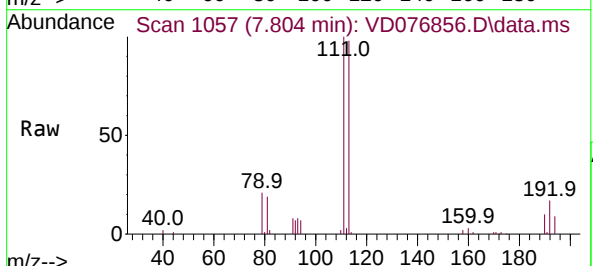


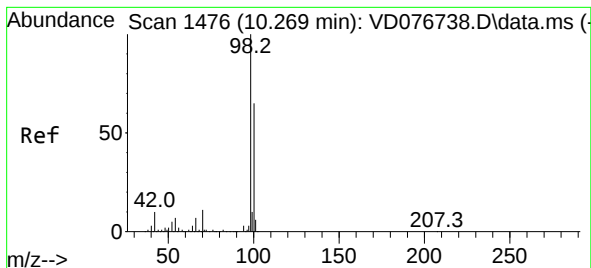

#50
Toluene-d8
Concen: 53.975 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. -0.000 min
Lab File: VD076856.D
Acq: 28 Jul 2023 15:53




Instrument :
MSVOA_D
ClientSampleId :
B-P16A


Tgt Ion: 98 Resp: 423916
Ion Ratio Lower Upper
98 100
100 66.0 50.3 75.5

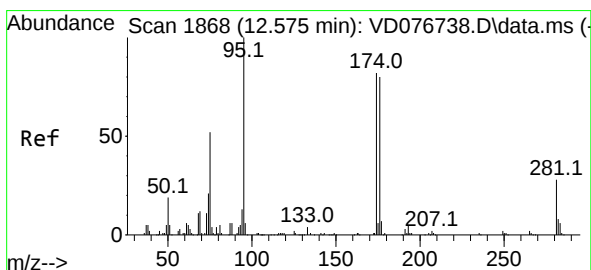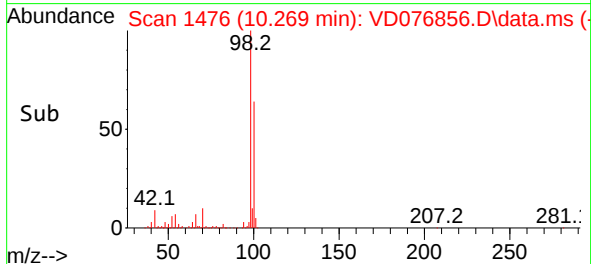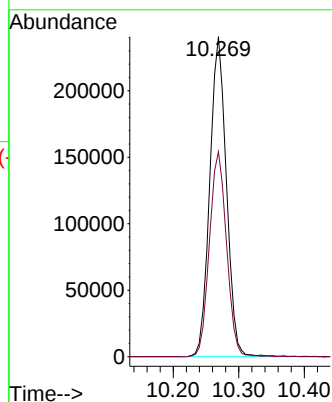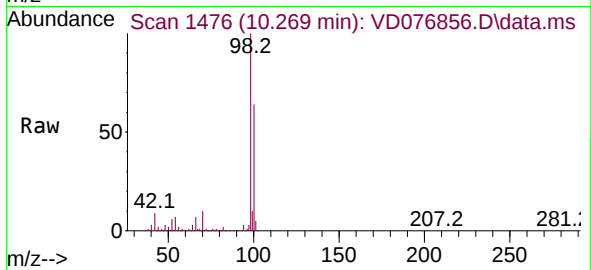

#62
4-Bromofluorobenzene
Concen: 47.055 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD076856.D
Acq: 28 Jul 2023 15:53

Tgt Ion: 95 Resp: 119554
Ion Ratio Lower Upper
95 100
174 86.7 0.0 201.8
176 85.1 0.0 191.8


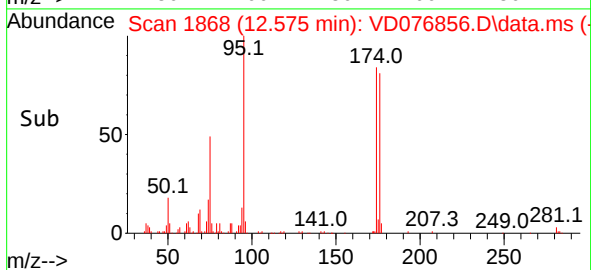
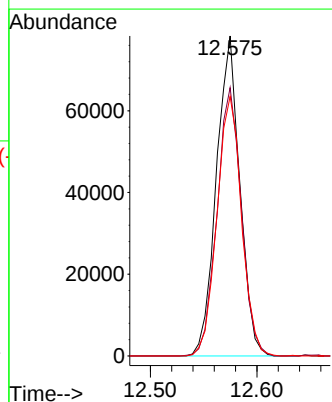
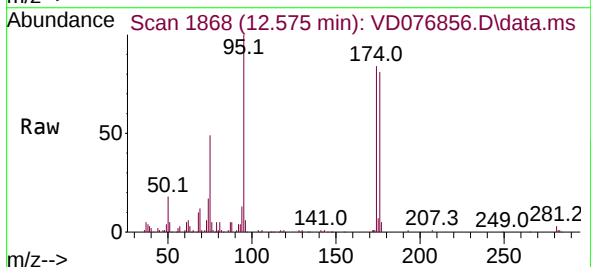


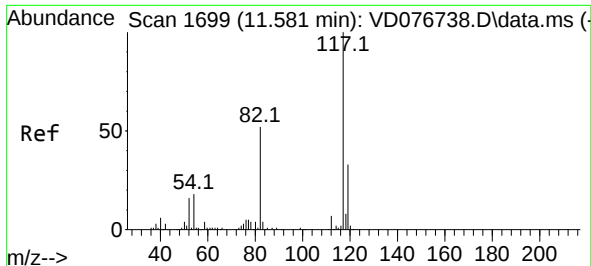

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 1
Delta R.T. -0.000 min
Lab File: VD076856.D
Acq: 28 Jul 2023 15:53

Instrument :
MSVOA_D
ClientSampleId :
B-P16A

Tgt Ion:117 Resp: 321181
Ion Ratio Lower Upper
117 100
82 51.0 38.3 57.5
119 29.9 25.0 37.4

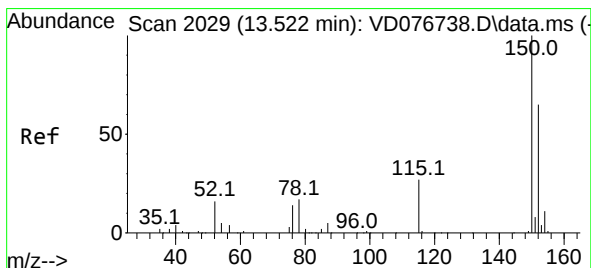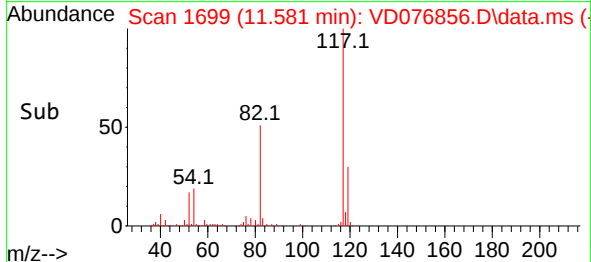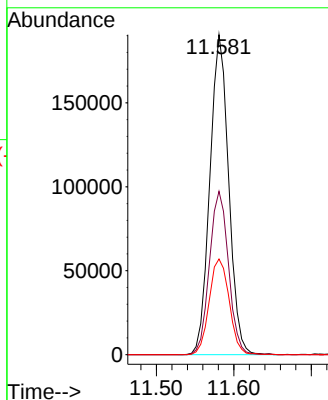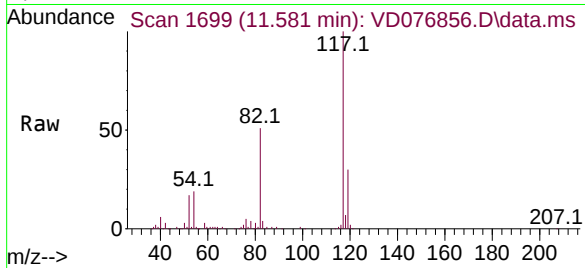

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. -0.006 min
Lab File: VD076856.D
Acq: 28 Jul 2023 15:53

Tgt Ion:152 Resp: 137900
Ion Ratio Lower Upper
152 100
115 57.4 27.1 81.3
150 160.3 0.0 353.6

