
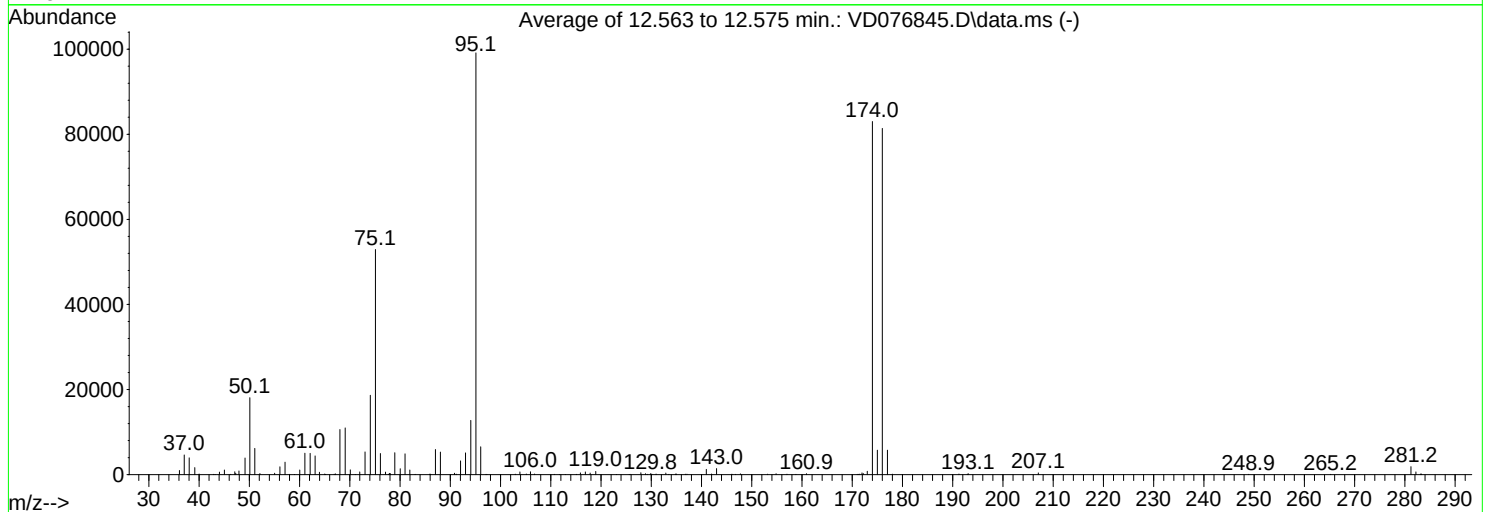


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD072823\
Data File : VD076845.D
Acq On : 28 Jul 2023 09:57
Operator : KP/SY
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D071423S.M
Title : SW846 8260
Last Update : Mon Jul 17 08:07:52 2023

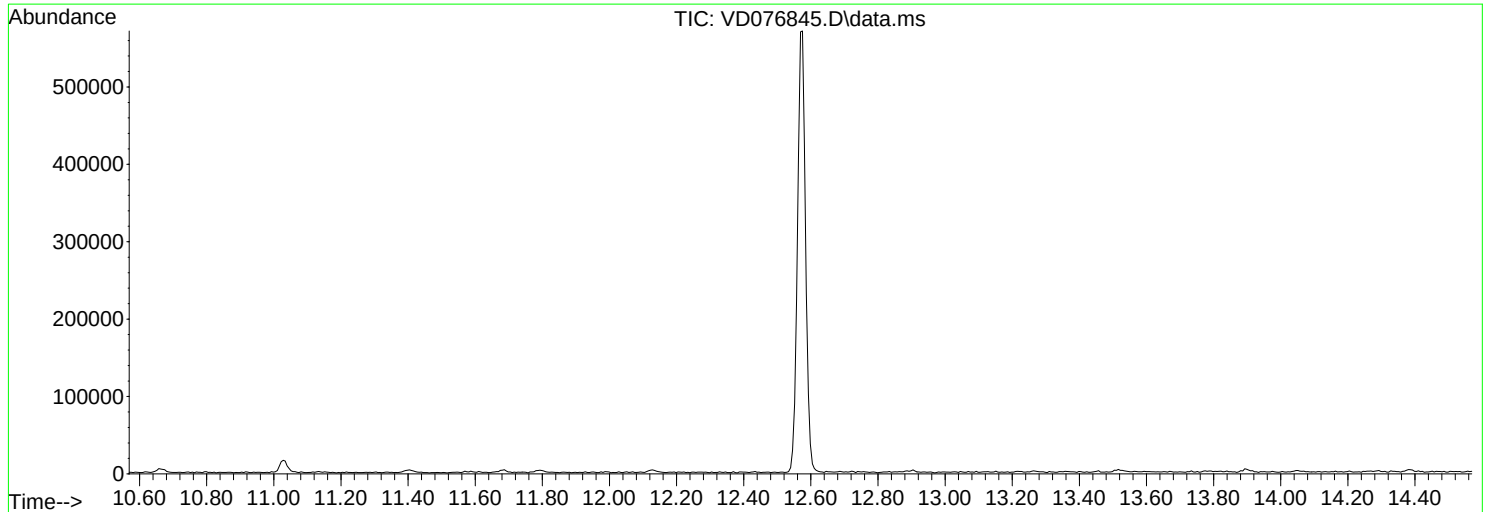

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	18099	PASS
75	95	30	60	53.4	52928	PASS
95	95	100	100	100.0	99141	PASS
96	95	5	9	6.6	6540	PASS
173	174	0.00	2	0.9	787	PASS
174	95	50	100	83.7	82997	PASS
175	174	5	9	6.9	5764	PASS
176	174	95	101	98.1	81389	PASS
177	176	5	9	7.1	5750	PASS