


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD073019\
Data File : VD063230.D
Acq On : 30 Jul 2019 9:34
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D072919S.M
Title : SW846 8260
Last Update : Tue Jul 30 03:04:50 2019

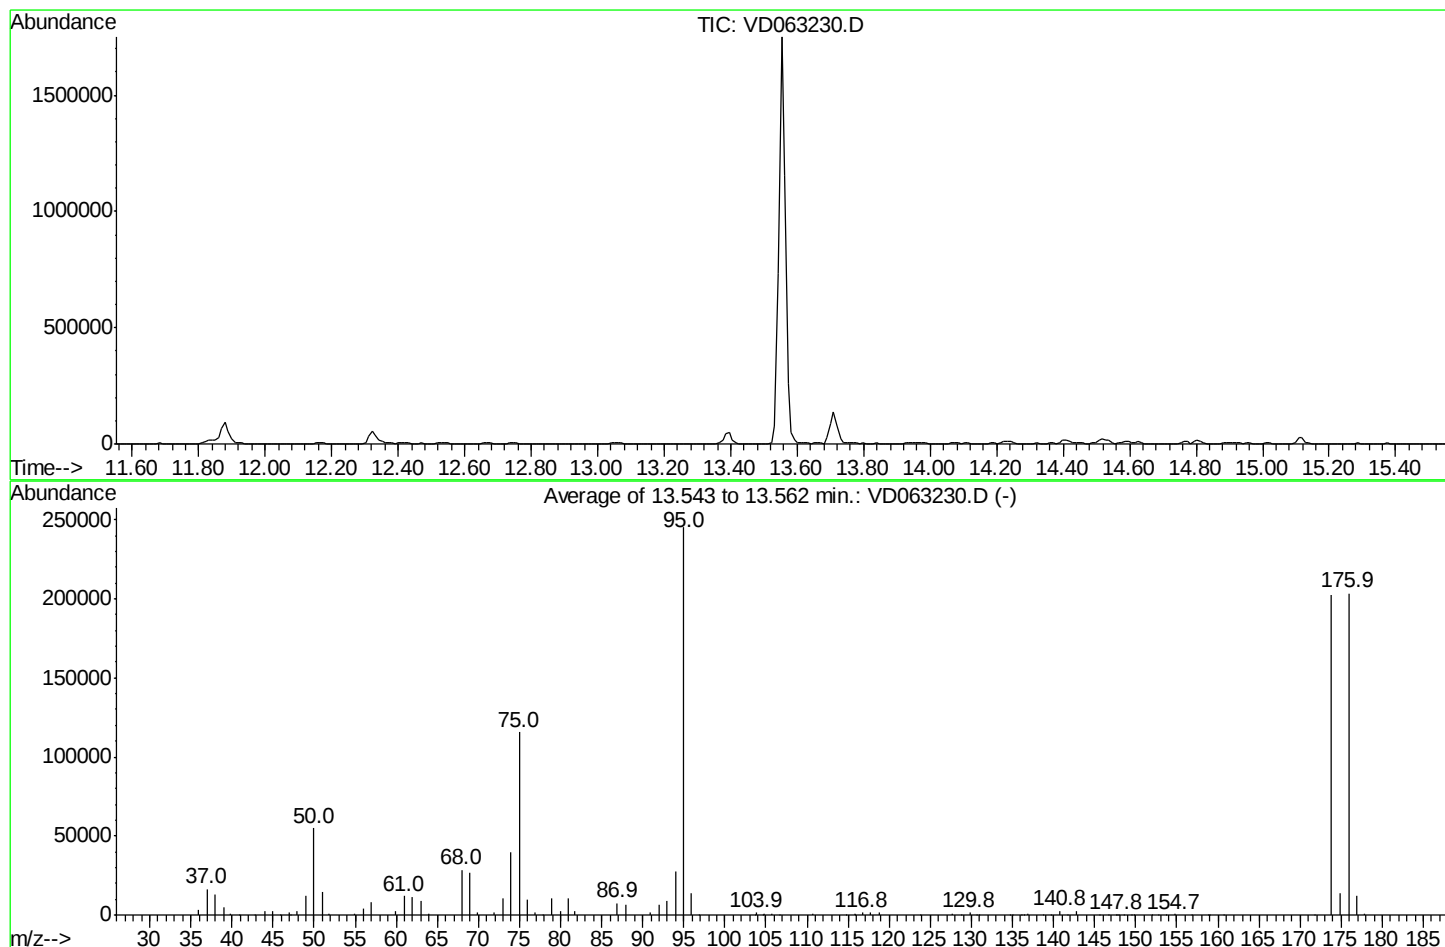

AutoFind: Scans 1231, 1232, 1233; Background Corrected with Scan 1227

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	55037	PASS
75	95	30	60	47.2	115677	PASS
95	95	100	100	100.0	245184	PASS
96	95	5	9	5.7	14084	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	82.5	202282	PASS
175	174	5	9	6.9	13884	PASS
176	174	95	101	100.5	203365	PASS
177	176	5	9	5.9	12042	PASS