


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD073019\
Data File : VD063254.D
Acq On : 30 Jul 2019 21:52
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D072919S.M
Title : SW846 8260
Last Update : Tue Jul 30 03:04:50 2019

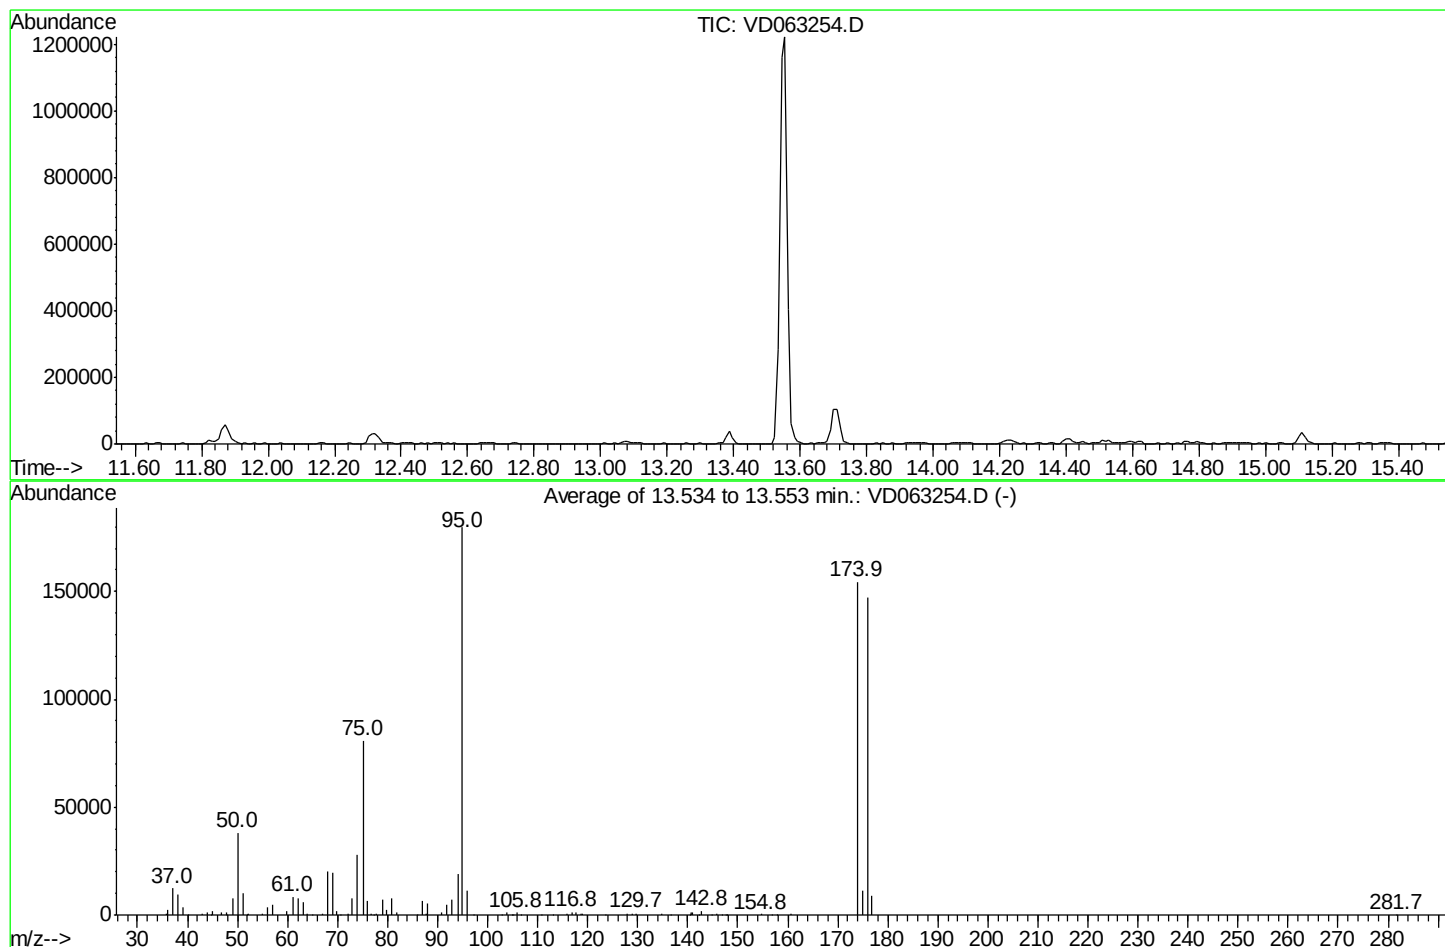

AutoFind: Scans 1230, 1231, 1232; Background Corrected with Scan 1226

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	38277	PASS
75	95	30	60	45.1	81018	PASS
95	95	100	100	100.0	179730	PASS
96	95	5	9	6.3	11367	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	86.0	154544	PASS
175	174	5	9	7.2	11181	PASS
176	174	95	101	95.2	147088	PASS
177	176	5	9	6.3	9217	PASS