

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD073020\
 Data File : VD066105.D
 Acq On : 30 Jul 2020 12:23
 Operator : VA/SY
 Sample : L3489-10
 Misc : 5.02G/5.00ml/MSVOA D/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 CS-10

Quant Time: Jul 31 02:53:42 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D072120S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 21 12:34:13 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.98	168	226609	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.86	114	361566	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	396171	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	215717	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.33	65	103981	56.39	ug/l	0.00
Spiked Amount 50.000			Recovery	=	112.78%	
35) Dibromofluoromethane	7.91	113	109765	50.05	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.10%	
50) Toluene-d8	10.34	98	437833	53.59	ug/l	0.00
Spiked Amount 50.000			Recovery	=	107.18%	
62) 4-Bromofluorobenzene	12.64	95	183476	64.77	ug/l	0.00
Spiked Amount 50.000			Recovery	=	129.54%	
Target Compounds						
7) Trichlorofluoromethane	3.29	101	3333	1.025	ug/l	97
8) Diethyl Ether	3.70	74	1788	1.990	ug/l	70
20) Methylene Chloride	4.96	84	19661	6.975	ug/l	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD073020\
Data File : VD066105.D
Acq On : 30 Jul 2020 12:23
Operator : VA/SY
Sample : L3489-10
Misc : 5.02G/5.00ml/MSVOA D/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
CS-10

Quant Time: Jul 31 02:53:42 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D072120S.M
Quant Title : SW846 8260
QLast Update : Tue Jul 21 12:34:13 2020
Response via : Initial Calibration

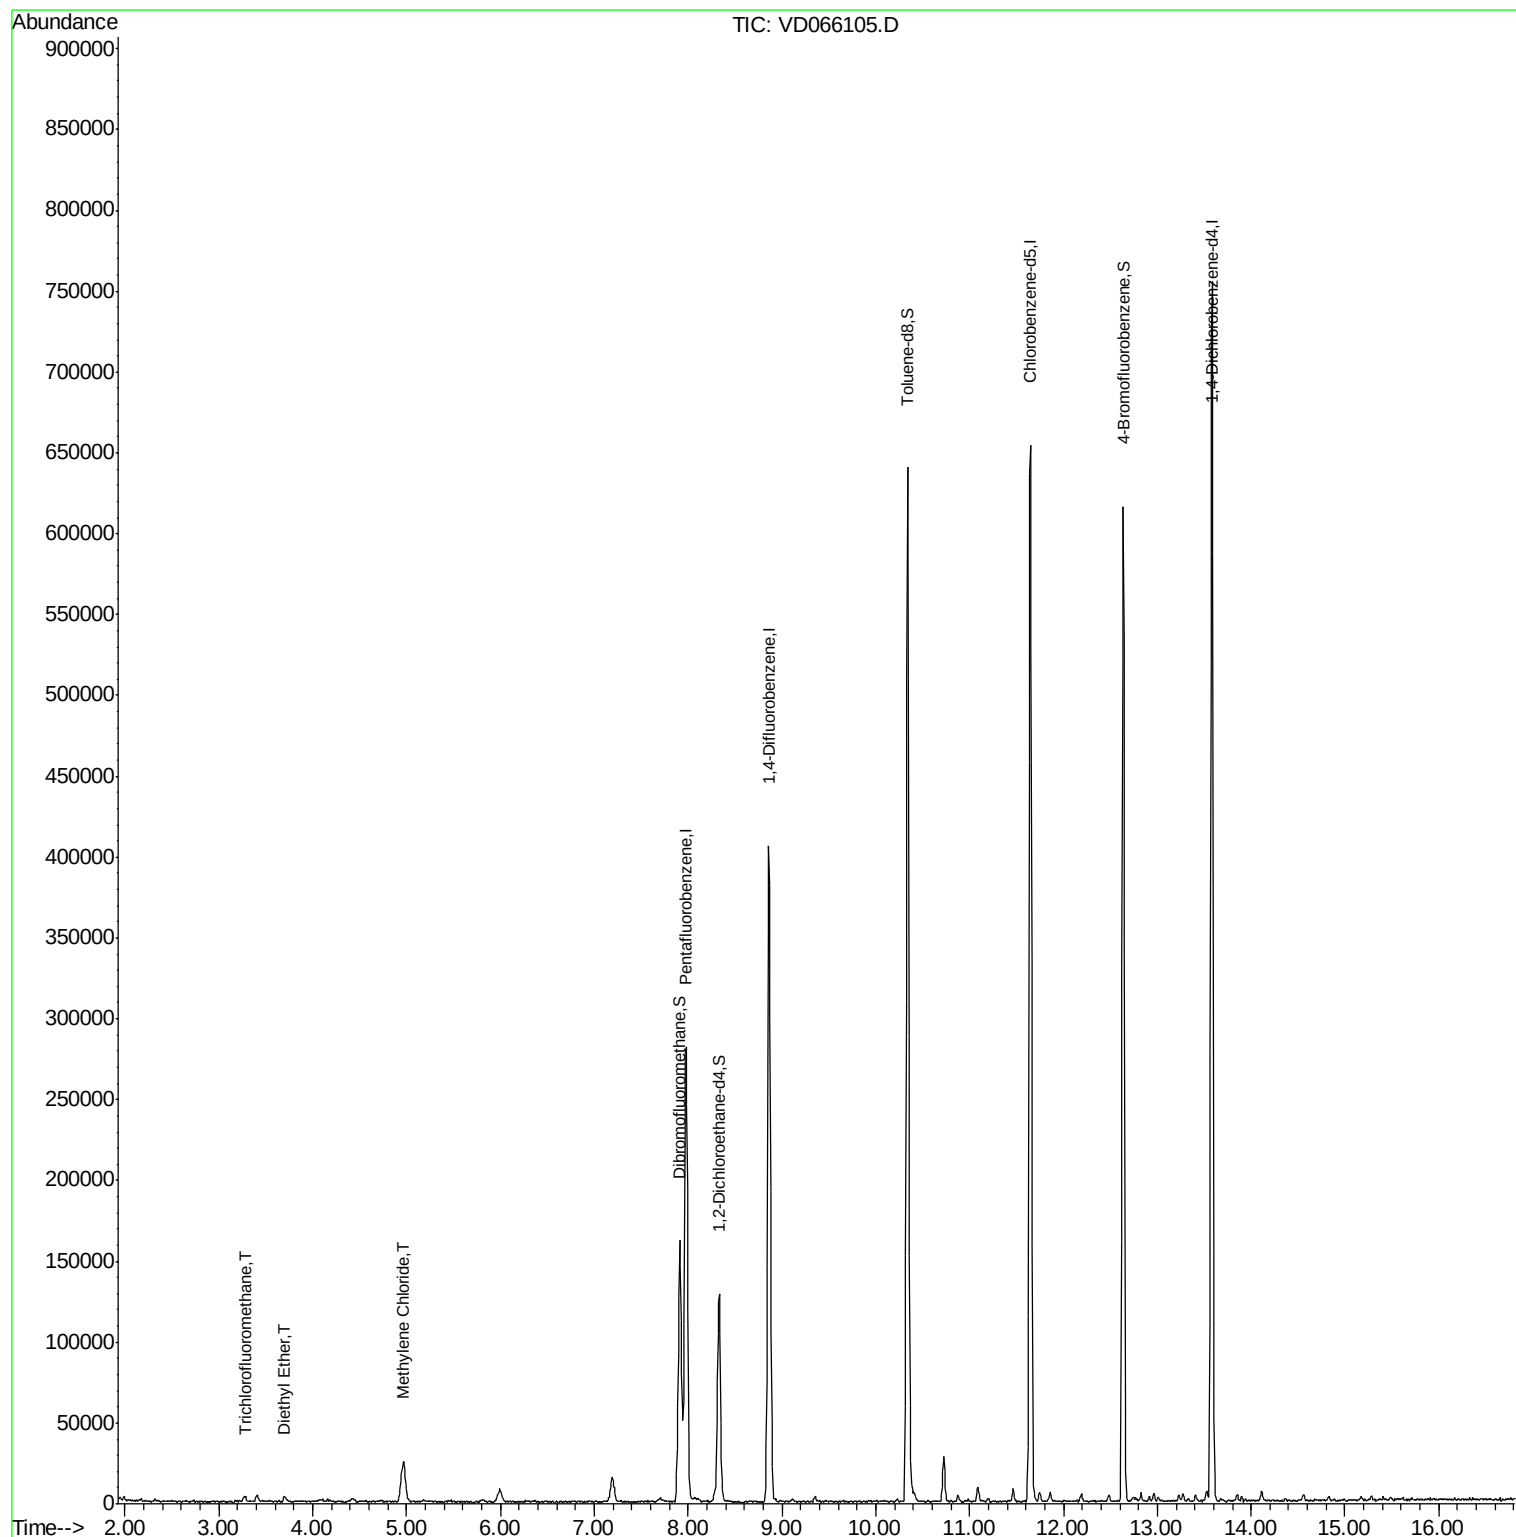

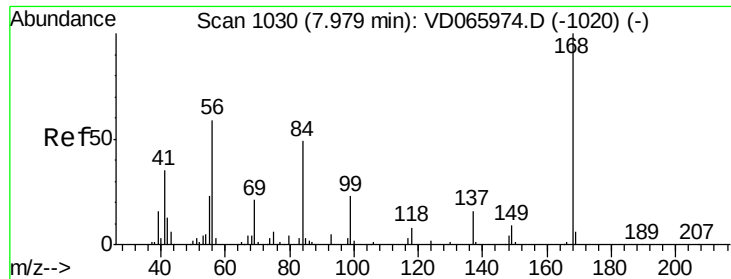

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.98 min Scan# 1030

Delta R.T. 0.00 min

Lab File: VD066105.D

Acq: 30 Jul 2020 12:23

Instrument :

MSVOA_D

ClientSampleId :


CS-10

Tot Ion:168 Resp: 226609

Ion Ratio Lower Upper




168 100

99 52.3 40.8 61.2

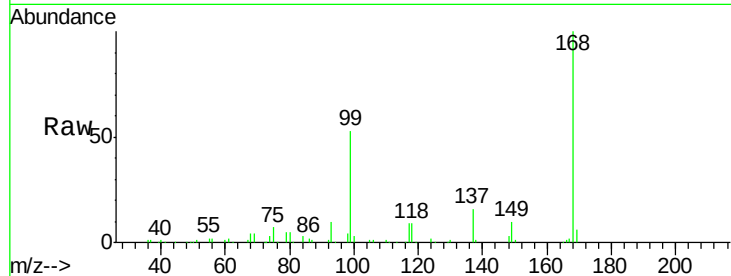

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

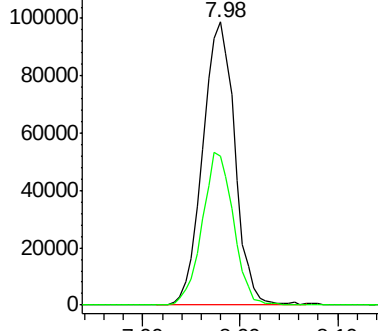

#7

Trichlorofluoromethane

Concen: 1.025 ug/l

RT: 3.29 min Scan# 232

Delta R.T. 0.01 min

Lab File: VD066105.D


Acq: 30 Jul 2020 12:23

Tgt Ion:101 Resp: 3333

Ion Ratio Lower Upper



101 100


103 62.8 52.1 78.1



Abundance Ion 100.90 (100.60 to 101.60): V

Ion 102.80 (102.50 to 103.50): V

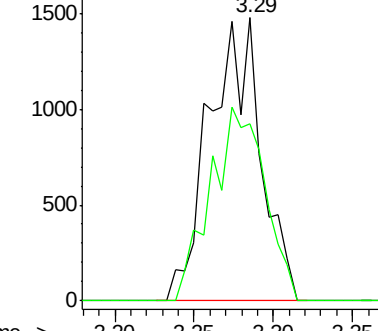

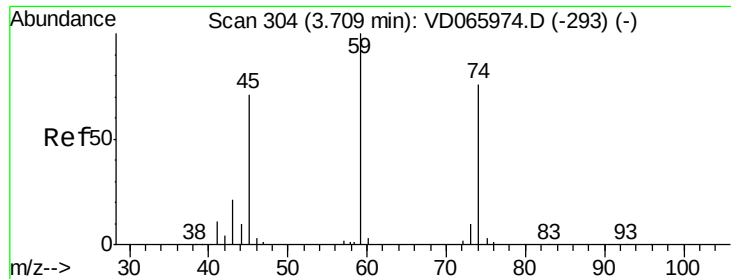

#8

Diethyl Ether

Concen: 1.990 ug/l

RT: 3.70 min Scan# 302

Delta R.T. -0.01 min

Lab File: VD066105.D

Acq: 30 Jul 2020 12:23

Instrument :

MSVOA_D

ClientSampleId :





CS-10

Tot Ion: 74 Resp: 1788

Ion Ratio Lower Upper

74 100

45 69.6 49.9 149.6

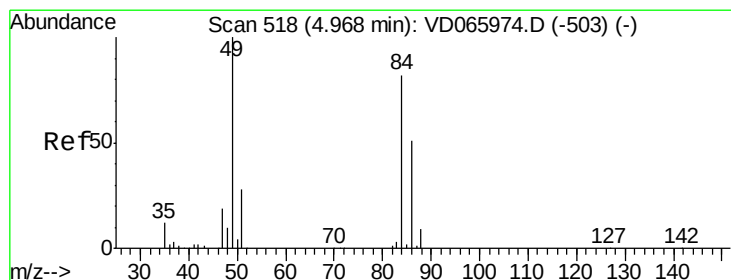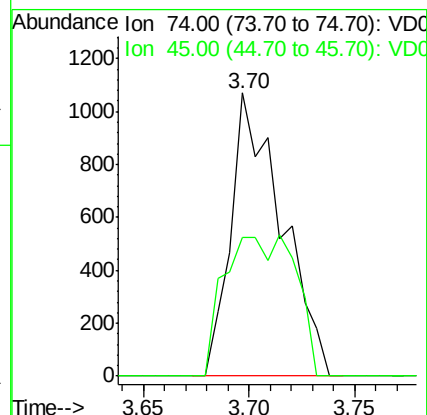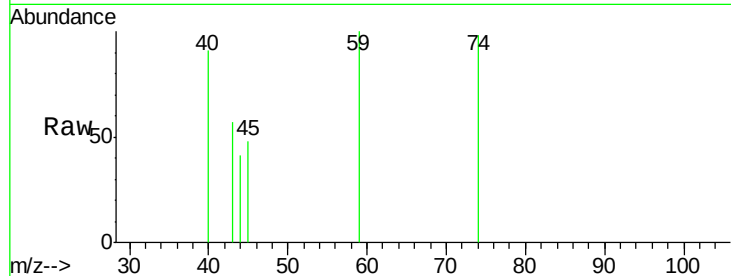

#20

Methylene Chloride

Concen: 6.975 ug/l

RT: 4.96 min Scan# 517

Delta R.T. -0.01 min

Lab File: VD066105.D

Acq: 30 Jul 2020 12:23

Tgt Ion: 84 Resp: 19661




Ion Ratio Lower Upper


84 100

49 109.7 97.7 146.5

51 30.8 27.4 41.2

86 54.6 49.4 74.2

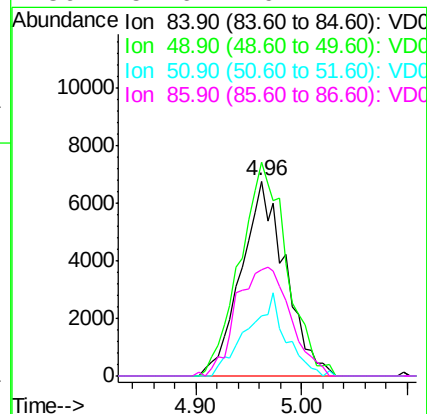

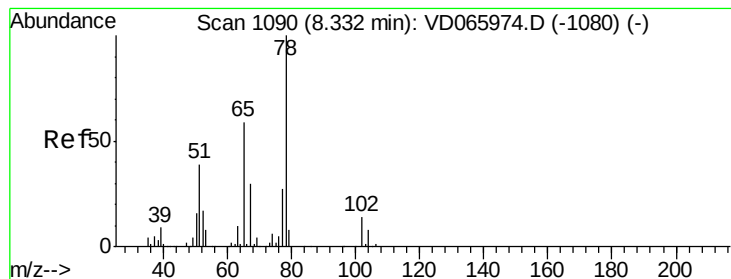

#33

1,2-Dichloroethane-d4

Concen: 56.392 ug/l

RT: 8.33 min Scan# 1089

Delta R.T. -0.01 min

Lab File: VD066105.D

Acq: 30 Jul 2020 12:23

Instrument :

MSVOA_D

ClientSampled :


CS-10

Tot Ion: 65 Resp: 103981

Ion Ratio Lower Upper

65 100

67 50.0 0.0 105.0



Abundance Ion 64.90 (64.60 to 65.60): VDC

Ion 66.90 (66.60 to 67.60): VDC

8.33

50000

40000



30000

20000

10000

0

Time--> 8.20 8.30 8.40



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.86 min Scan# 1180

Delta R.T. -0.01 min

Lab File: VD066105.D

Acq: 30 Jul 2020 12:23


Tgt Ion: 114 Resp: 361566

Ion Ratio Lower Upper

114 100

63 18.4 0.0 39.6

88 14.4 0.0 31.2



Abundance Ion 113.90 (113.60 to 114.60): VDC

Ion 63.00 (62.70 to 63.70): VDC

Ion 87.90 (87.60 to 88.60): VDC

8.86

250000

200000


150000


100000

50000

0

Time--> 8.80 8.90 9.00









#35
 Dibromofluoromethane
 Concen: 50.052 ug/l
 RT: 7.91 min Scan# 1019
 Delta R.T. -0.01 min
 Lab File: VD066105.D
 Acq: 30 Jul 2020 12:23

Instrument :
 MSVOA_D
 ClientSampleId :
 CS-10

Tot Ion	Ratio	Lower	Upper
113	100		
111	103.8	83.2	124.8
192	23.6	18.7	28.1

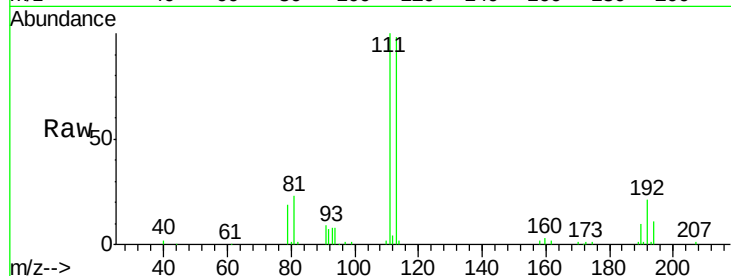


Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V


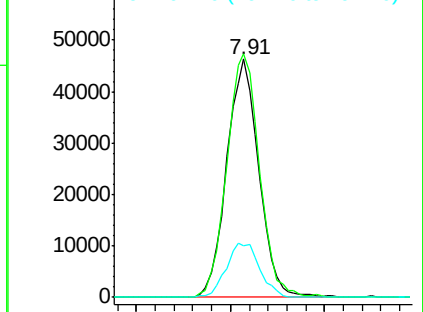



#50
 Toluene-d8
 Concen: 53.593 ug/l
 RT: 10.34 min Scan# 1431
 Delta R.T. -0.01 min
 Lab File: VD066105.D
 Acq: 30 Jul 2020 12:23

Tgt Ion	Ratio	Lower	Upper
98	100		
100	67.1	52.7	79.1



Abundance Ion 98.00 (97.70 to 98.70): V
 Ion 100.00 (99.70 to 100.70): V




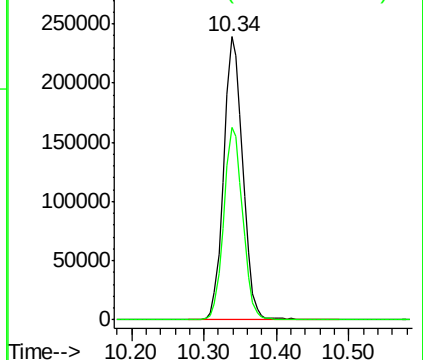


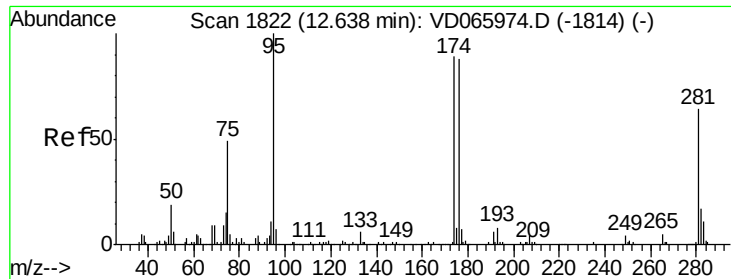

#62
4-Bromofluorobenzene
Concen: 64.771 ug/l
RT: 12.64 min Scan# 1822
Delta R.T. 0.00 min
Lab File: VD066105.D
Acq: 30 Jul 2020 12:23




Instrument :
MSVOA_D
ClientSampled :
CS-10


Tot Ion: 95 Resp: 183476
Ion Ratio Lower Upper
95 100
174 94.0 0.0 178.8
176 90.1 0.0 172.6

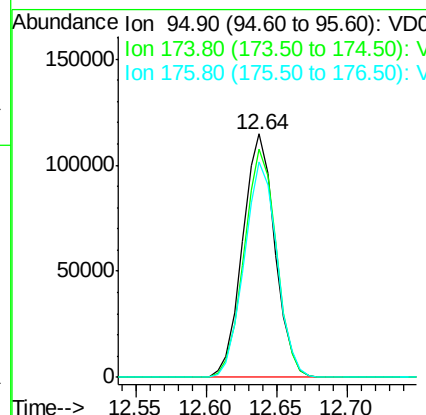

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.65 min Scan# 1654
Delta R.T. 0.00 min
Lab File: VD066105.D
Acq: 30 Jul 2020 12:23

Tgt Ion: 117 Resp: 396171
Ion Ratio Lower Upper
117 100
82 48.7 41.1 61.7
119 29.8 25.9 38.9

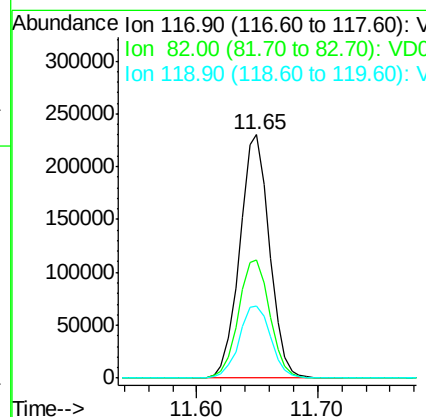

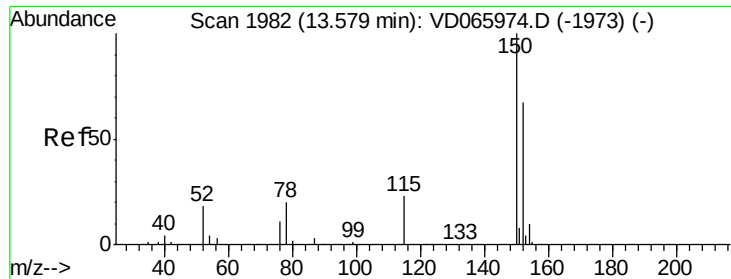

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.58 min Scan# 1983

Delta R.T. 0.01 min

Lab File: VD066105.D

Acq: 30 Jul 2020 12:23

Instrument :

MSVOA_D

ClientSampleId :

CS-10


Tot Ion:152 Resp: 215717

Ion Ratio Lower Upper

152 100

115 55.7 27.9 83.7

150 159.0 0.0 348.2



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

