
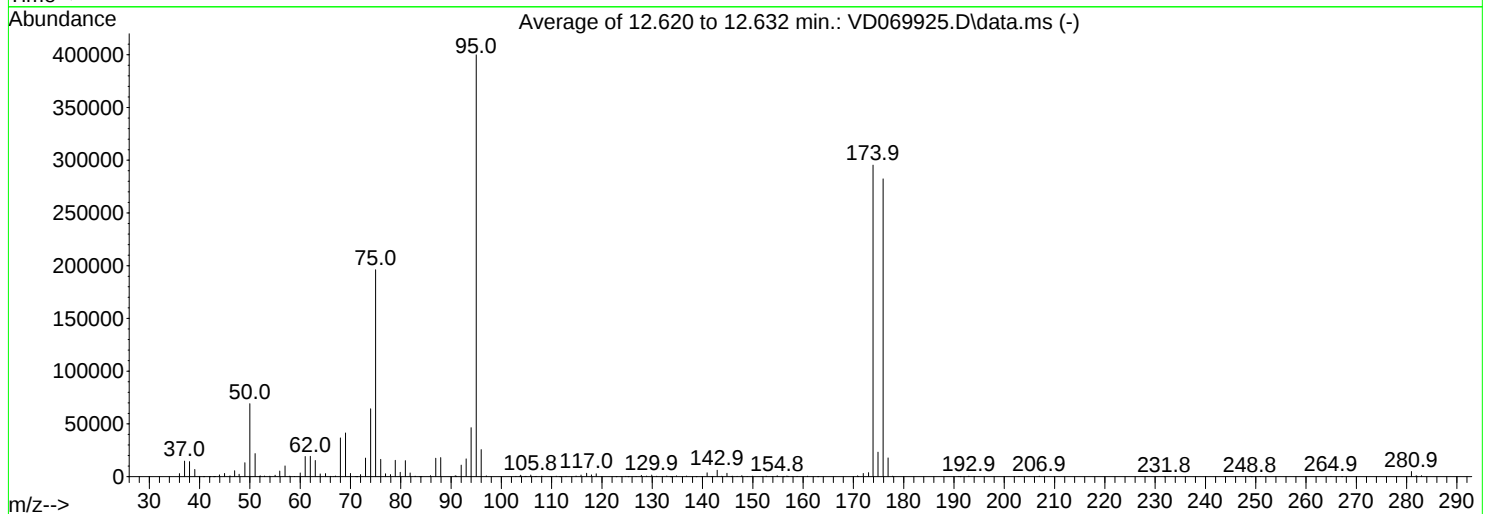


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD073021\
Data File : VD069925.D
Acq On : 30 Jul 2021 08:28
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D072221S.M
Title : SW846 8260
Last Update : Fri Jul 23 04:51:13 2021

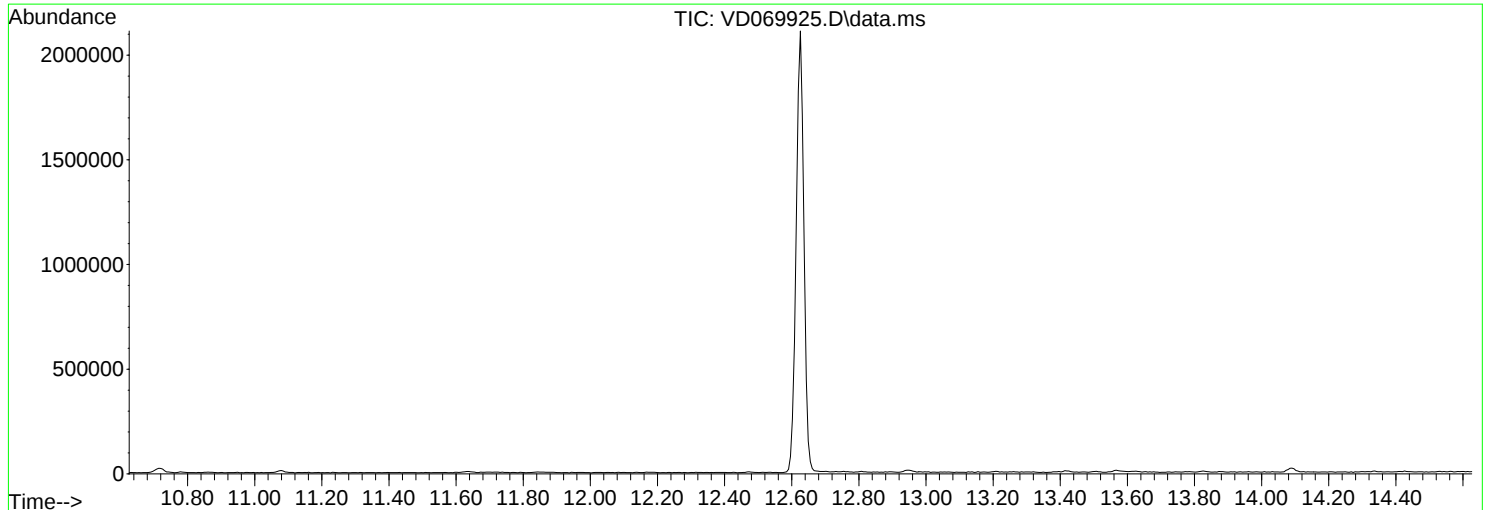

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.3	69136	PASS
75	95	30	60	49.1	196181	PASS
95	95	100	100	100.0	399915	PASS
96	95	5	9	6.4	25581	PASS
173	174	0.00	2	1.3	3799	PASS
174	95	50	100	73.9	295360	PASS
175	174	5	9	7.8	23155	PASS
176	174	95	101	95.6	282325	PASS
177	176	5	9	6.3	17693	PASS