

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD073118\
 Data File : VD059667.D
 Acq On : 31 Jul 2018 21:43
 Operator : VA/AP
 Sample : J4228-04RE
 Misc : 5.06/5ml/MSVOA D/SOIL
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 G.L.B(8.0)-1ARE

Quant Time: Aug 01 06:43:47 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D072418S.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 25 07:10:33 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-5.61
34) 1,4-Difluorobenzene	6.68	114	214	50.00	ug/l	0.02
63) Chlorobenzene-d5	10.68	117	247	50.00	ug/l	0.02
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-12.90

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	0.00	65	0	0.00	ug/l	
Spiked Amount						
			Recovery	=	0.00%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount						
			Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0	0.00	ug/l	
Spiked Amount						
			Recovery	=	0.00%	
62) 4-Bromofluorobenzene	0.00	95	0	0.00	ug/l	
Spiked Amount						
			Recovery	=	0.00%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD073118\
Data File : VD059667.D
Acq On : 31 Jul 2018 21:43
Operator : VA/AP
Sample : J4228-04RE
Misc : 5.06/5ml/MSVOA D/SOIL
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
G.L.B(8.0)-1ARE

Quant Time: Aug 01 06:43:47 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D072418S.M
Quant Title : SW846 8260
QLast Update : Wed Jul 25 07:10:33 2018
Response via : Initial Calibration

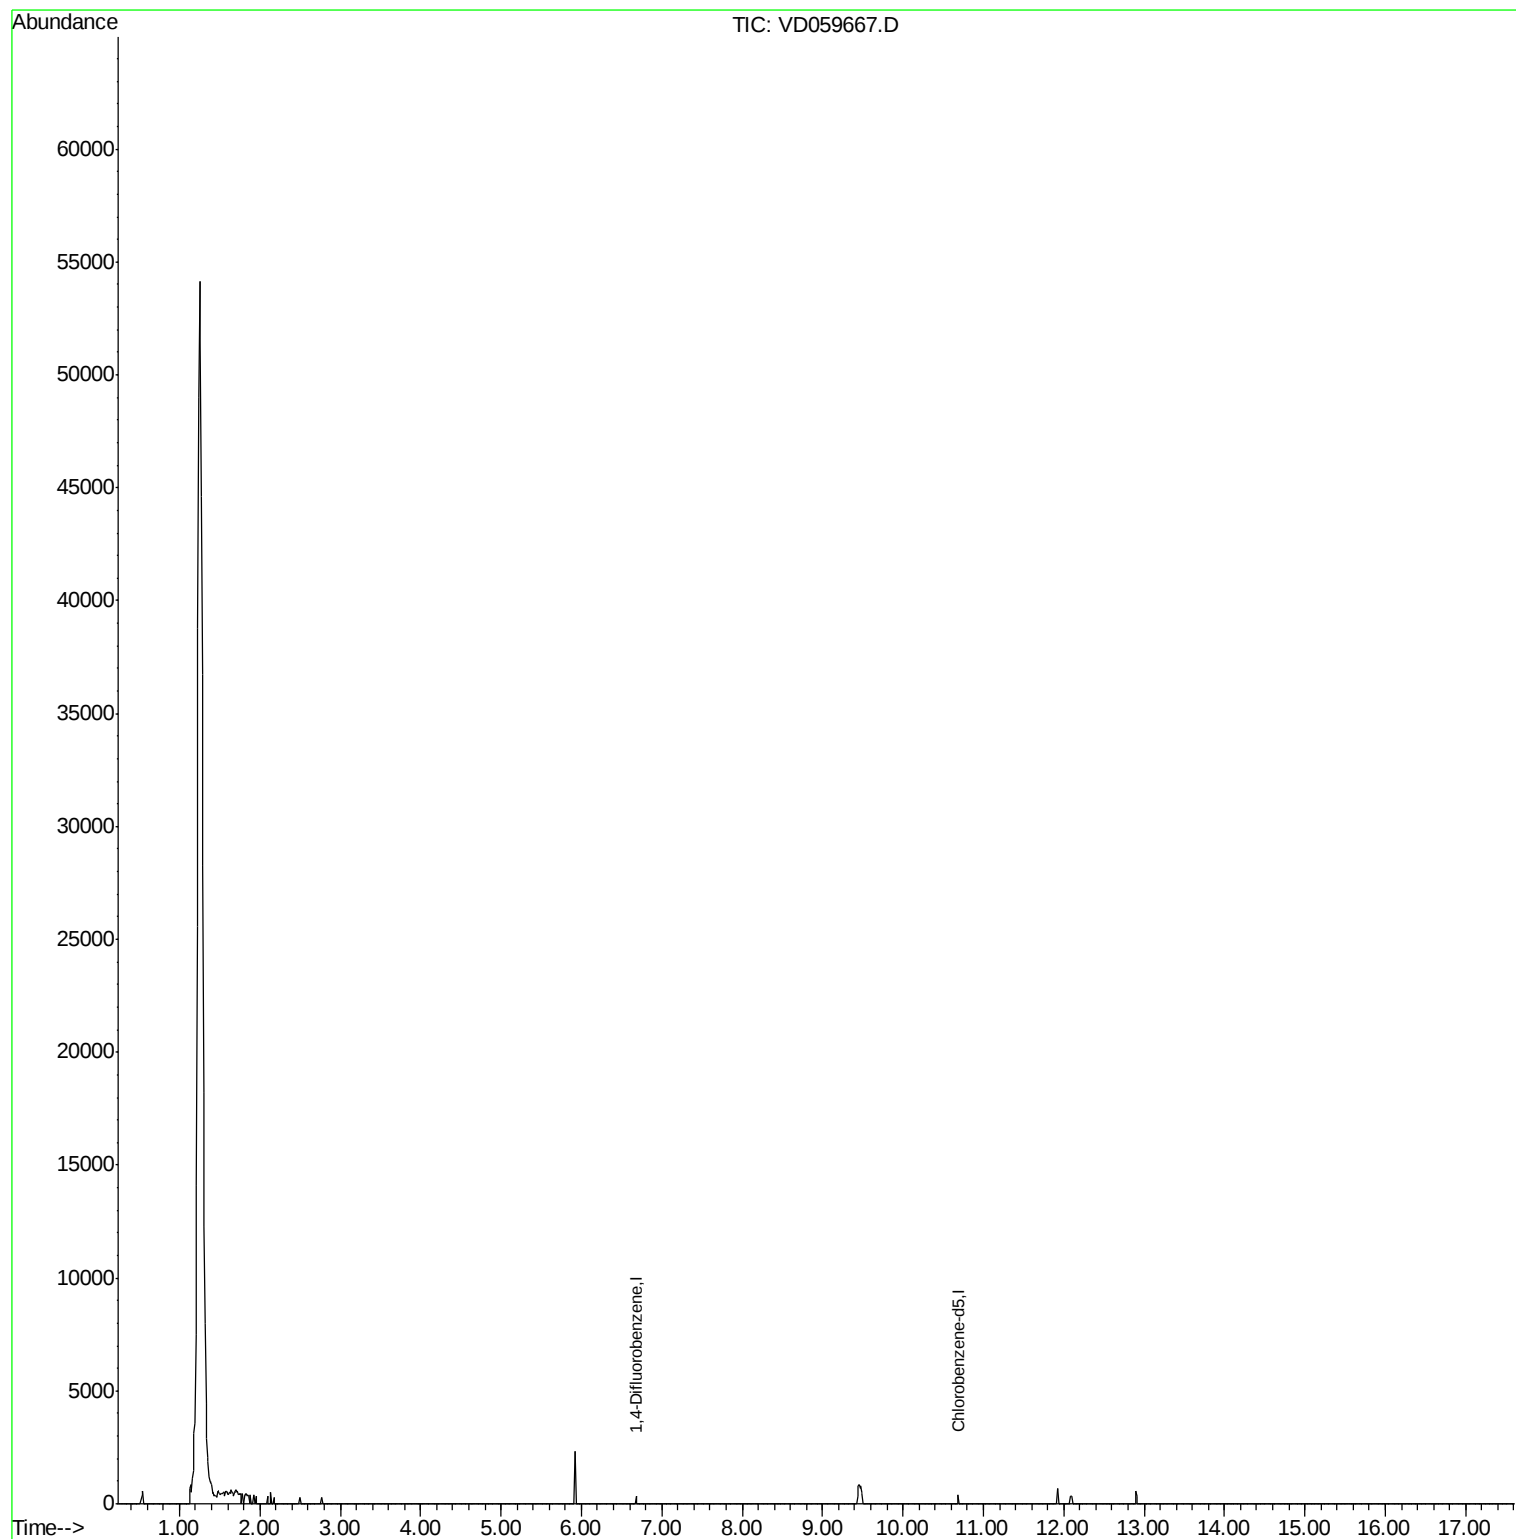

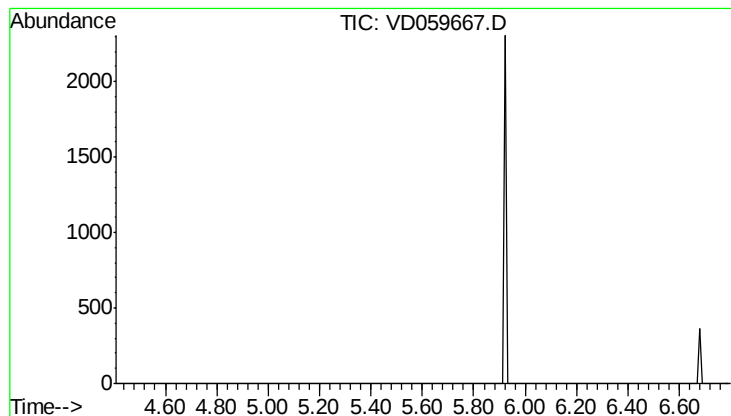

#1

Pentafluorobenzene

Concen: 0.000 ug/l

Expected RT: 5.61 min

Lab File: VD059667.D

Acq: 31 Jul 2018 21:43

Tot Ion: 168

Sig Exp Ratio

168 100



99 59.1

Instrument :

MSVOA_D

ClientSampleId :

G.L.B(8.0)-1ARE

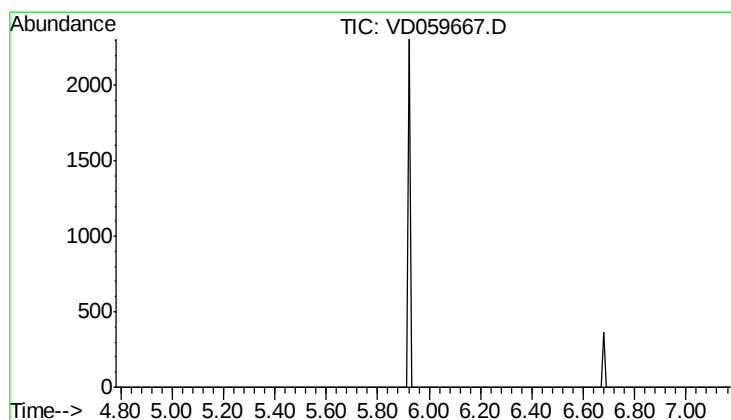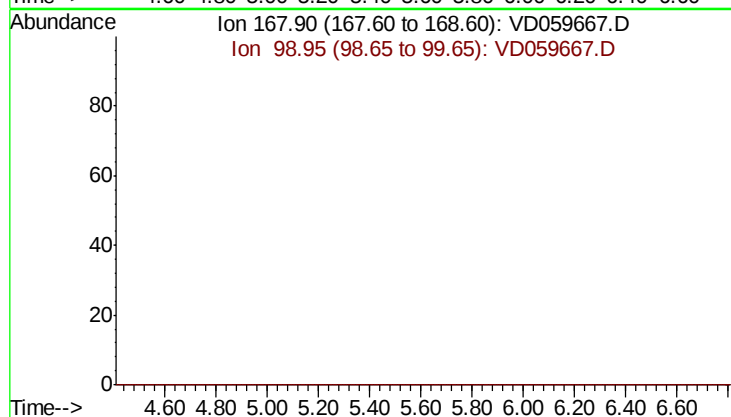

#33

1,2-Dichloroethane-d4

Concen: N.D. ug/l

Expected RT: 5.98 min

Lab File: VD059667.D


Acq: 31 Jul 2018 21:43

Tgt Ion: 65

Sig Exp Ratio

65 100

67 43.2




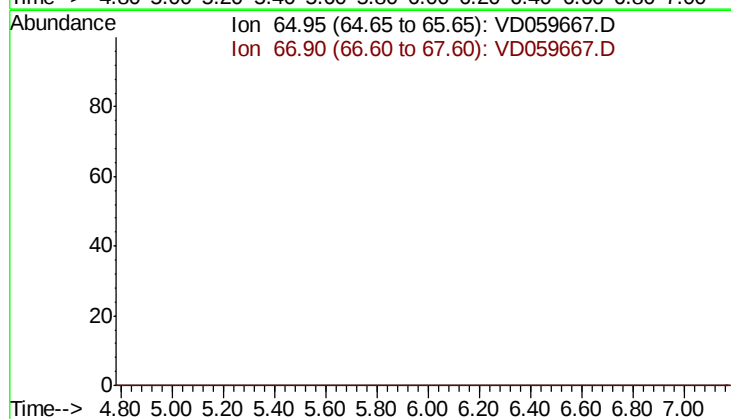




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.68 min Scan# 656
 Delta R.T. 0.02 min
 Lab File: VD059667.D
 Acq: 31 Jul 2018 21:43

Instrument :
 MSVOA_D
 ClientSampleId :
 G.L.B(8.0)-1ARE


Tot Ion	Ion	Ratio	Lower	Upper
114	100			
63	0.0	0.0	43.8	
88	0.0	0.0	39.0	

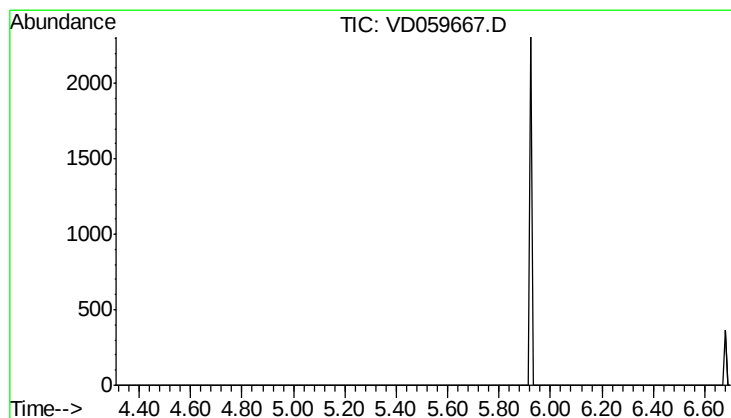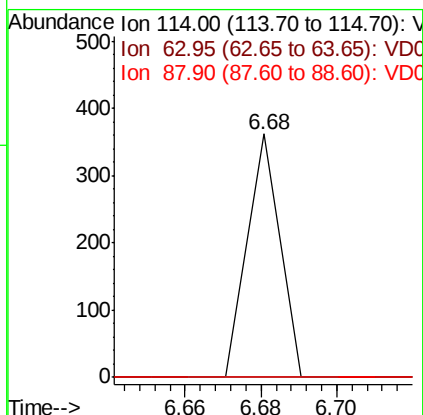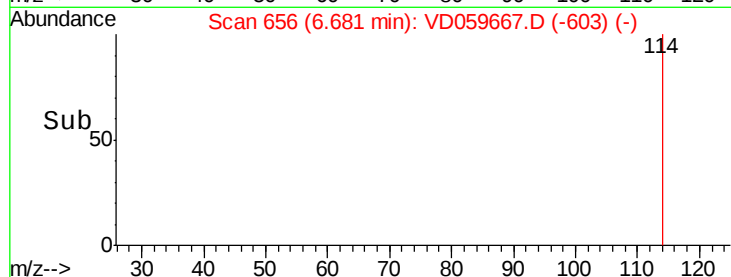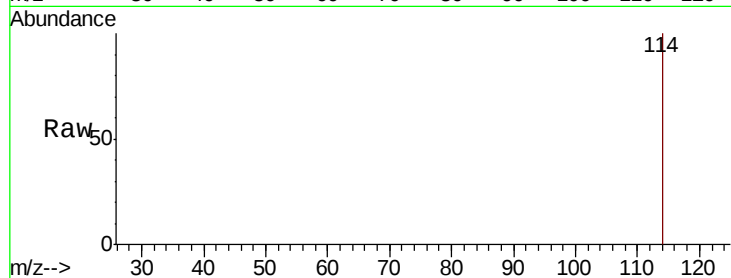


#35
 Dibromofluoromethane
 Concen: 50.000 ug/l
 Expected RT: 5.51 min

Lab File: VD059667.D
 Acq: 31 Jul 2018 21:43

Tgt Ion	Sig	Exp Ratio
113	100	
111	100.6	
192	18.1	

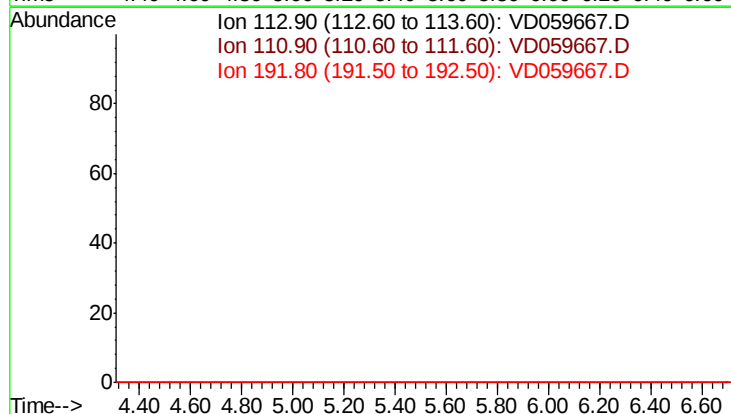


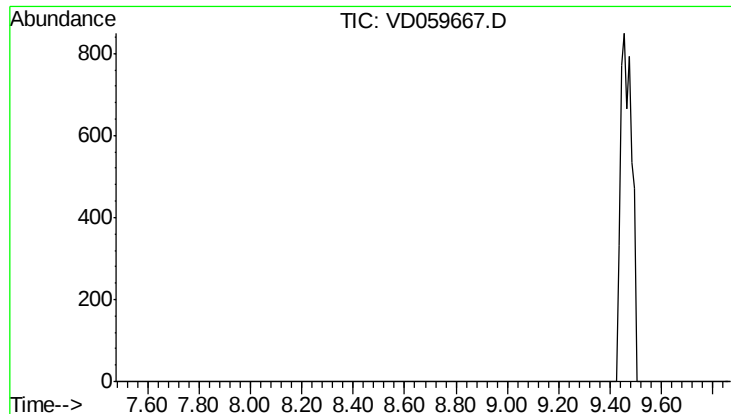


#50
Toluene-d8
Concen: N.D. ug/l
Expected RT: 8.68 min

Lab File: VD059667.D
Acq: 31 Jul 2018 21:43

Instrument :
MSVOA_D
ClientSampleId :
G.L.B(8.0)-1ARE


Tot Ion	98
Sig	Exp Ratio
98	100
100	66.5

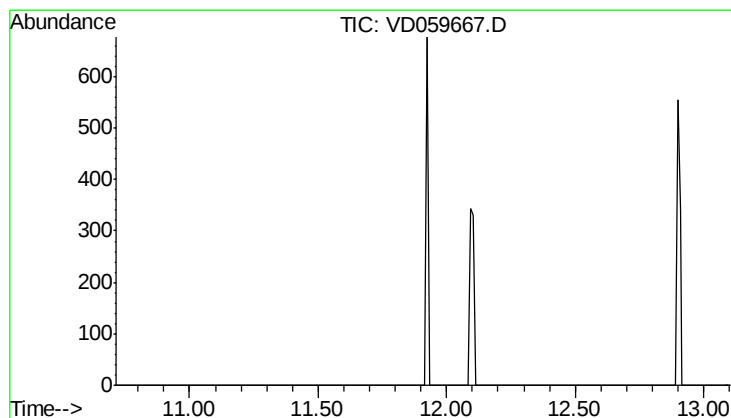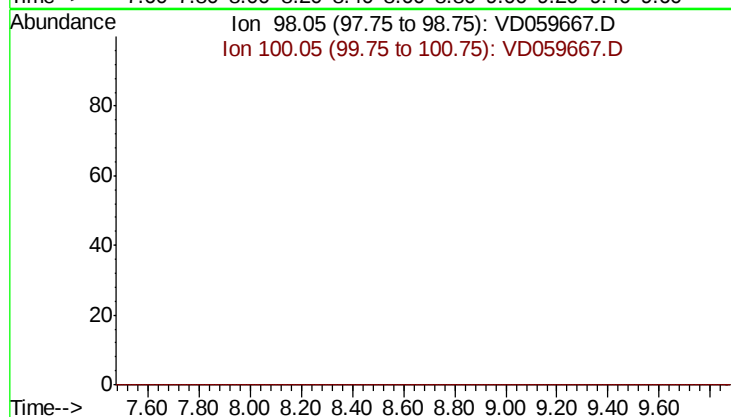


#62
4-Bromofluorobenzene
Concen: N.D. ug/l
Expected RT: 11.91 min

Lab File: VD059667.D
Acq: 31 Jul 2018 21:43

Tgt Ion	95
Sig	Exp Ratio
95	100
174	80.3
176	76.4




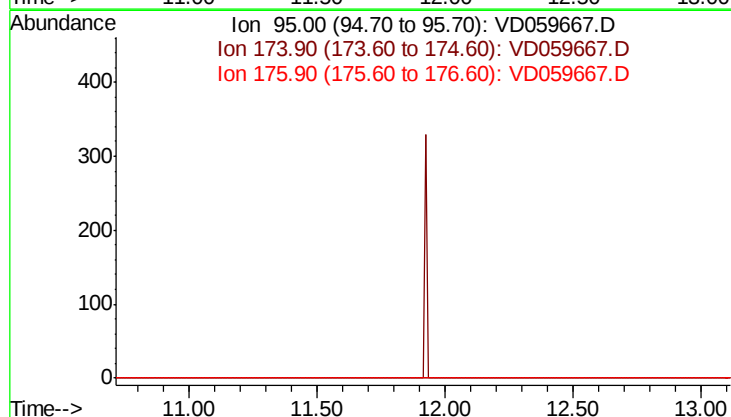


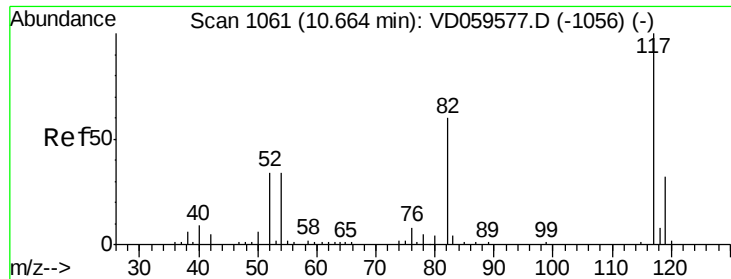

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.68 min Scan# 1063
Delta R.T. 0.02 min
Lab File: VD059667.D
Acq: 31 Jul 2018 21:43

Instrument :
MSVOA_D
ClientSampleId :
G.L.B(8.0)-1ARE

Tot Ion:117 Resp: 247
Ion Ratio Lower Upper
117 100
82 0.0 48.2 72.2#
119 0.0 25.4 38.2#

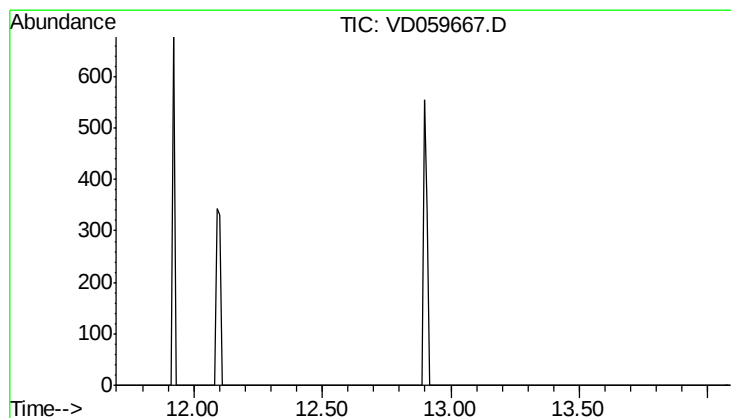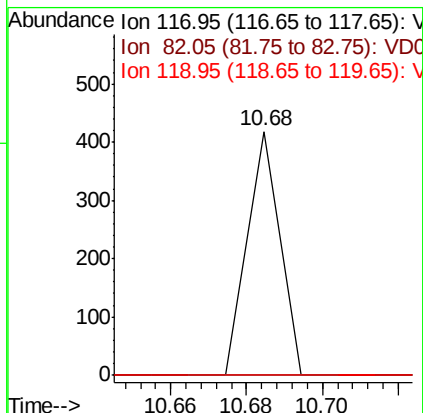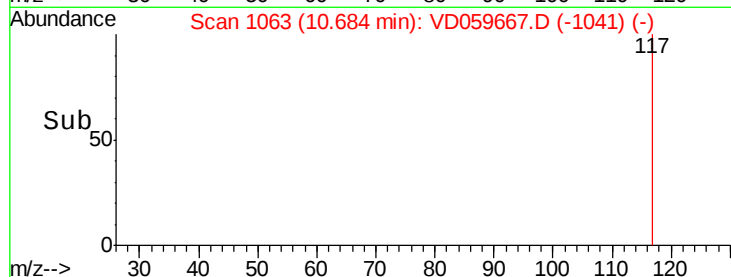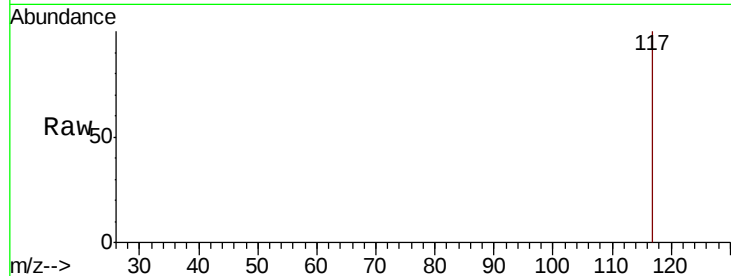

#72
1,4-Dichlorobenzene-d4
Concen: 0.000 ug/l
Expected RT: 12.90 min

Lab File: VD059667.D
Acq: 31 Jul 2018 21:43

Tgt Ion: 152
Sig Exp Ratio
152 100
115 59.1
150 157.2

