


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD073118\
 Data File : VD059647.D
 Acq On : 31 Jul 2018 9:52
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D072418S.M
 Title : SW846 8260
 Last Update : Wed Jul 25 07:10:33 2018

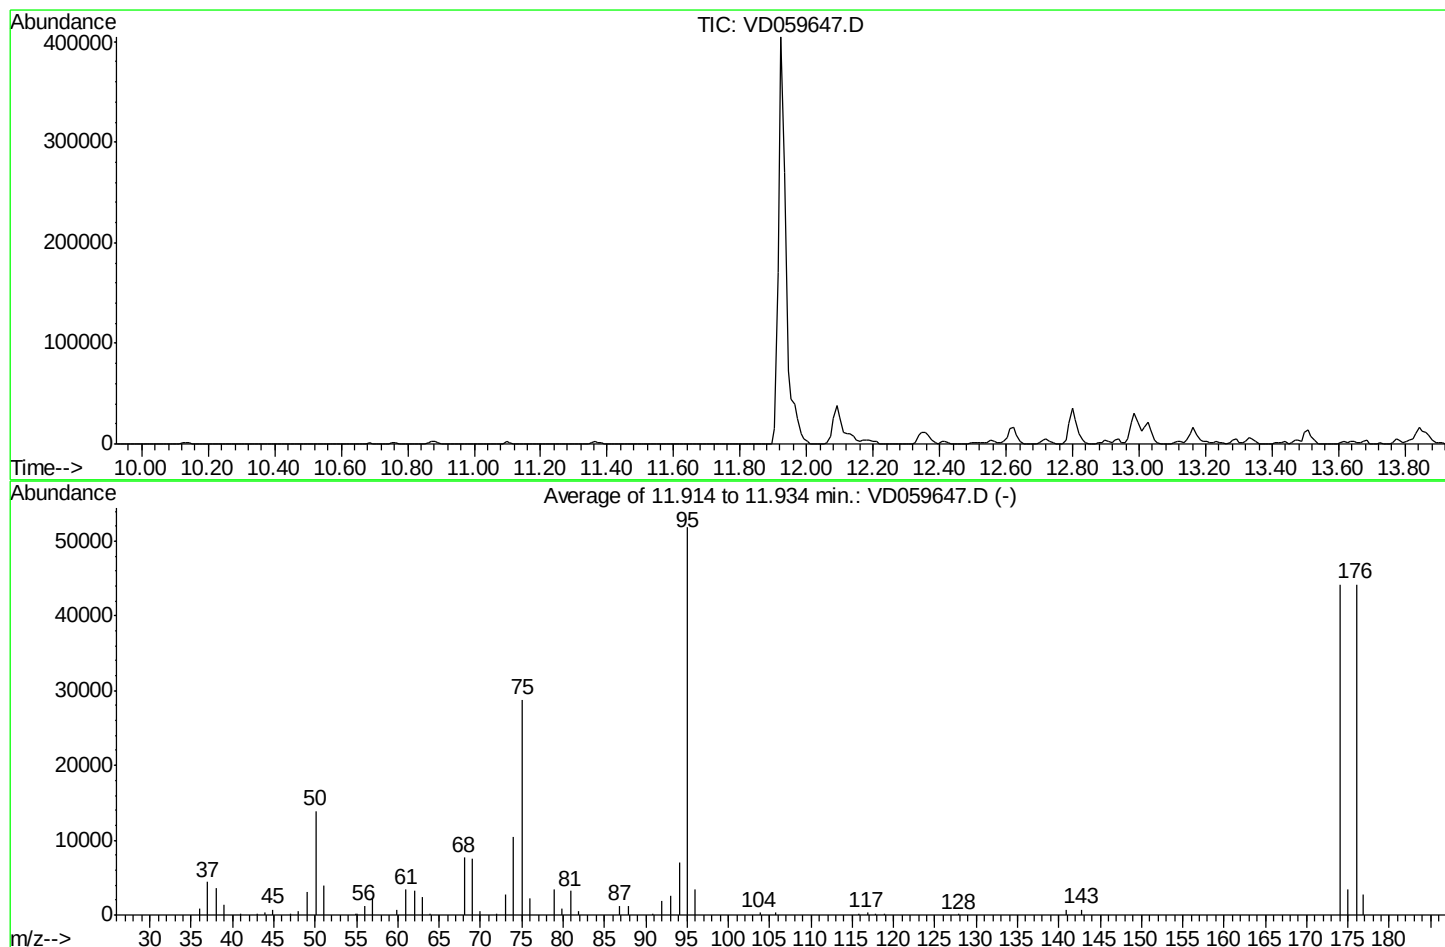

AutoFind: Scans 1188, 1189, 1190; Background Corrected with Scan 1184

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	26.8	13870	PASS
75	95	30	60	55.6	28837	PASS
95	95	100	100	100.0	51837	PASS
96	95	5	9	6.6	3433	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	85.2	44144	PASS
175	174	5	9	7.6	3361	PASS
176	174	95	101	100.1	44168	PASS
177	176	5	9	6.1	2682	PASS