


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD080119\
 Data File : VD063284.D
 Acq On : 1 Aug 2019 9:42
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D072919S.M
 Title : SW846 8260
 Last Update : Tue Jul 30 03:04:50 2019

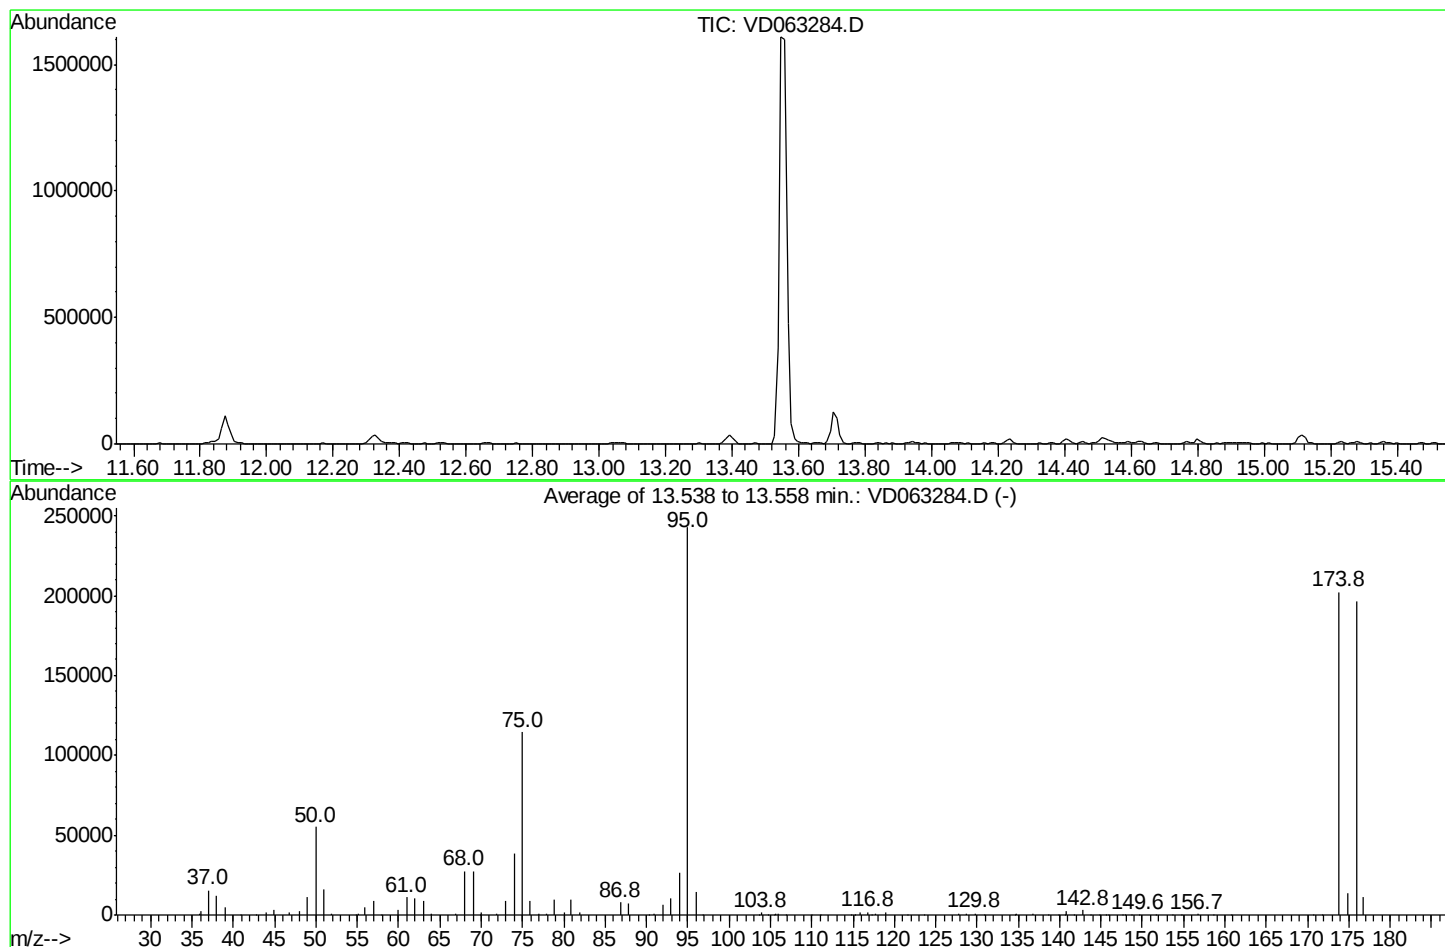

AutoFind: Scans 1230, 1231, 1232; Background Corrected with Scan 1226

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	55186	PASS
75	95	30	60	47.2	114626	PASS
95	95	100	100	100.0	242832	PASS
96	95	5	9	5.9	14287	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	83.3	202304	PASS
175	174	5	9	6.8	13839	PASS
176	174	95	101	97.1	196498	PASS
177	176	5	9	5.8	11462	PASS