


Dichlorodifluoromethane

Response Ratio

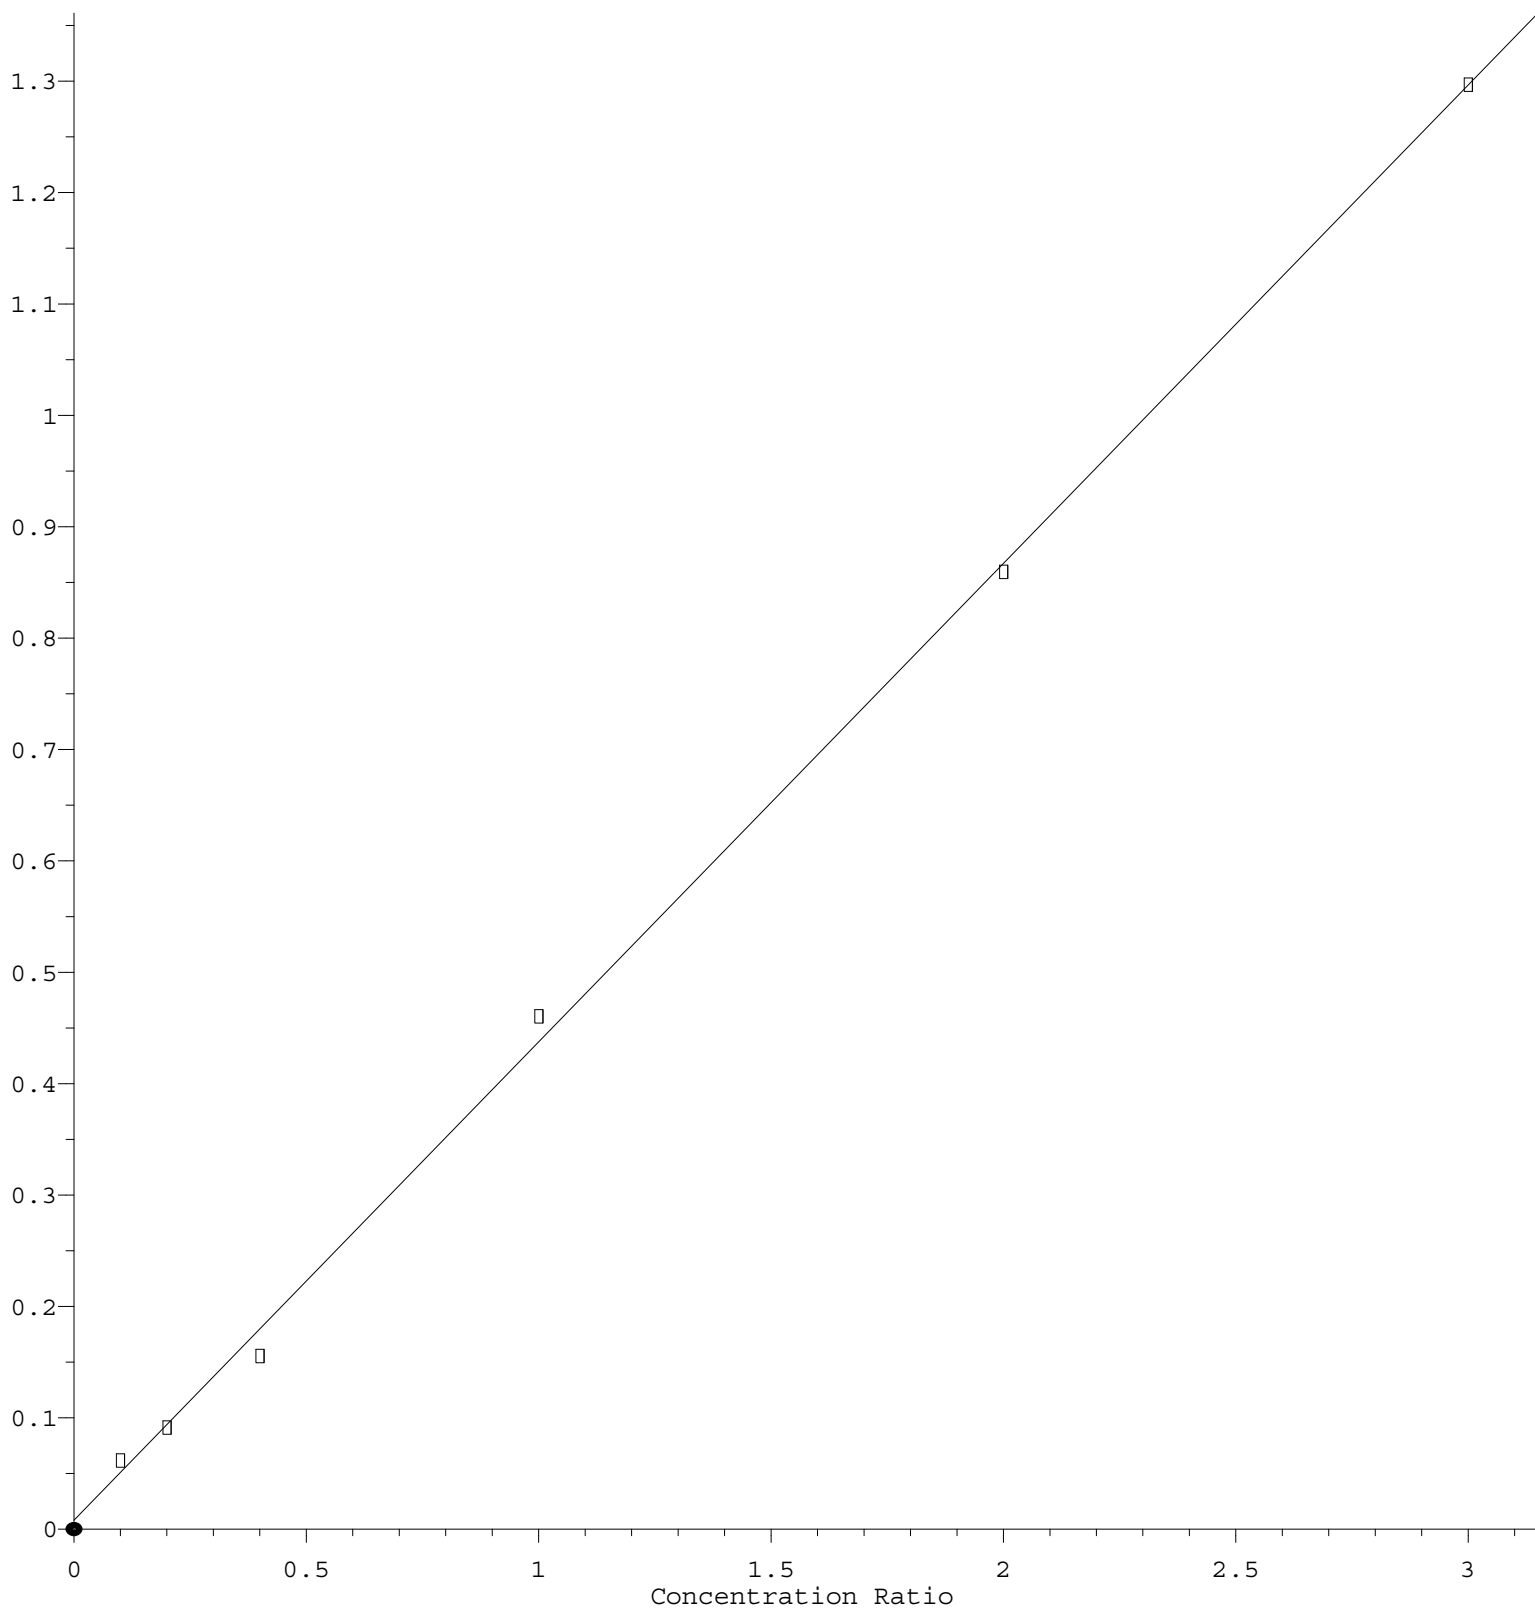


$$\text{Response} = 4.295\text{e-}001 * \text{Amt} + 7.801\text{e-}003$$

Coef of Det (r^2) = 0.998957 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D080122S.M

Calibration Table Last Updated: Tue Aug 02 05:13:57 2022


Tert butyl alcohol

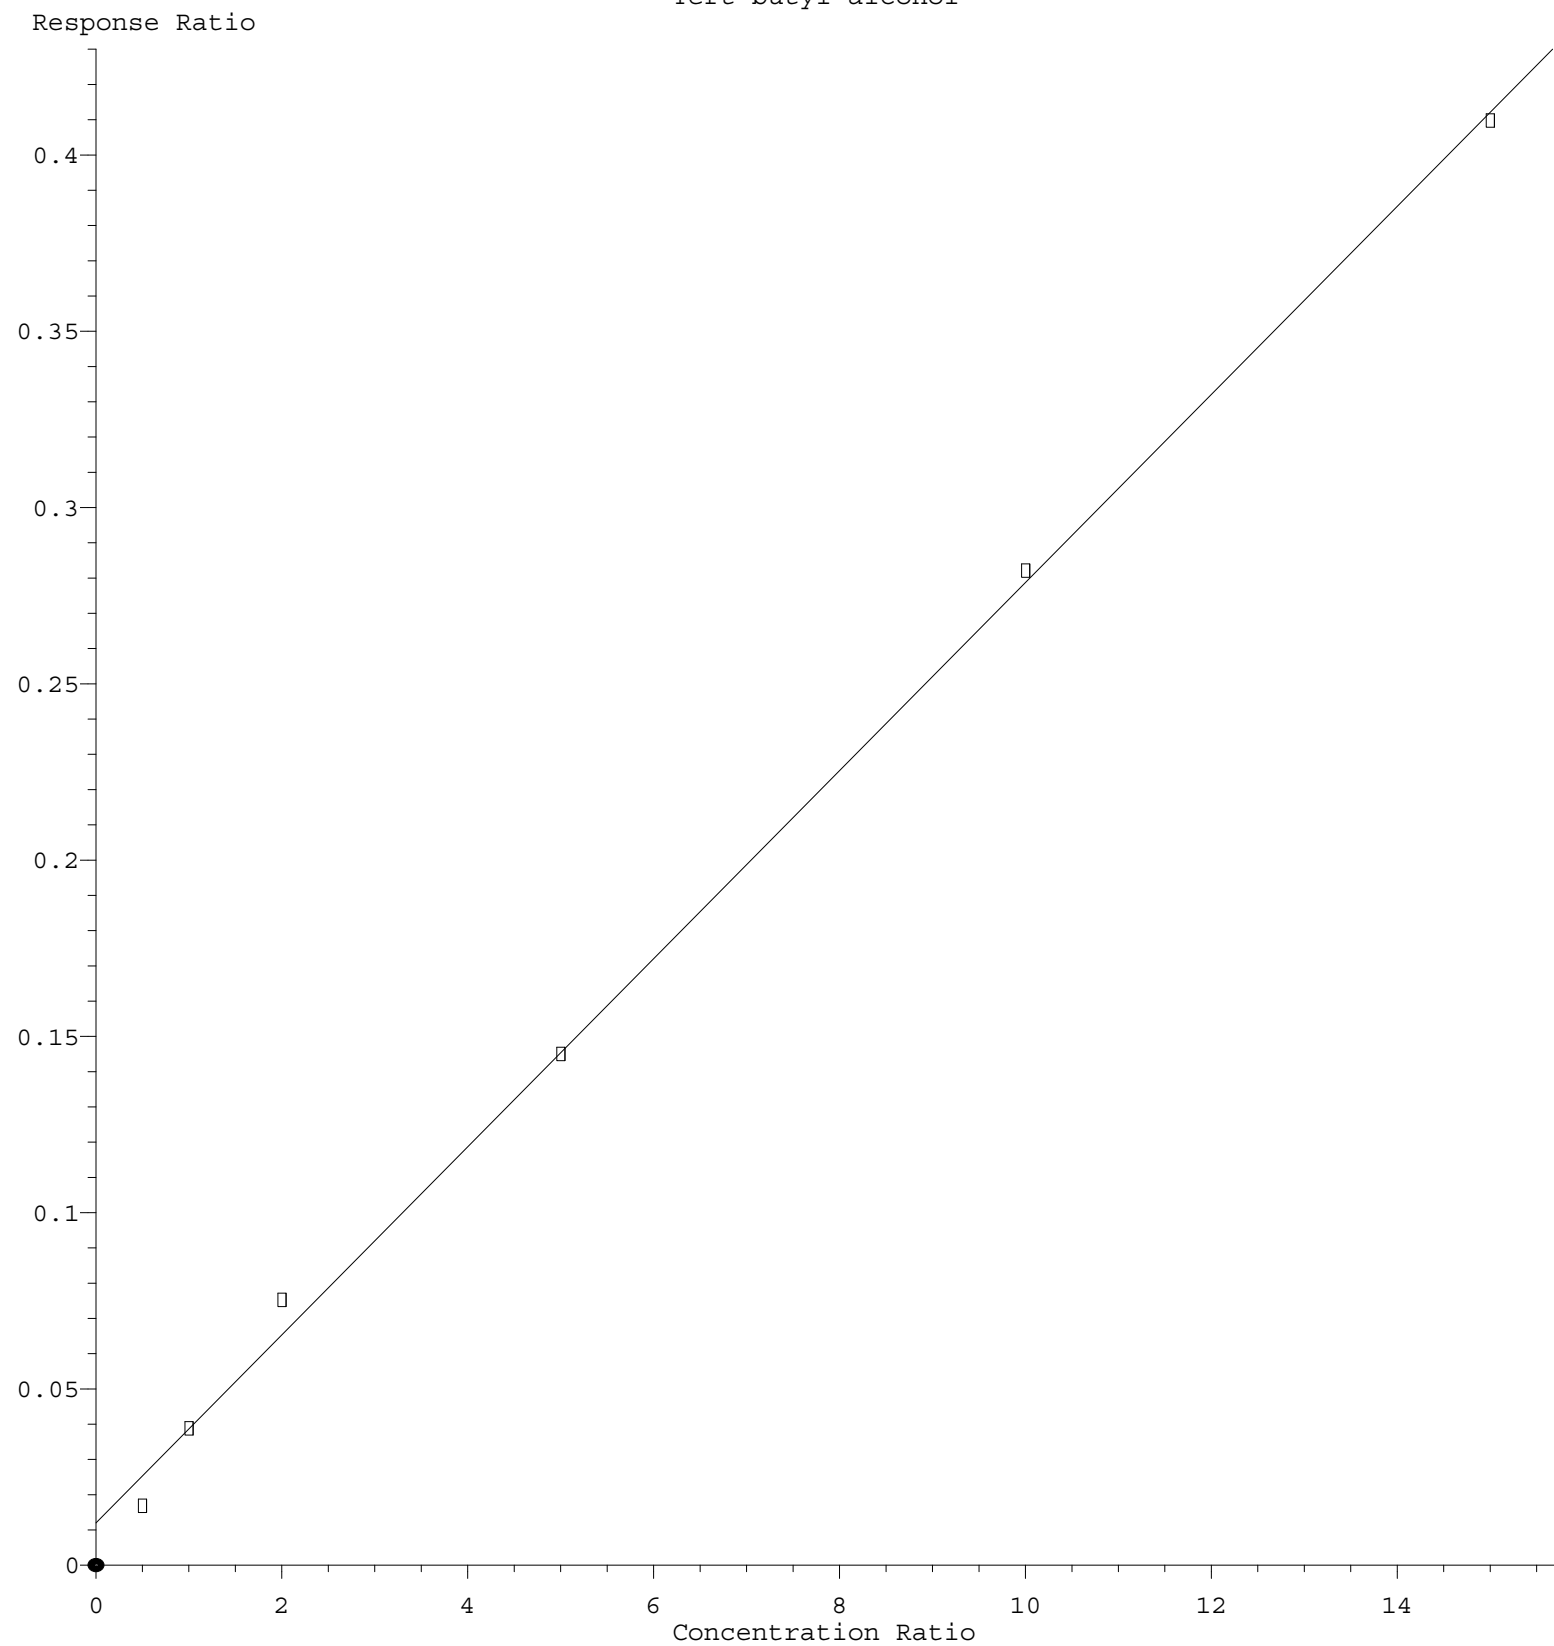

Response = $2.668 \times 10^{-2} \times \text{Amt} + 1.235 \times 10^{-2}$
Coef of Det (r^2) = 0.998444 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D080122S.M
Calibration Table Last Updated: Tue Aug 02 05:13:57 2022

1,2,3-Trichloropropane

Response Ratio

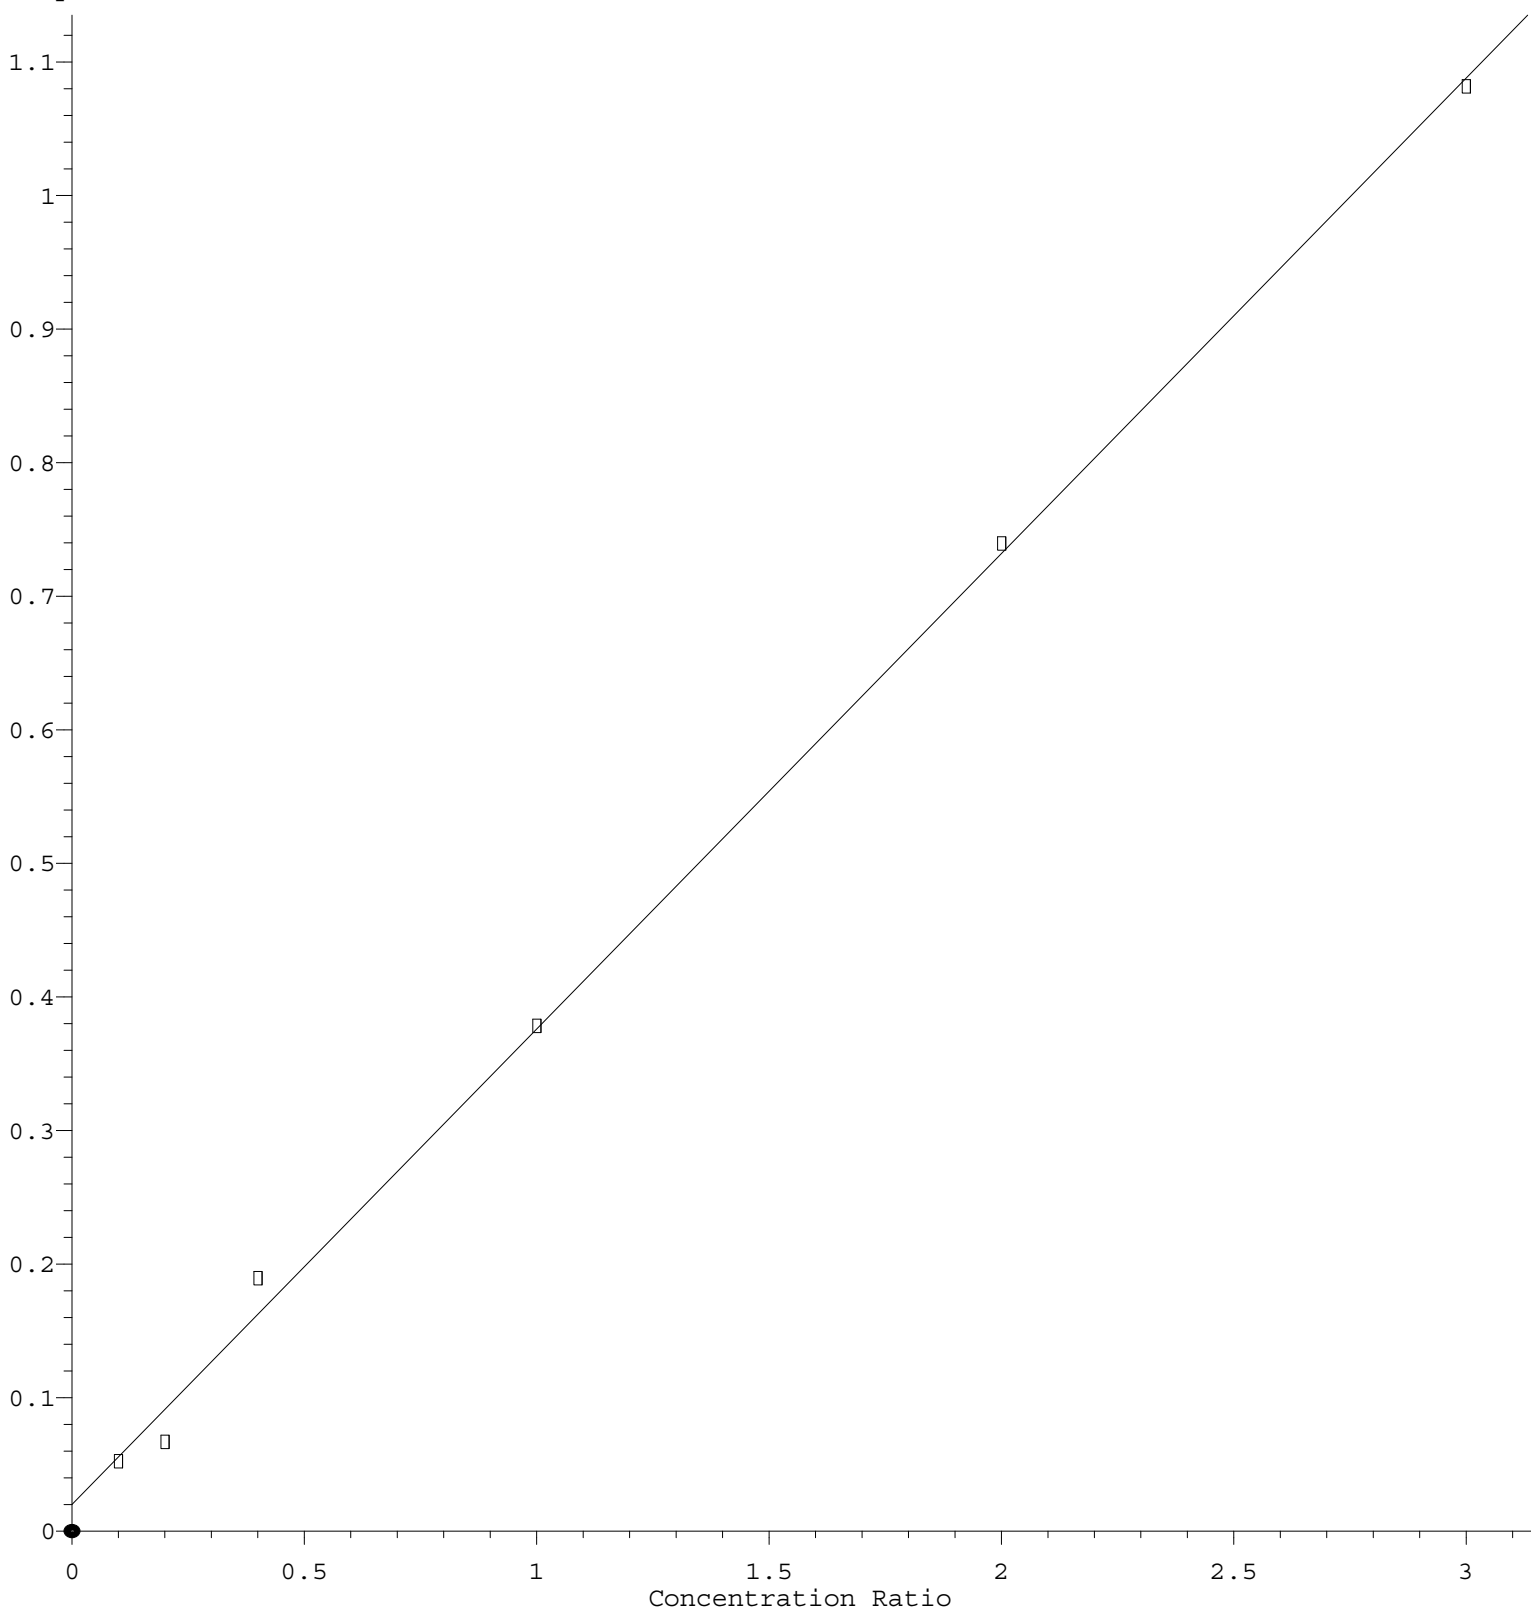

$$\text{Response} = 3.561\text{e-}001 * \text{Amt} + 2.034\text{e-}002$$


Coef of Det (r^2) = 0.998326 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D080122S.M

Calibration Table Last Updated: Tue Aug 02 05:13:57 2022

1,2-Dichloroethane-d4

Response Ratio

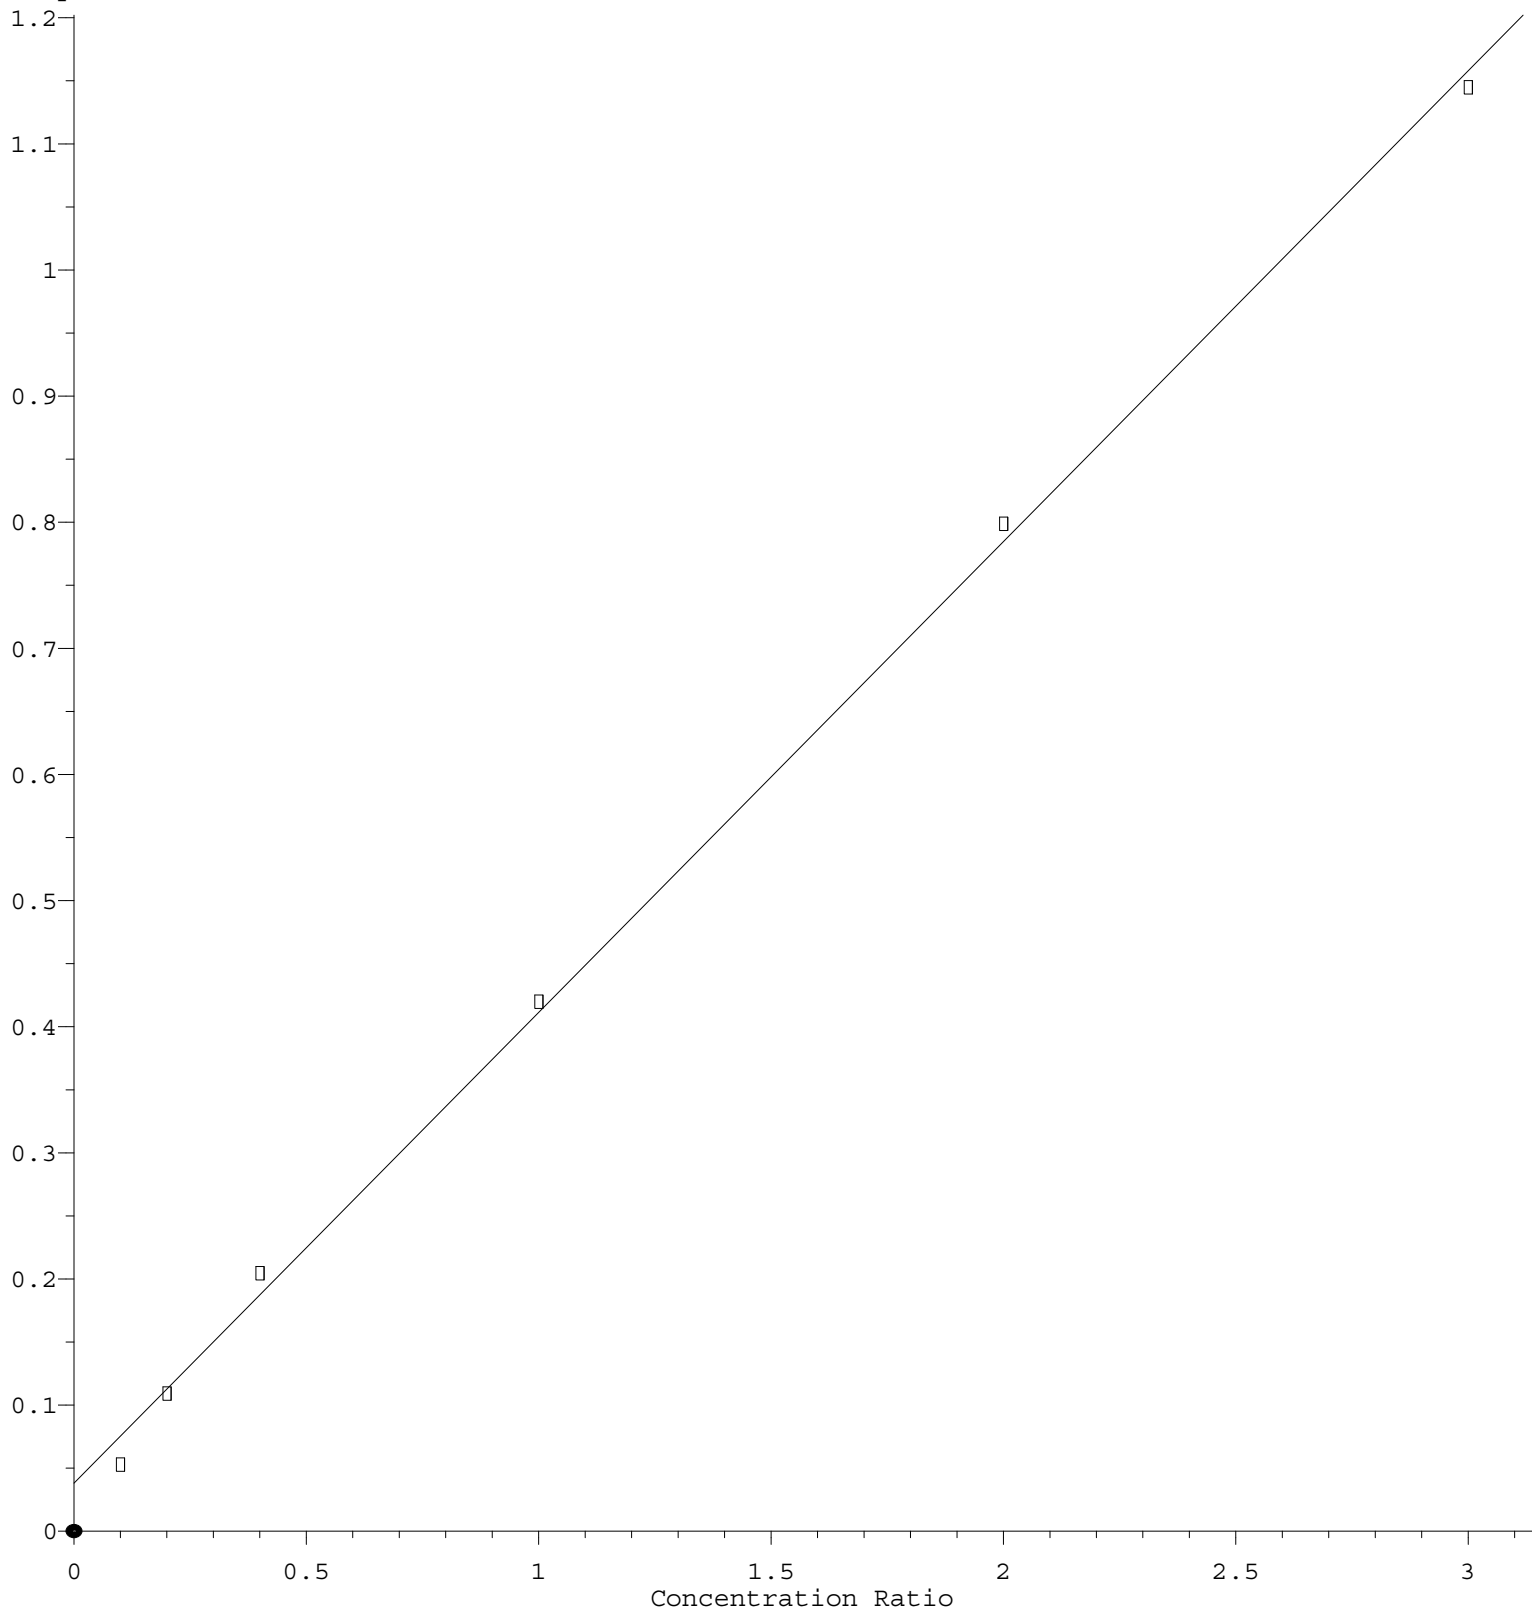

$$\text{Response} = 3.734\text{e-}001 * \text{Amt} + 3.795\text{e-}002$$


Coef of Det (r^2) = 0.998663 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D080122S.M

Calibration Table Last Updated: Tue Aug 02 05:13:57 2022

Methylene Chloride

Response Ratio

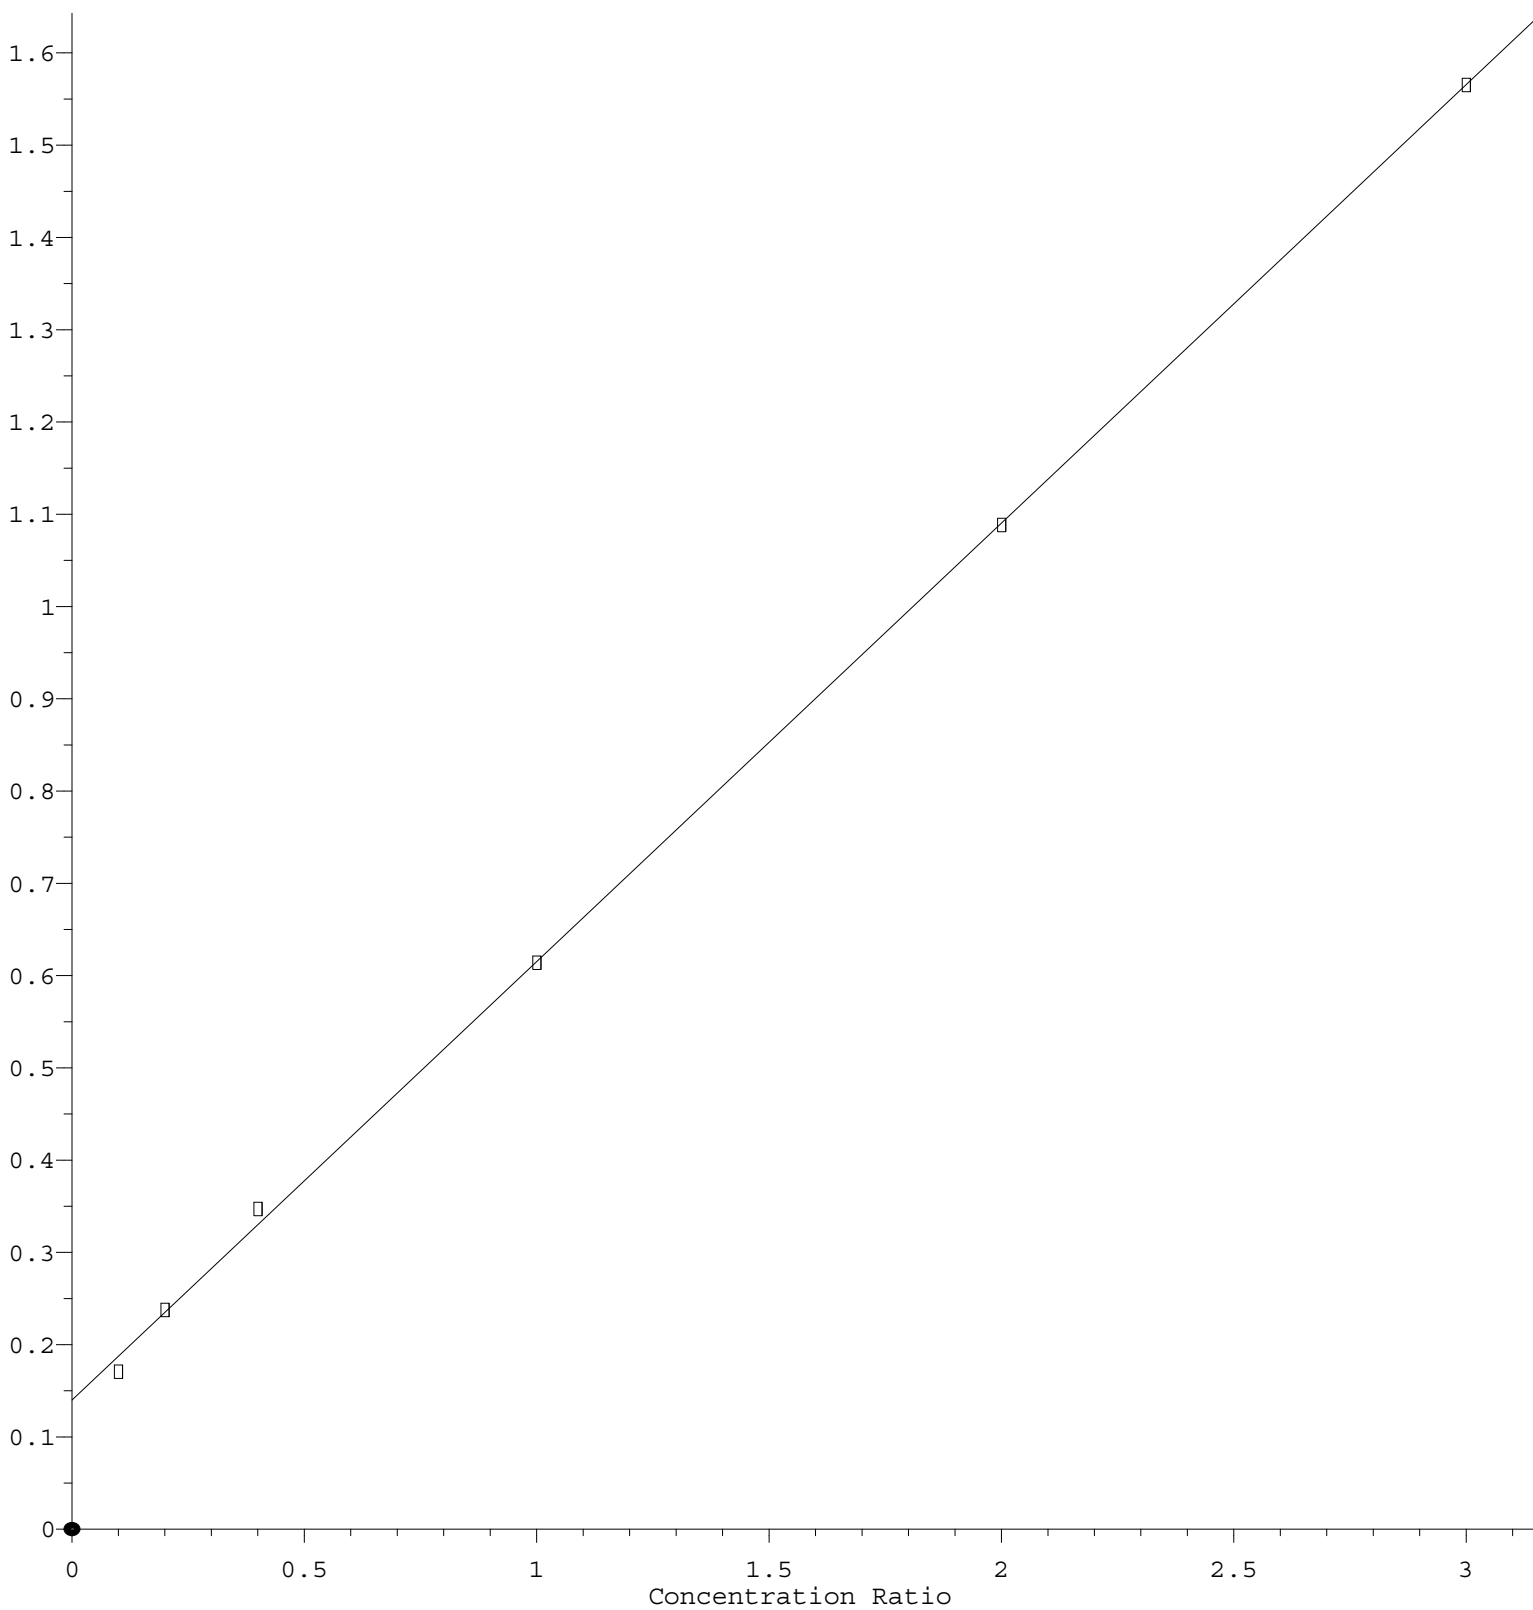


$$\text{Response} = 4.752\text{e-}001 * \text{Amt} + 1.398\text{e-}001$$

Coef of Det (r^2) = 0.999616 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D080122S.M

Calibration Table Last Updated: Tue Aug 02 05:13:57 2022


Methyl Acetate

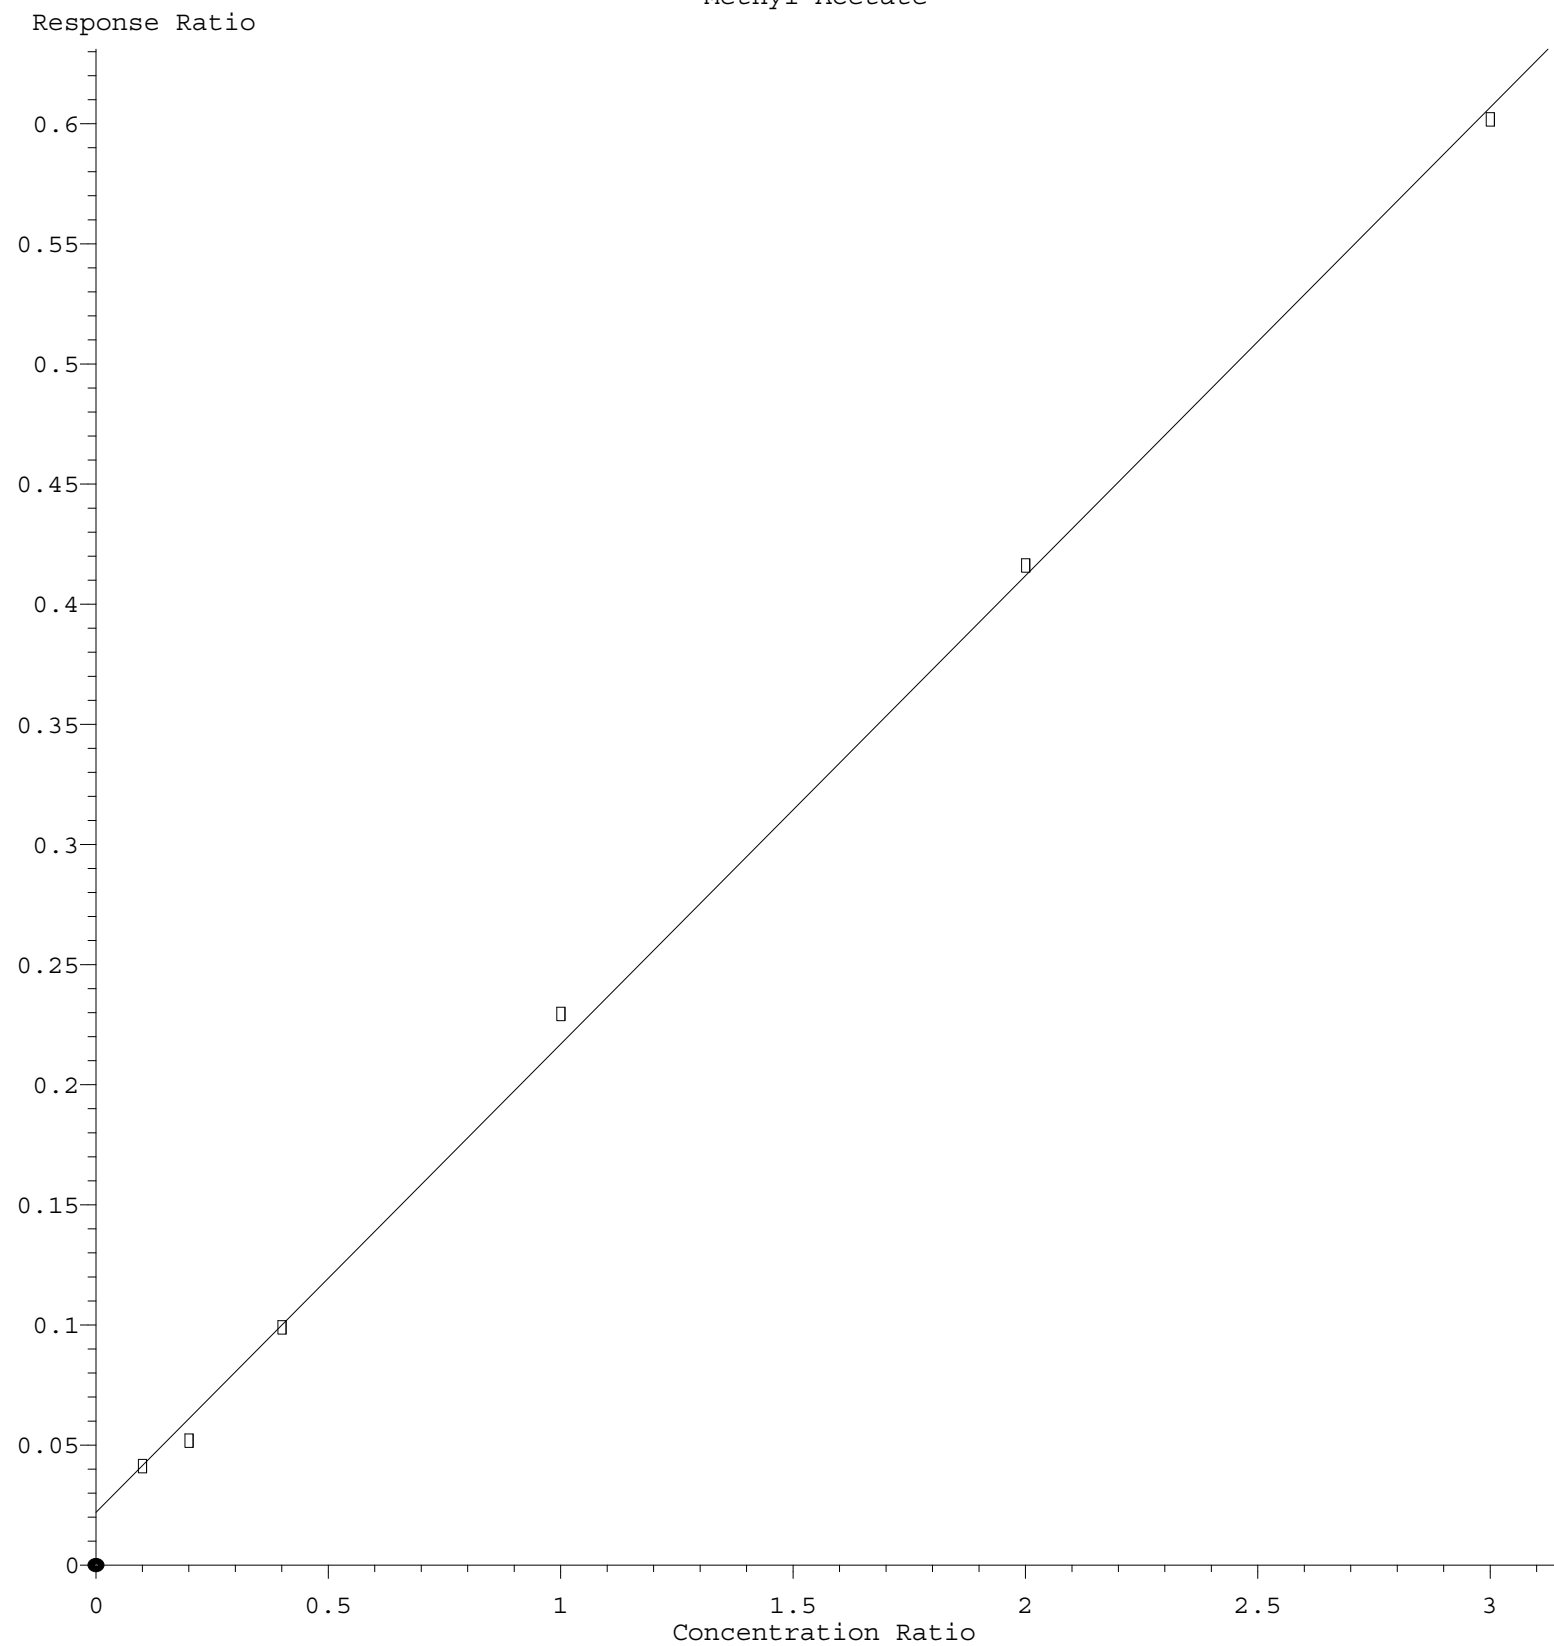

Response = 1.952e-001 * Amt + 2.186e-002
Coef of Det (r^2) = 0.998898 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D080122S.M
Calibration Table Last Updated: Tue Aug 02 05:13:57 2022

Carbon Disulfide

Response Ratio

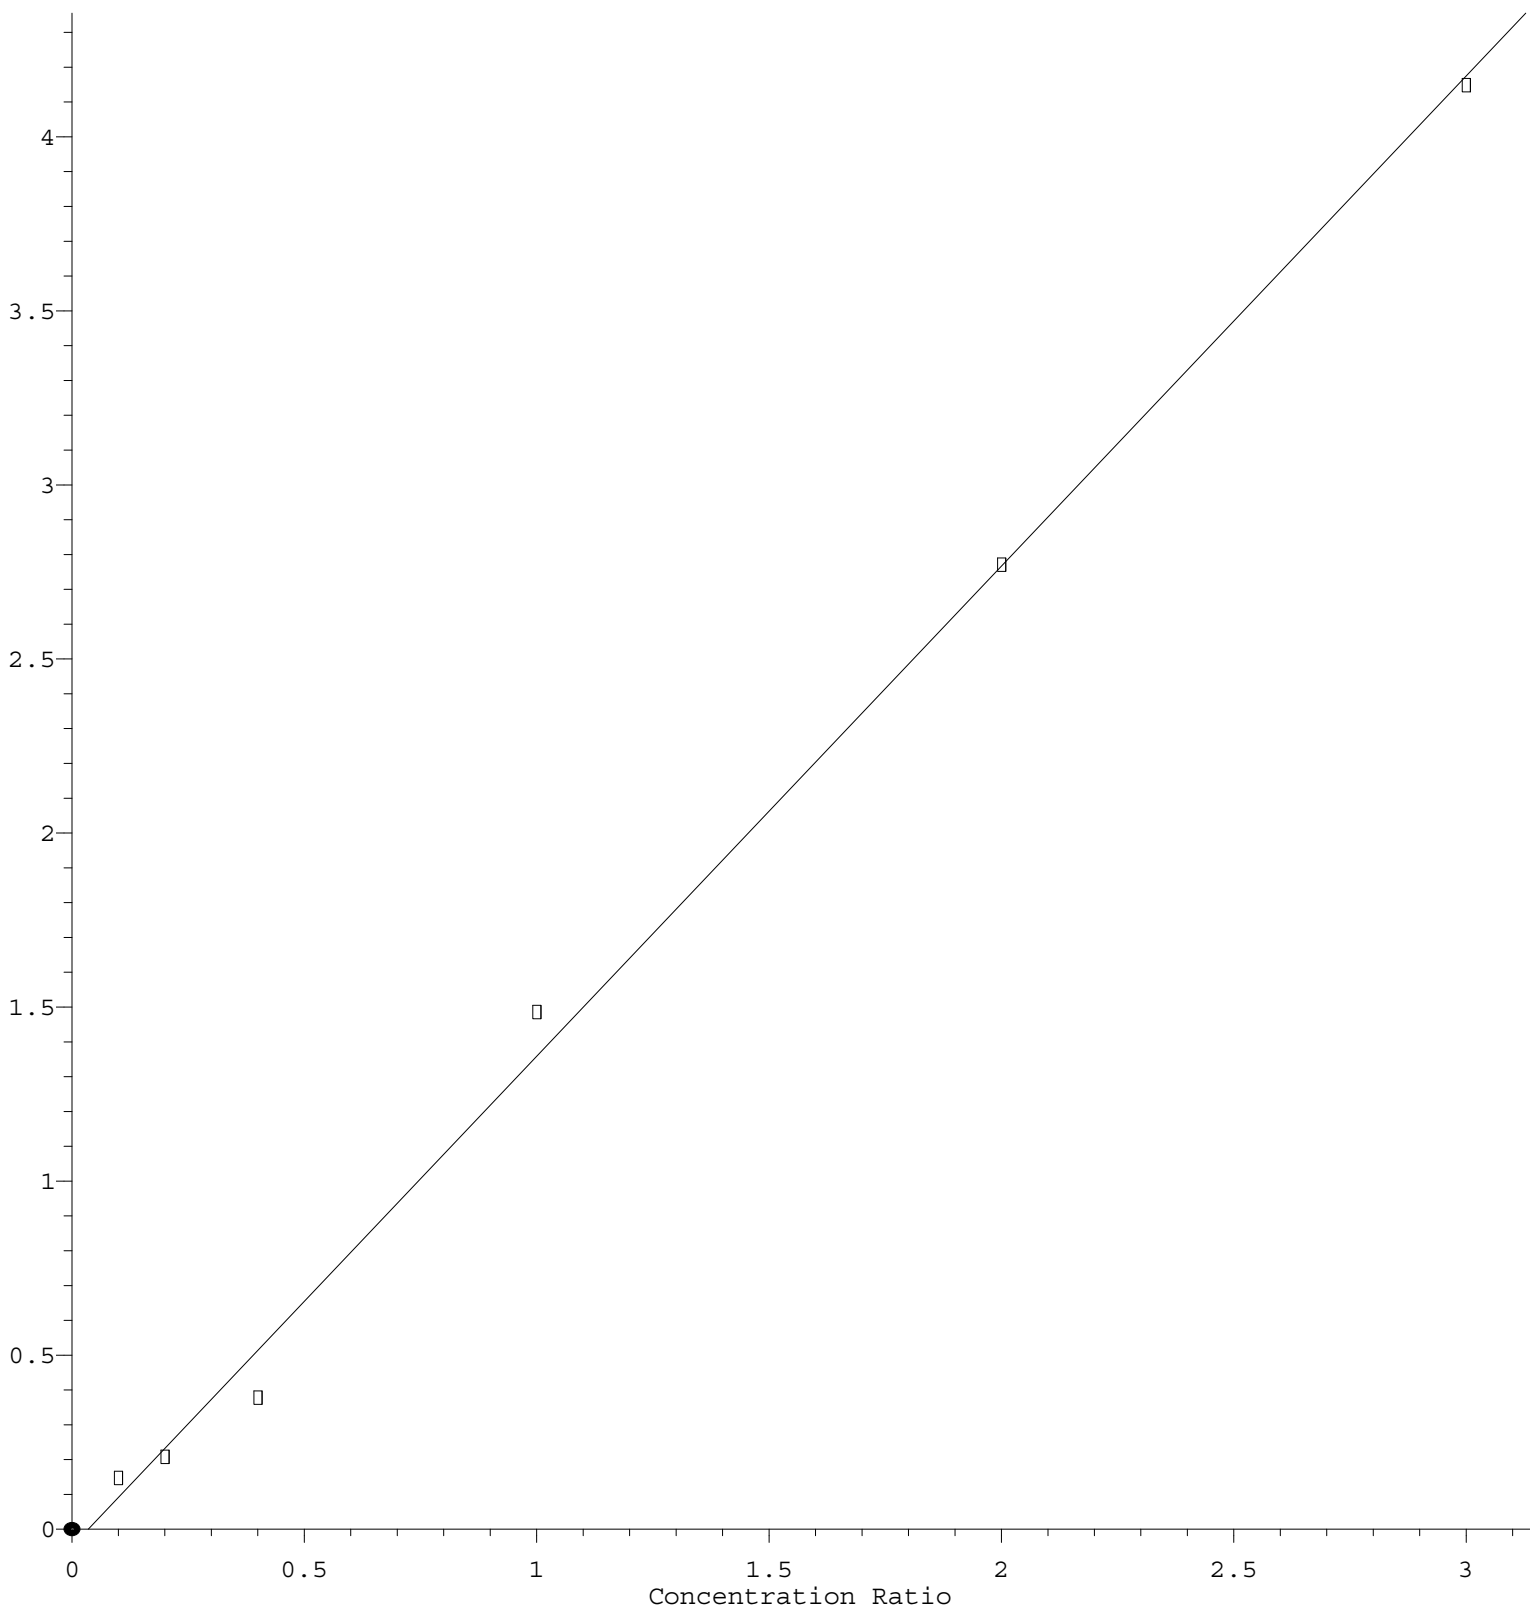

$$\text{Response} = 1.408\text{e}+000 * \text{Amt} - 4.980\text{e}-002$$


Coef of Det (r^2) = 0.997081 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D080122S.M

Calibration Table Last Updated: Tue Aug 02 05:13:57 2022


Acetone

Response Ratio

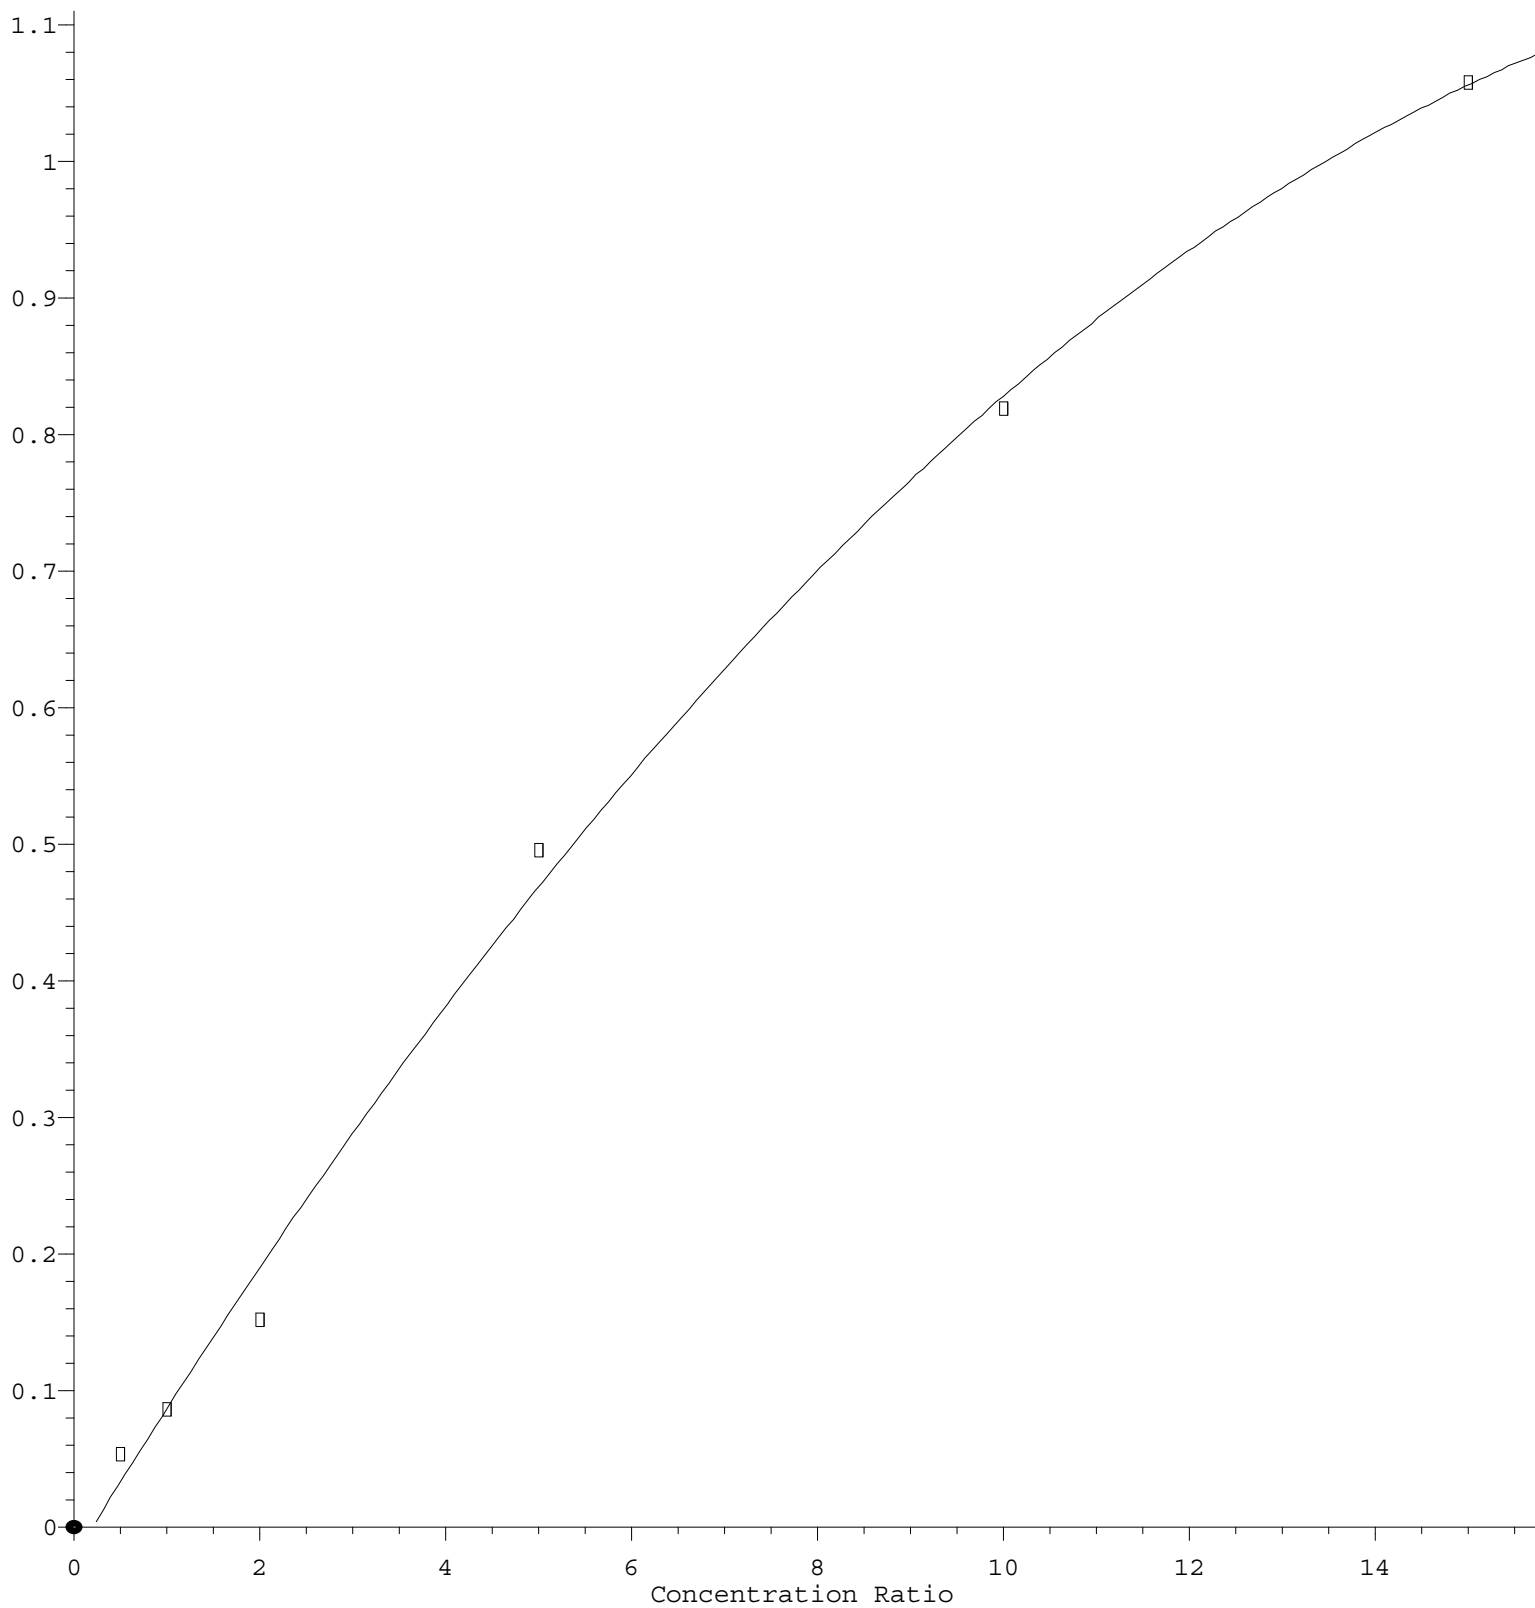

$R = -2.630e-003 A^2 + 1.113e-001 A - 2.171e-002$
 Coef of Det (r^2) = 0.996958 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D080122S.M
 Calibration Table Last Updated: Tue Aug 02 05:13:57 2022

Acrolein

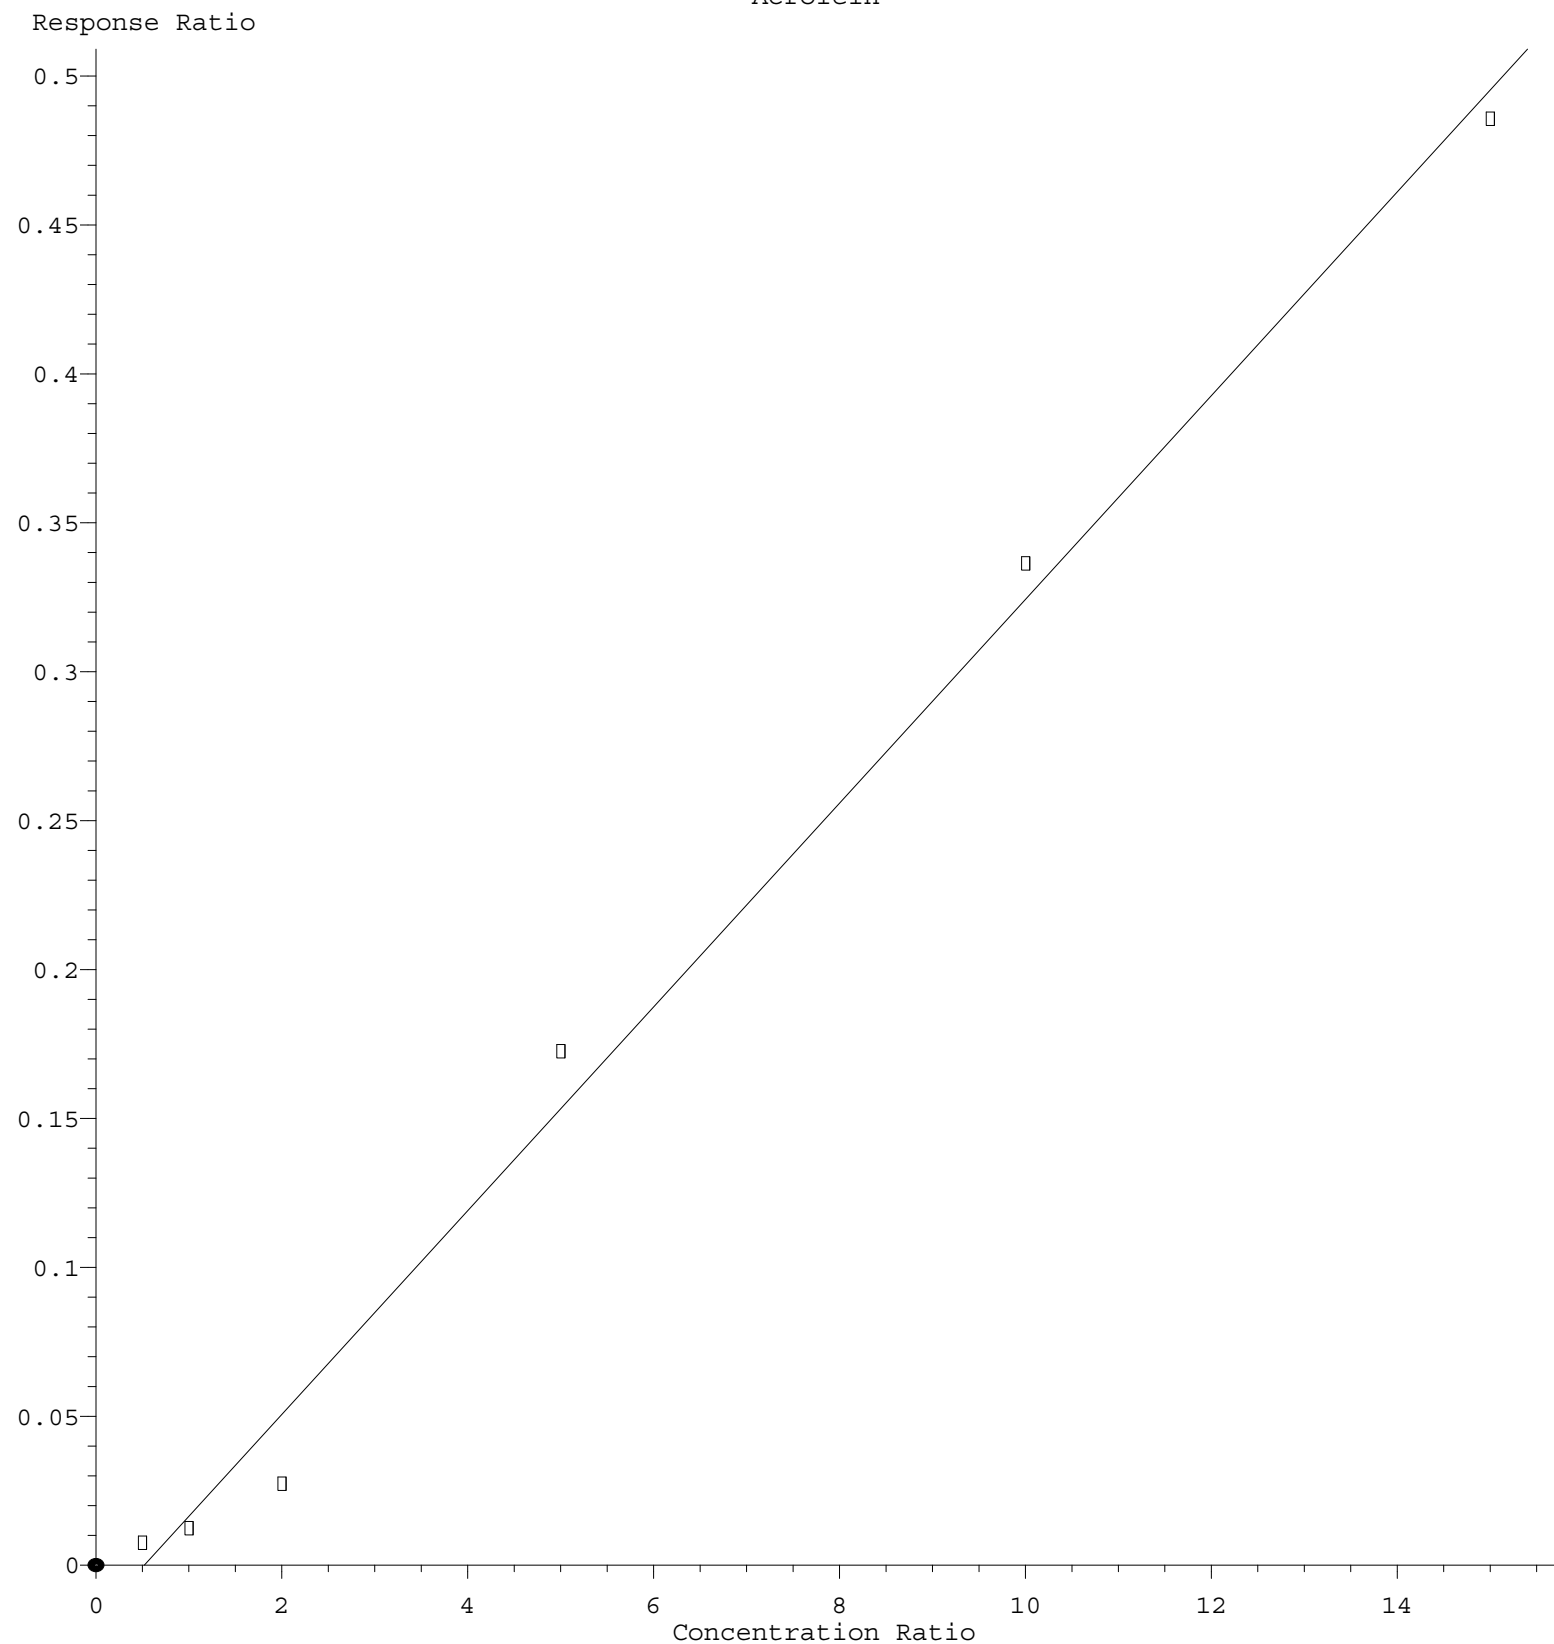

Response = $3.427 \times 10^{-2} \times \text{Amt} - 1.772 \times 10^{-2}$
 Coef of Det (r^2) = 0.993794 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D080122S.M
 Calibration Table Last Updated: Tue Aug 02 05:13:57 2022