
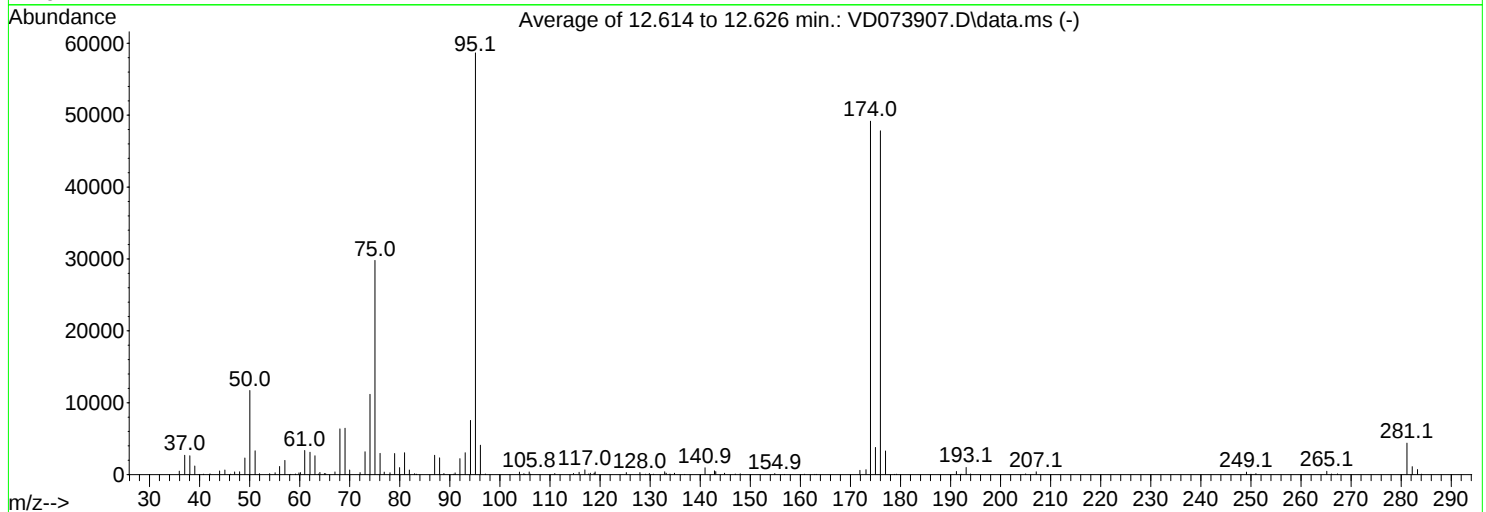


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080122\
Data File : VD073907.D
Acq On : 01 Aug 2022 09:28
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D080122S.M
Title : SW846 8260
Last Update : Tue Aug 02 05:13:57 2022

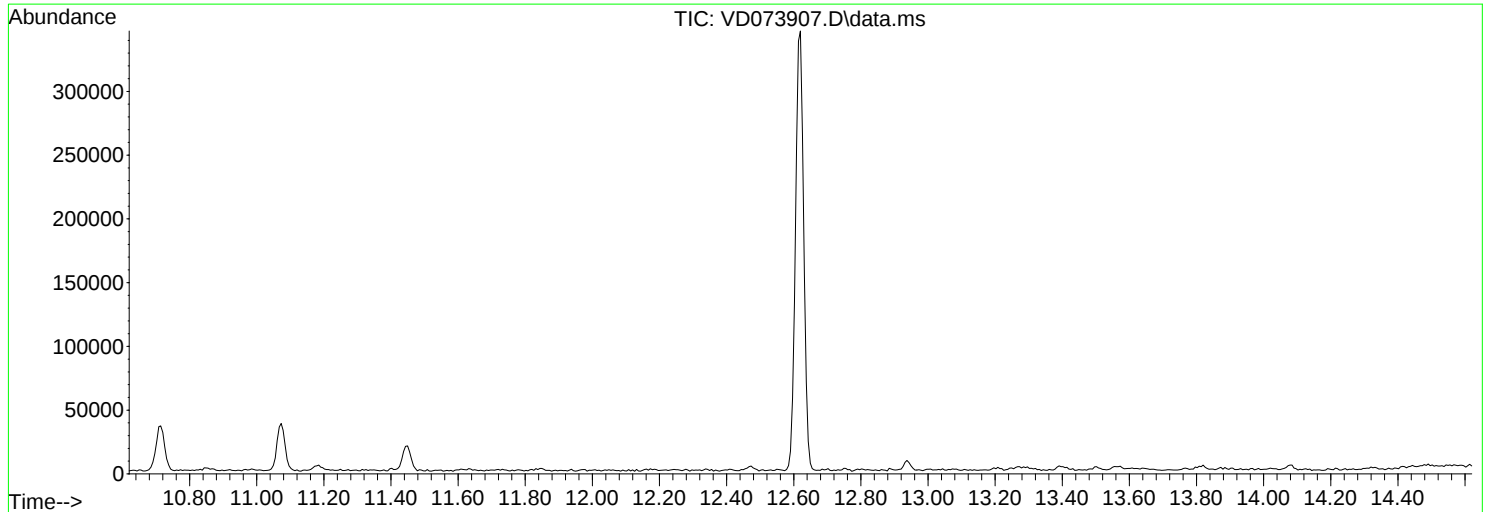

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1809

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.9	11701	PASS
75	95	30	60	50.8	29797	PASS
95	95	100	100	100.0	58672	PASS
96	95	5	9	7.0	4097	PASS
173	174	0.00	2	1.4	700	PASS
174	95	50	100	83.8	49168	PASS
175	174	5	9	7.7	3786	PASS
176	174	95	101	97.3	47837	PASS
177	176	5	9	6.9	3292	PASS