
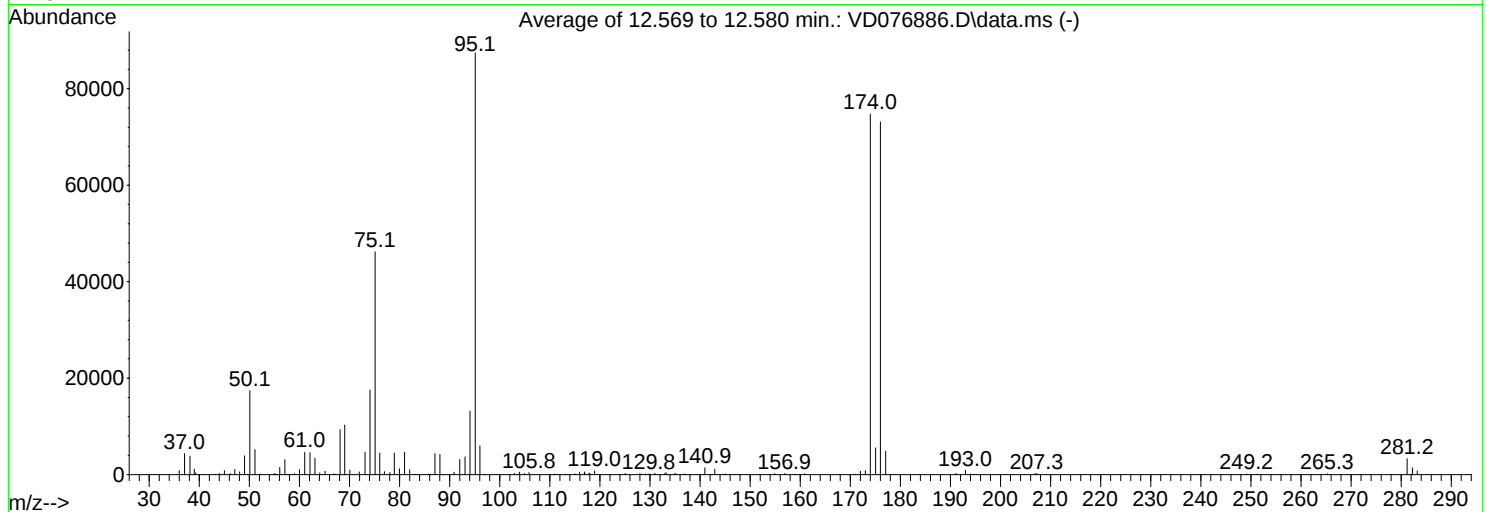


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD080123\  
Data File : VD076886.D  
Acq On : 01 Aug 2023 08:52  
Operator : KP/SY  
Sample : BFB  
Misc : 5.00G/5.0ml/MSVOA\_D/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D071423S.M  
Title : SW846 8260  
Last Update : Mon Jul 17 08:07:52 2023

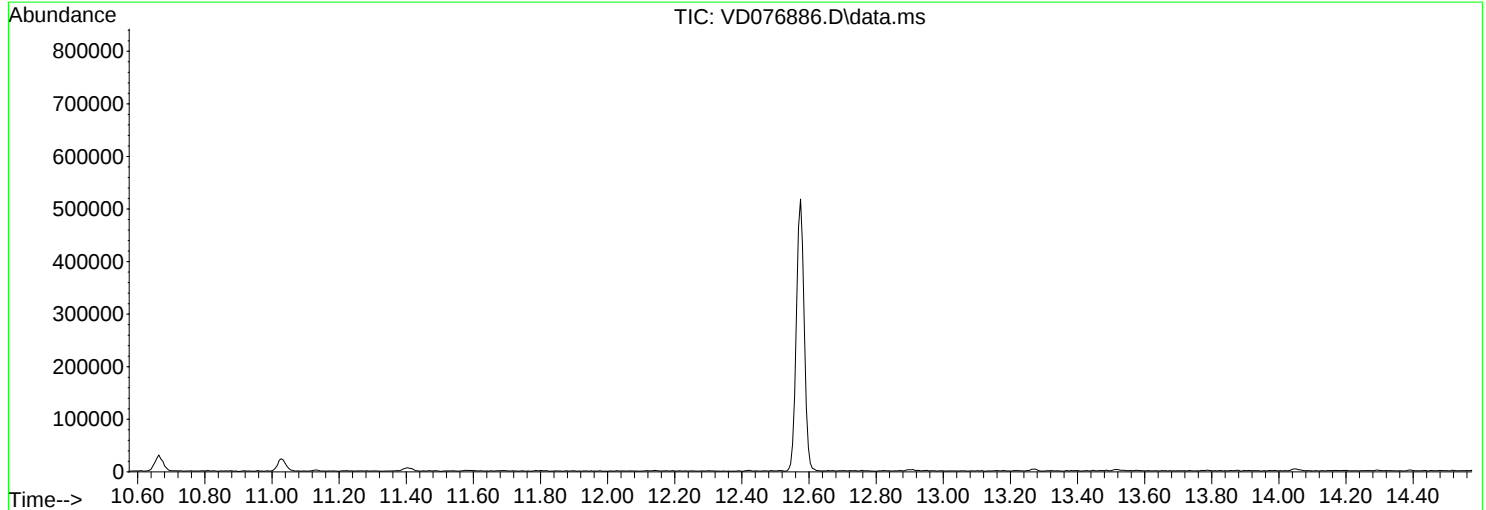

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 19.9         | 17406      | PASS                |
| 75             | 95              | 30              | 60              | 52.8         | 46195      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 87429      | PASS                |
| 96             | 95              | 5               | 9               | 6.8          | 5971       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.1          | 839        | PASS                |
| 174            | 95              | 50              | 100             | 85.5         | 74712      | PASS                |
| 175            | 174             | 5               | 9               | 7.4          | 5539       | PASS                |
| 176            | 174             | 95              | 101             | 97.8         | 73104      | PASS                |
| 177            | 176             | 5               | 9               | 6.7          | 4879       | PASS                |