

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD080219\
 Data File : VD063326.D
 Acq On : 2 Aug 2019 19:35
 Operator : VA/AP
 Sample : K4130-08
 Misc : 5.82g/5ml/MSVOA D/SOIL
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 1S-F2-(30)

Quant Time: Aug 04 04:35:33 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D072919S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 30 03:04:50 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.02	168	125161	50.00	ug/l	-0.02
34) 1,4-Difluorobenzene	8.20	114	182729	50.00	ug/l	0.00
63) Chlorobenzene-d5	12.35	117	173561	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	14.51	152	100286	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.43	65	99785	71.85	ug/l	0.00
Spiked Amount 50.000			Recovery	=	143.70%	
35) Dibromofluoromethane	6.90	113	81775	52.42	ug/l	0.00
Spiked Amount 50.000			Recovery	=	104.84%	
50) Toluene-d8	10.39	98	143472	41.09	ug/l	0.00
Spiked Amount 50.000			Recovery	=	82.18%	
62) 4-Bromofluorobenzene	13.54	95	73706	46.32	ug/l	0.00
Spiked Amount 50.000			Recovery	=	92.64%	
Target Compounds						
20) Methylene Chloride	3.79	84	9373	8.570	ug/l	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD080219\
Data File : VD063326.D
Acq On : 2 Aug 2019 19:35
Operator : VA/AP
Sample : K4130-08
Misc : 5.82g/5ml/MSVOA D/SOIL
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
1S-F2-(30)

Quant Time: Aug 04 04:35:33 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D072919S.M
Quant Title : SW846 8260
QLast Update : Tue Jul 30 03:04:50 2019
Response via : Initial Calibration

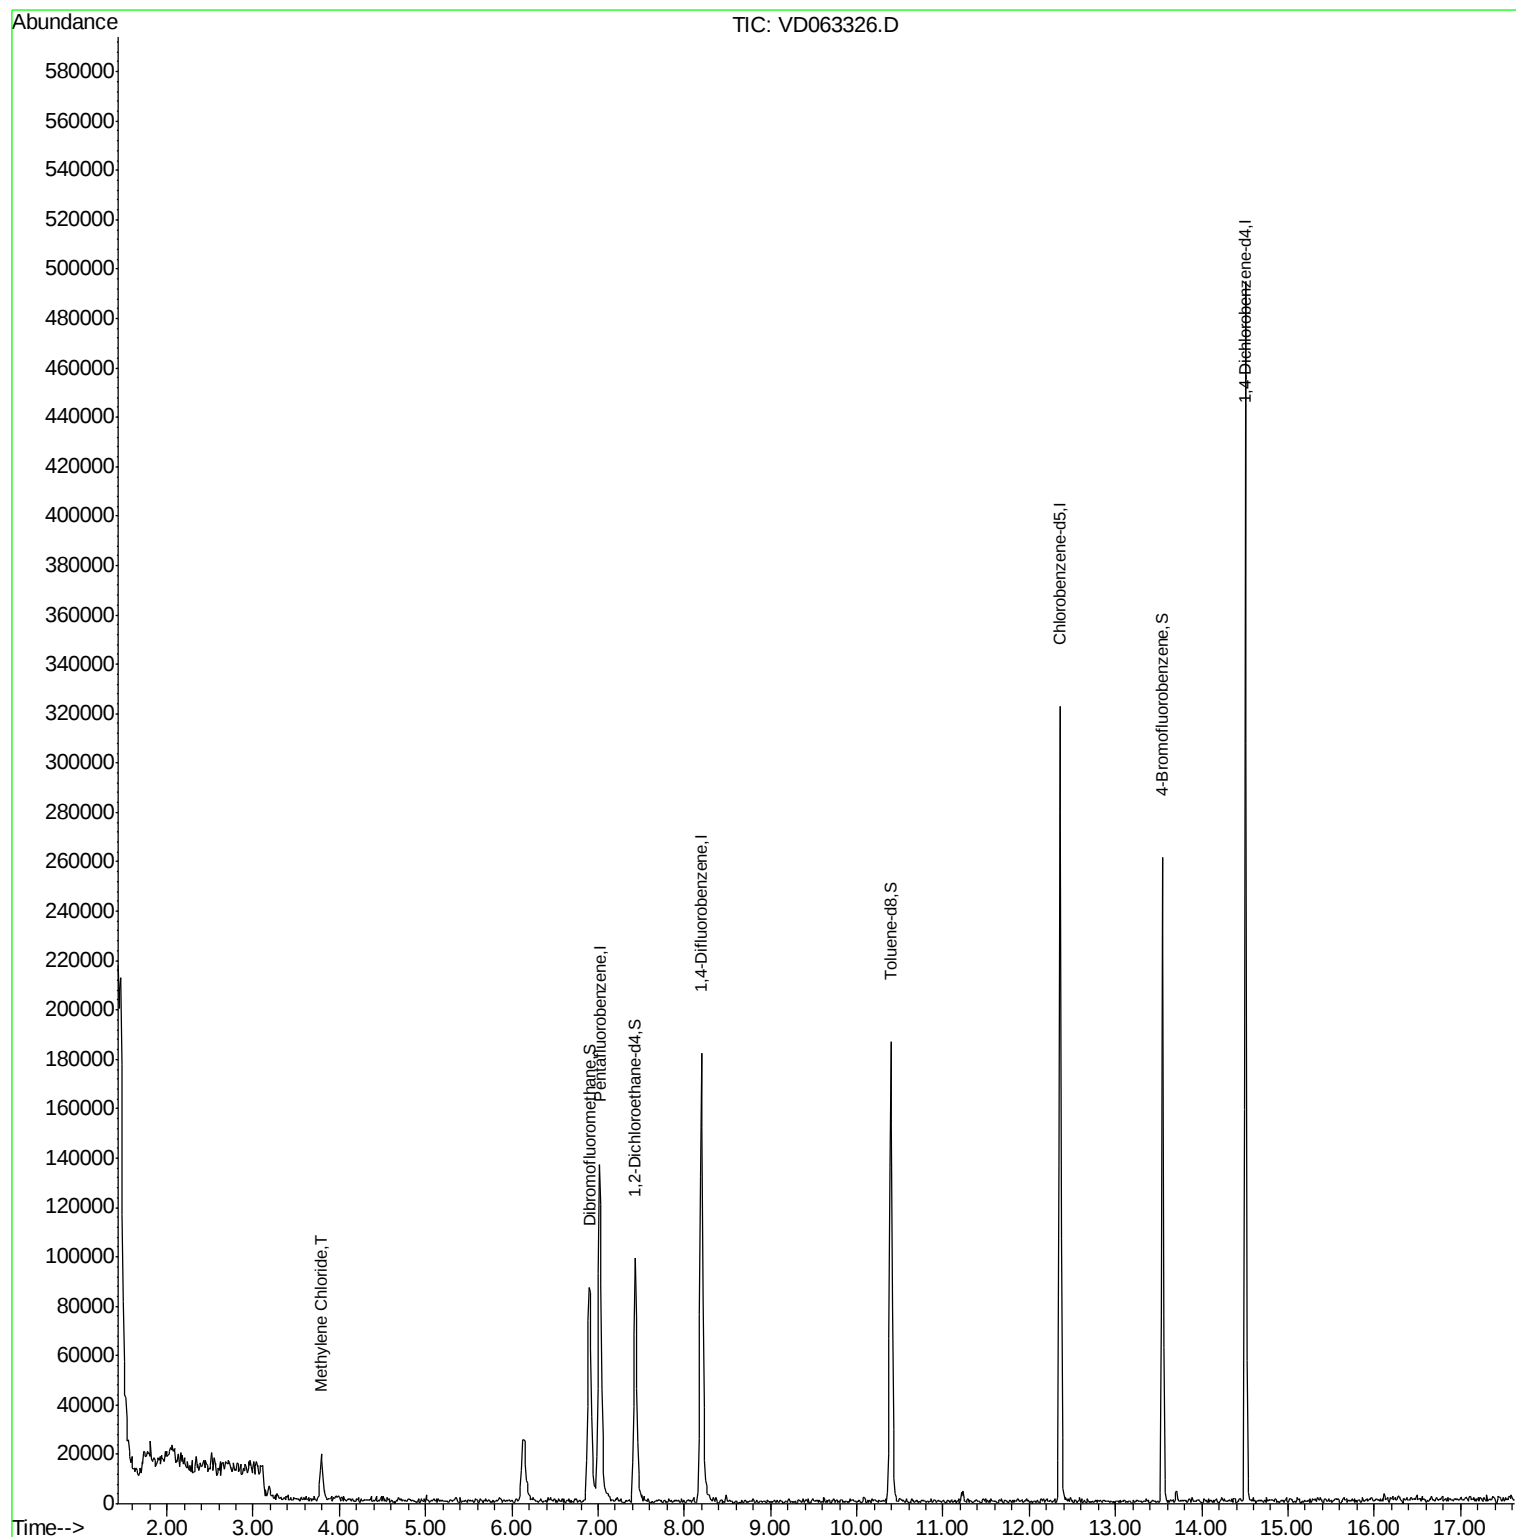

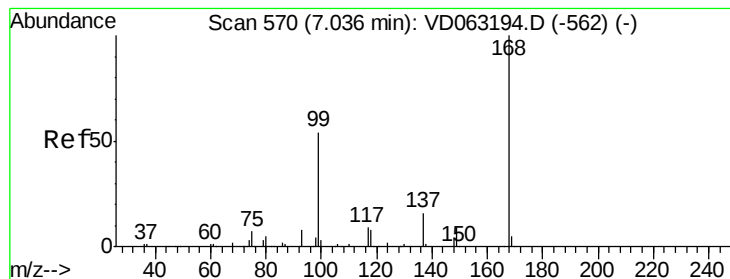

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.02 min Scan# 568

Delta R.T. -0.02 min

Lab File: VD063326.D

Acq: 2 Aug 2019 19:35

Instrument :

MSVOA_D

ClientSampleId :


1S-F2-(30)

Tot Ion:168 Resp: 125161

Ion Ratio Lower Upper




168 100

99 56.6 43.7 65.5

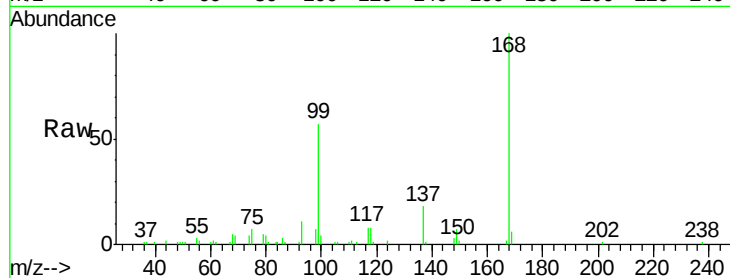

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.95 (98.65 to 99.65): VDC

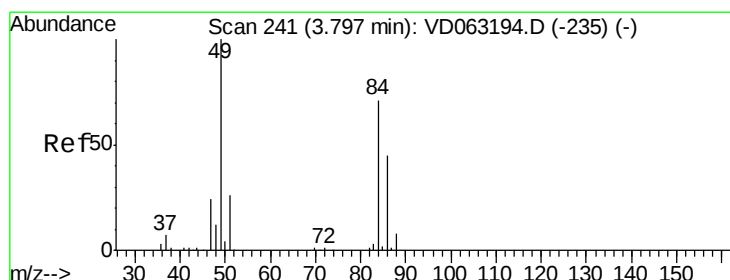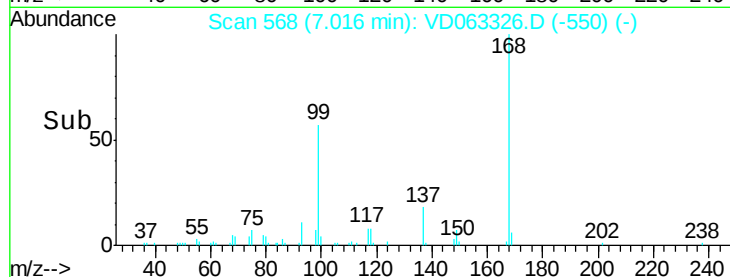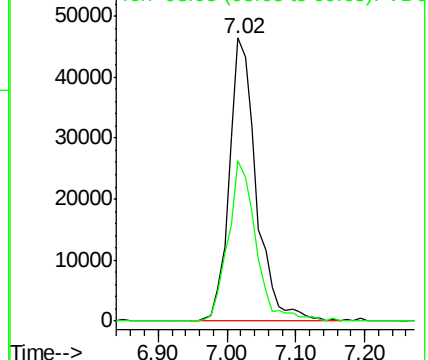

#20

Methylene Chloride

Concen: 8.570 ug/l

RT: 3.79 min Scan# 240

Delta R.T. -0.01 min

Lab File: VD063326.D

Acq: 2 Aug 2019 19:35

Tgt Ion: 84 Resp: 9373


Ion Ratio Lower Upper

84 100

49 132.0 112.5 168.7

51 39.6 29.6 44.4

86 68.5 50.4 75.6


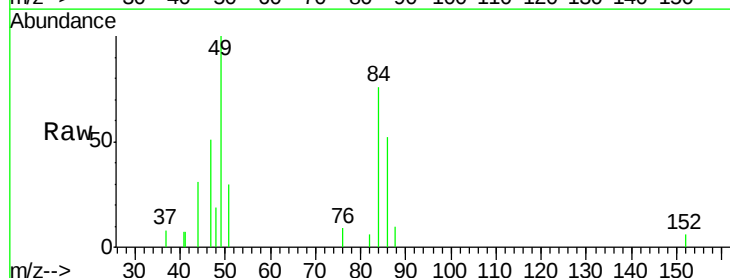



Abundance Ion 83.95 (83.65 to 84.65): VDC

Ion 48.90 (48.60 to 49.60): VDC

Ion 50.90 (50.60 to 51.60): VDC

Ion 85.90 (85.60 to 86.60): VDC

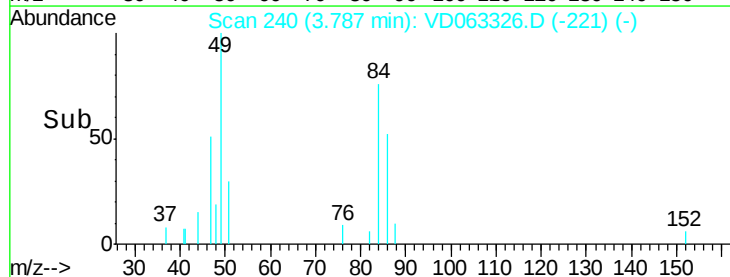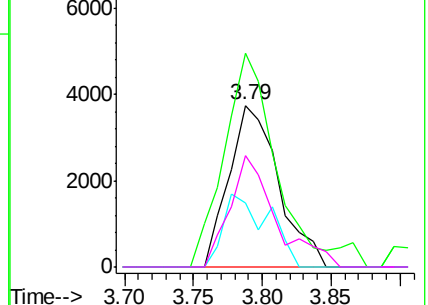

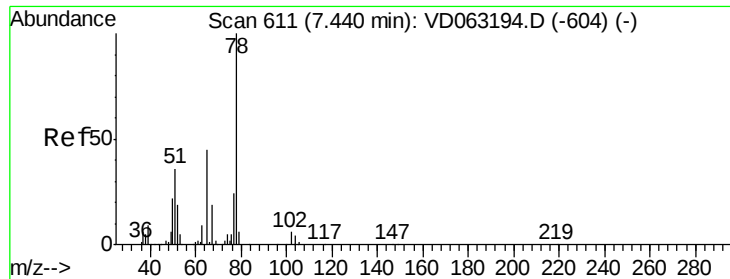

#33

1,2-Dichloroethane-d4

Concen: 71.851 ug/l

RT: 7.43 min Scan# 610

Delta R.T. -0.01 min

Lab File: VD063326.D

Acq: 2 Aug 2019 19:35

Instrument :

MSVOA_D

ClientSampleId :


1S-F2-(30)

Tot Ion: 65 Resp: 99785

Ion Ratio Lower Upper




65 100

67 50.1 0.0 85.8

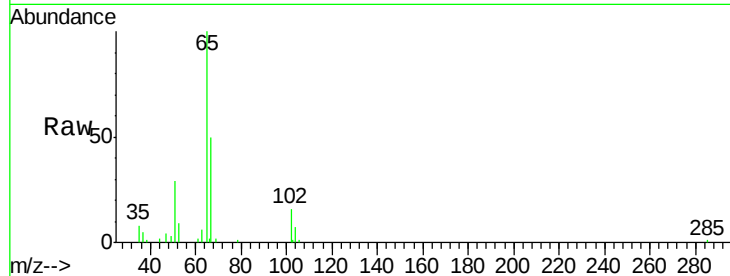

Abundance Ion 64.95 (64.65 to 65.65): VDC

Ion 66.90 (66.60 to 67.60): VDC

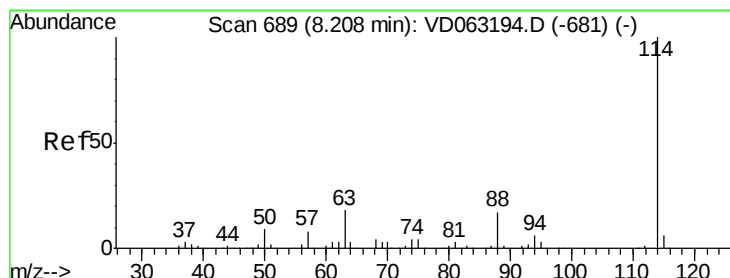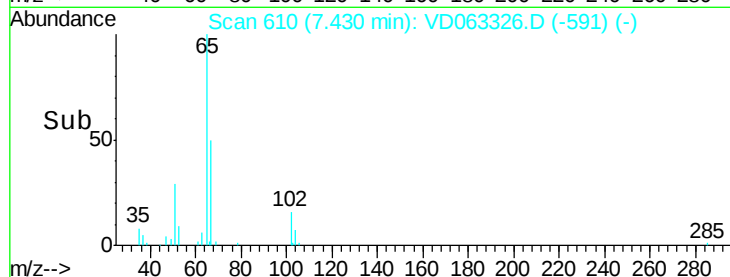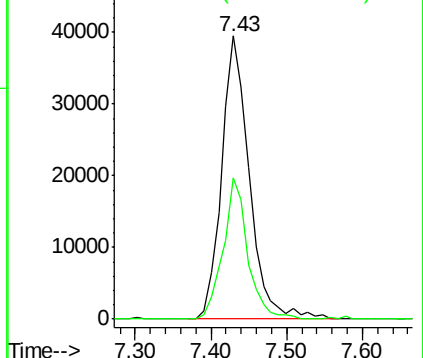

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.20 min Scan# 688

Delta R.T. -0.01 min

Lab File: VD063326.D

Acq: 2 Aug 2019 19:35


Tgt Ion: 114 Resp: 182729

Ion Ratio Lower Upper

114 100

63 24.3 0.0 35.2



88 18.2 0.0 34.6

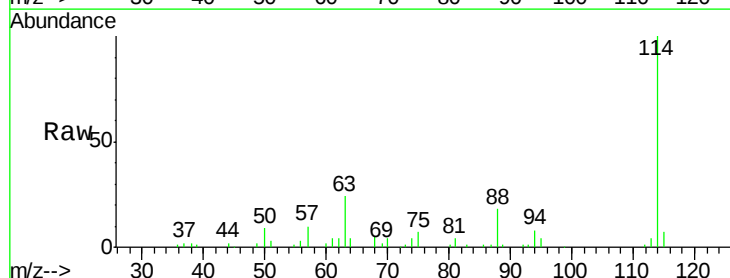

Abundance Ion 114.00 (113.70 to 114.70): V

Ion 62.95 (62.65 to 63.65): VDC

Ion 87.90 (87.60 to 88.60): VDC

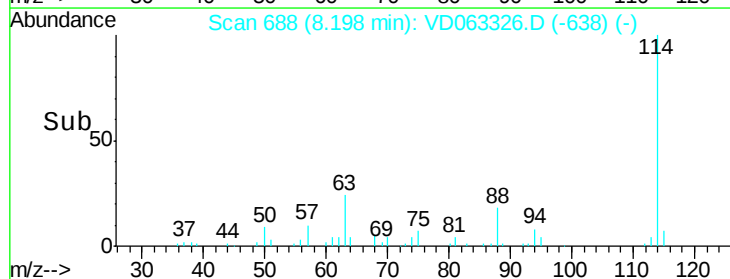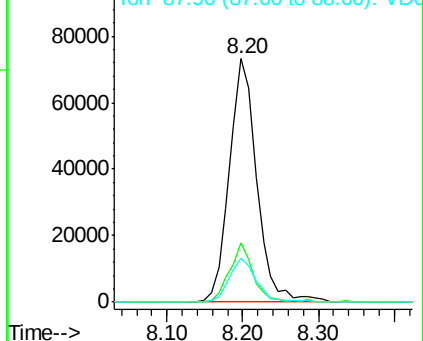



#35

Dibromofluoromethane

Concen: 52.416 ug/l

RT: 6.90 min Scan# 556

Delta R.T. -0.01 min

Lab File: VD063326.D

Acq: 2 Aug 2019 19:35

Instrument :

MSVOA_D

ClientSampleId :

1S-F2-(30)


Tot Ion:113 Resp: 81775

Ion Ratio Lower Upper

113 100

111 92.9 83.2 124.8




192 15.5 11.8 17.8

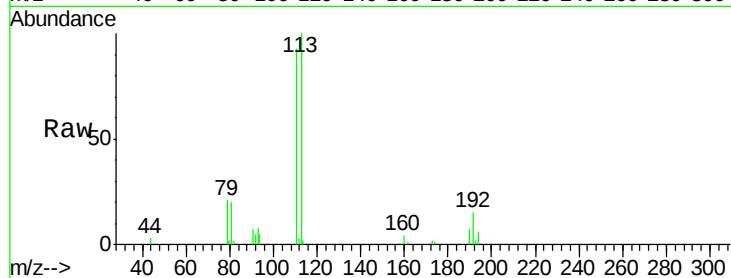

Abundance Ion 112.90 (112.60 to 113.60): V

Ion 110.90 (110.60 to 111.60): V

Ion 191.80 (191.50 to 192.50): V

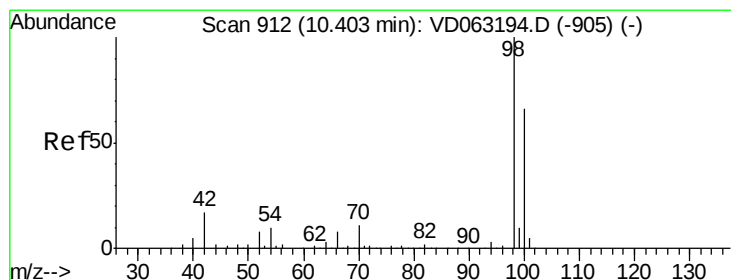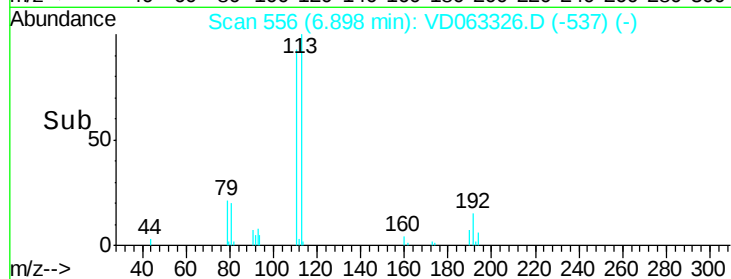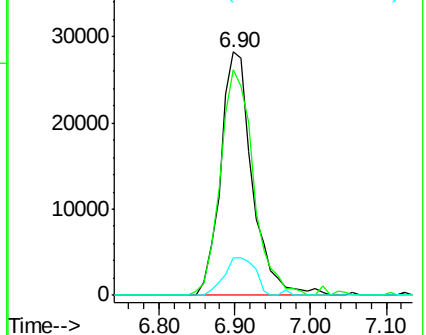

#50

Toluene-d8

Concen: 41.091 ug/l

RT: 10.39 min Scan# 911

Delta R.T. -0.01 min

Lab File: VD063326.D


Acq: 2 Aug 2019 19:35

Tgt Ion: 98 Resp: 143472

Ion Ratio Lower Upper



98 100


100 72.5 53.2 79.8

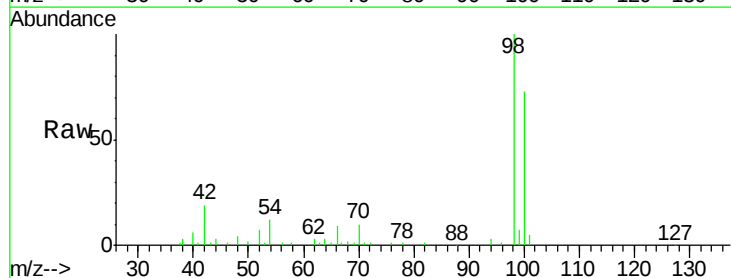

Abundance Ion 98.05 (97.75 to 98.75): V

Ion 100.05 (99.75 to 100.75): V

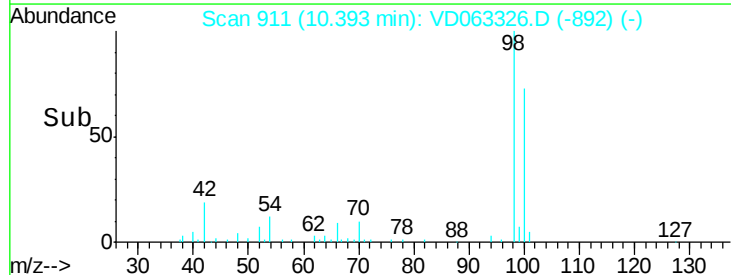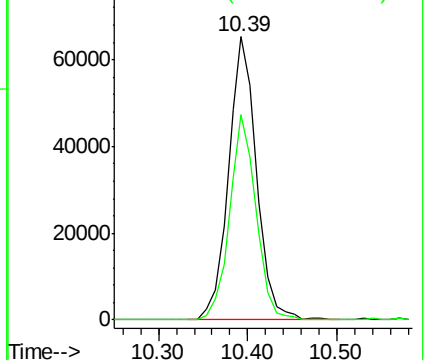

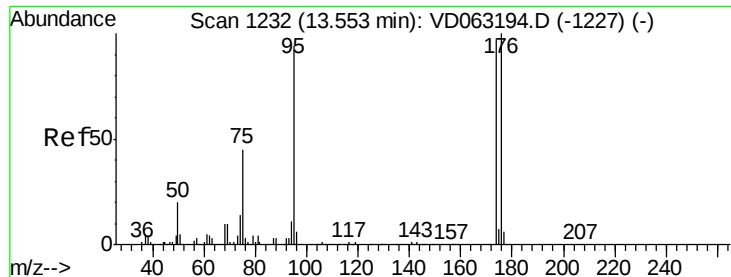

#62

4-Bromofluorobenzene

Concen: 46.325 ug/l

RT: 13.54 min Scan# 1231

Delta R.T. -0.01 min

Lab File: VD063326.D

Acq: 2 Aug 2019 19:35

Instrument :

MSVOA_D

ClientSampleId :

1S-F2-(30)


Tot Ion: 95 Resp: 73706

Ion Ratio Lower Upper

95 100

174 82.8 0.0 205.4




176 77.4 0.0 211.8

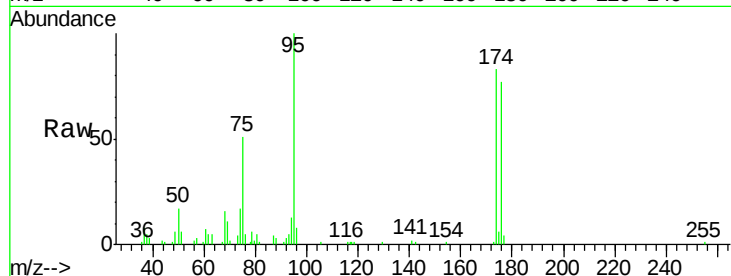

Abundance Ion 95.00 (94.70 to 95.70): VD

Ion 173.90 (173.60 to 174.60): V

Ion 175.90 (175.60 to 176.60): V

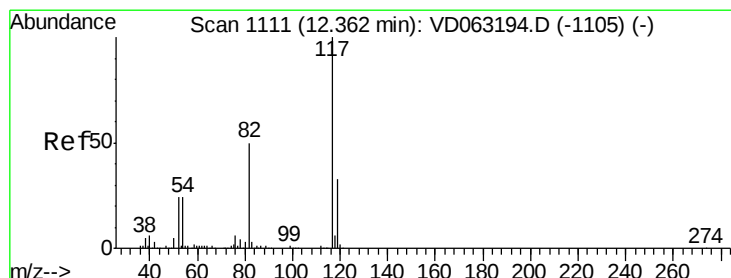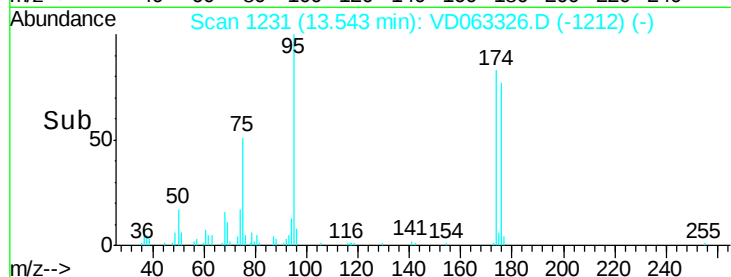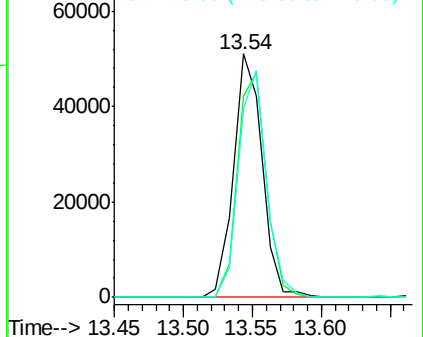

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 12.35 min Scan# 1110

Delta R.T. -0.01 min

Lab File: VD063326.D

Acq: 2 Aug 2019 19:35


Tgt Ion: 117 Resp: 173561

Ion Ratio Lower Upper

117 100

82 50.0 40.1 60.1



119 31.9 26.5 39.7

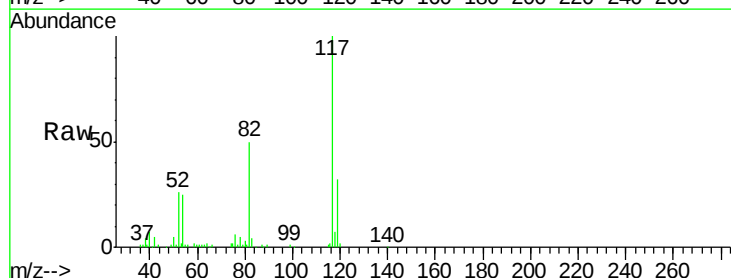


Abundance Ion 116.95 (116.65 to 117.65): V

Ion 82.05 (81.75 to 82.75): VD

Ion 118.95 (118.65 to 119.65): V

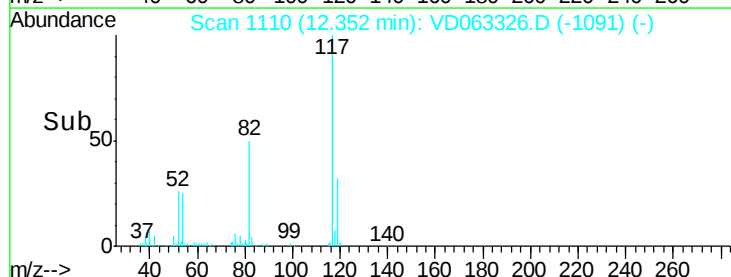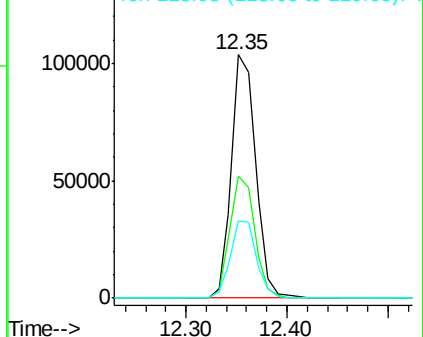

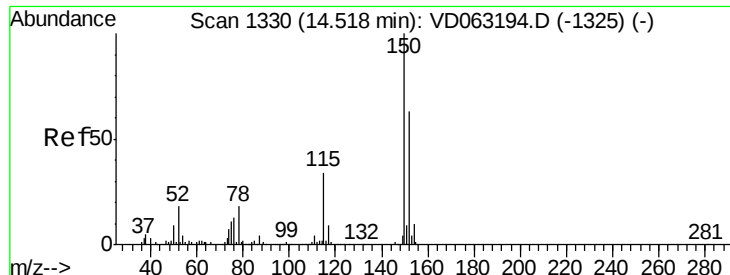

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 14.51 min Scan# 1329

Delta R.T. -0.01 min

Lab File: VD063326.D

Acq: 2 Aug 2019 19:35

Instrument :

MSVOA_D

ClientSampleId :

1S-F2-(30)


Tot Ion:152 Resp: 100286

Ion Ratio Lower Upper

152 100

115 58.5 27.5 82.4

150 161.8 0.0 320.6

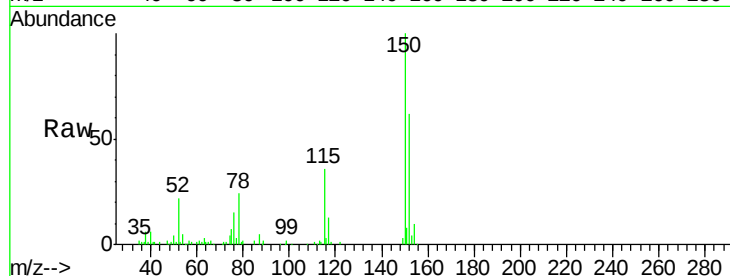

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 115.00 (114.70 to 115.70): V

Ion 149.90 (149.60 to 150.60): V

