


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD080219\
Data File : VD063306.D
Acq On : 2 Aug 2019 9:23
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D072919S.M
Title : SW846 8260
Last Update : Tue Jul 30 03:04:50 2019

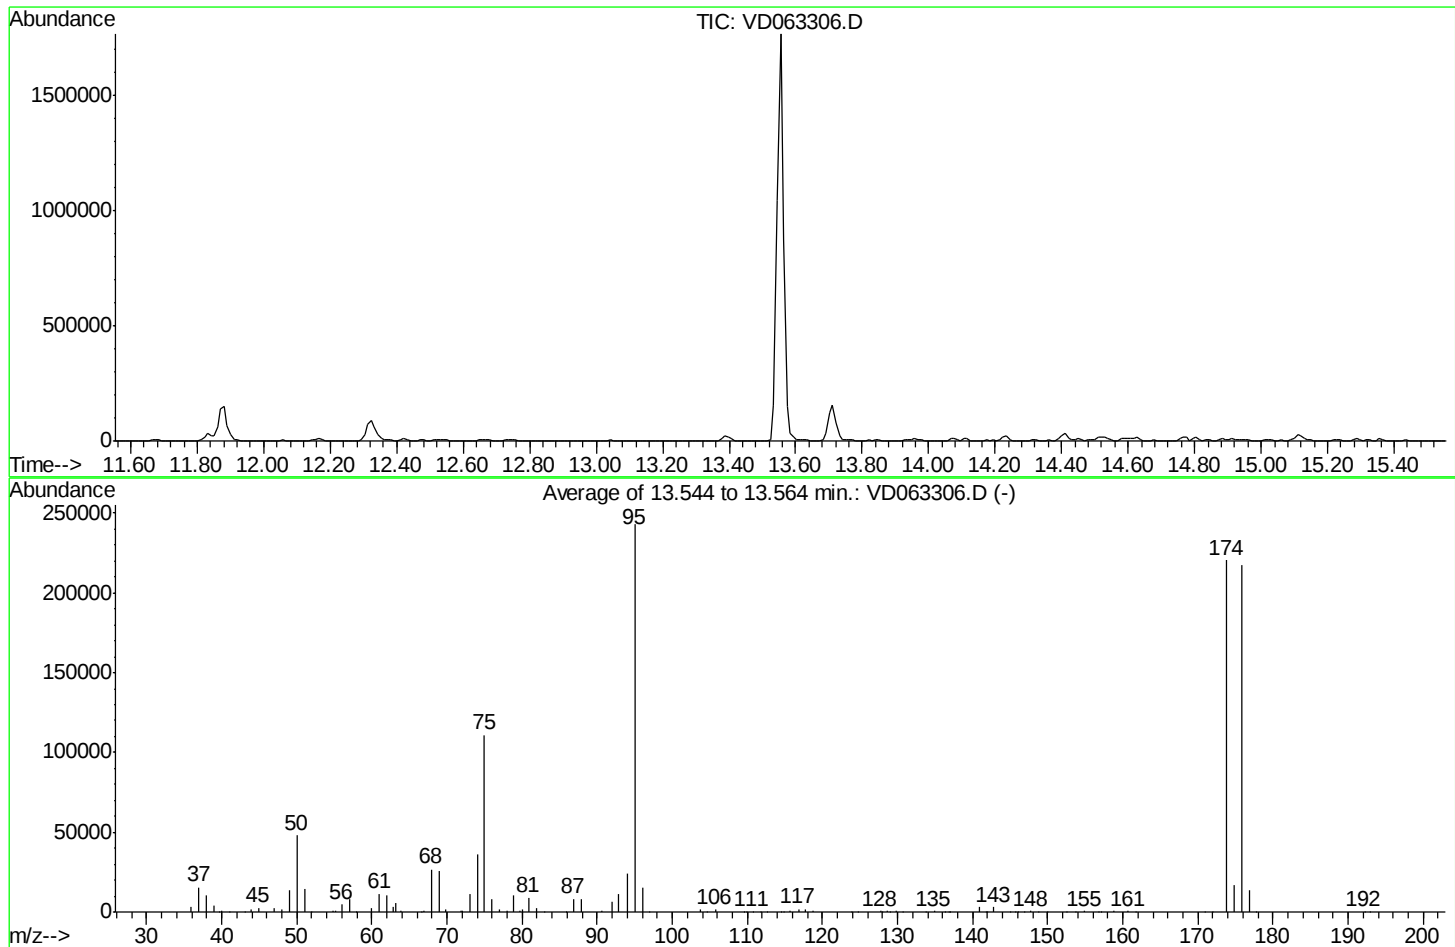

AutoFind: Scans 1231, 1232, 1233; Background Corrected with Scan 1226

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	48104	PASS
75	95	30	60	45.7	110933	PASS
95	95	100	100	100.0	242965	PASS
96	95	5	9	6.4	15548	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	90.7	220258	PASS
175	174	5	9	7.5	16480	PASS
176	174	95	101	98.5	217045	PASS
177	176	5	9	6.2	13431	PASS