


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD080219\
 Data File : VD063330.D
 Acq On : 2 Aug 2019 21:51
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D072919S.M
 Title : SW846 8260
 Last Update : Tue Jul 30 03:04:50 2019

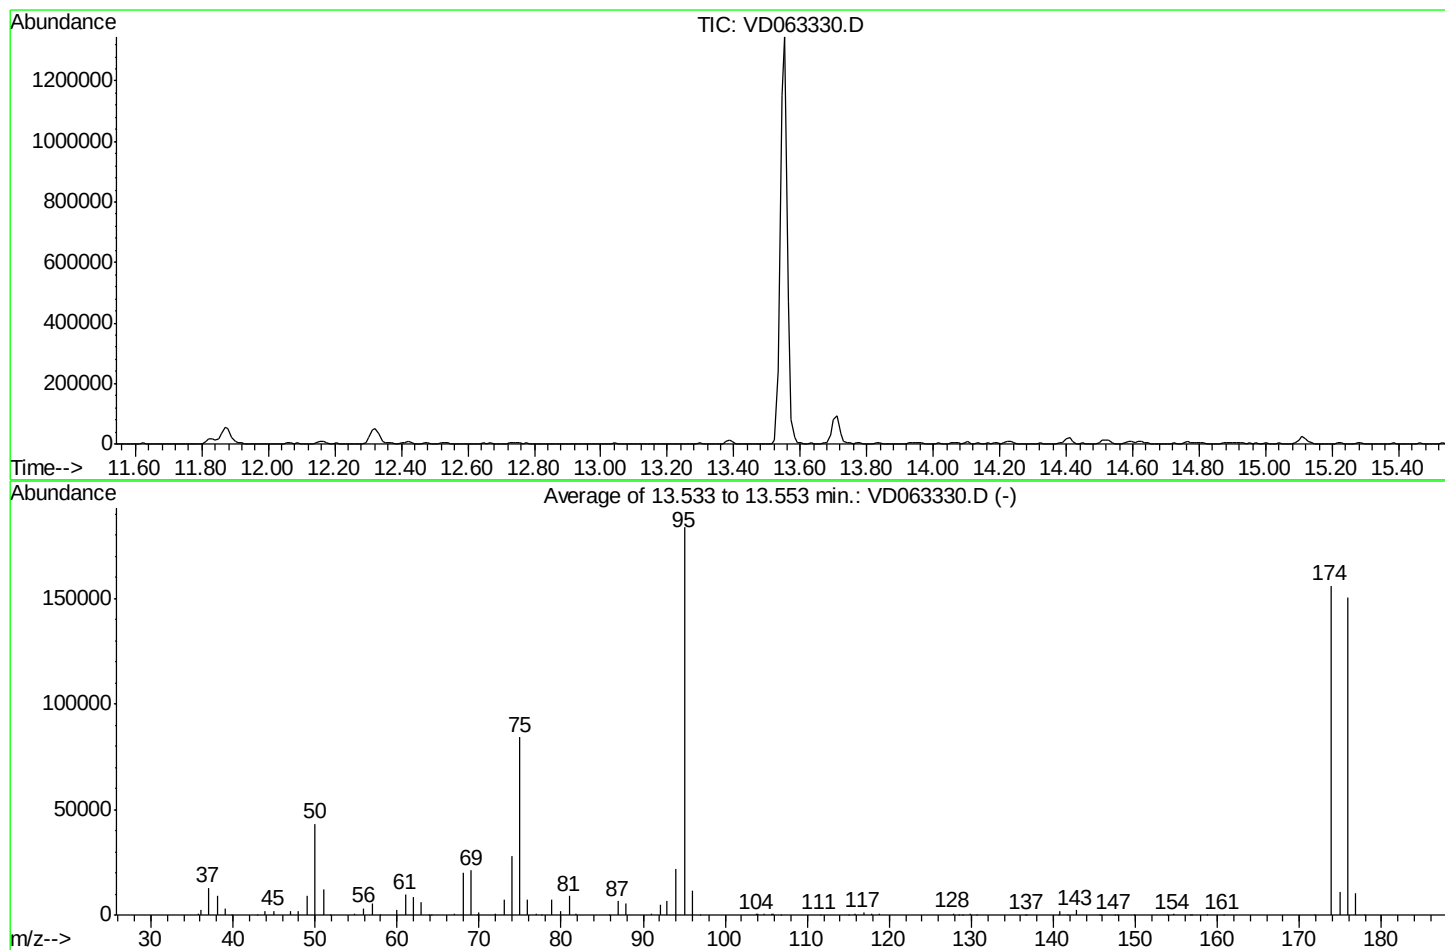

AutoFind: Scans 1230, 1231, 1232; Background Corrected with Scan 1226

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.6	43344	PASS
75	95	30	60	45.9	84365	PASS
95	95	100	100	100.0	183816	PASS
96	95	5	9	6.2	11439	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	84.9	156002	PASS
175	174	5	9	7.1	11116	PASS
176	174	95	101	96.4	150418	PASS
177	176	5	9	6.8	10263	PASS