
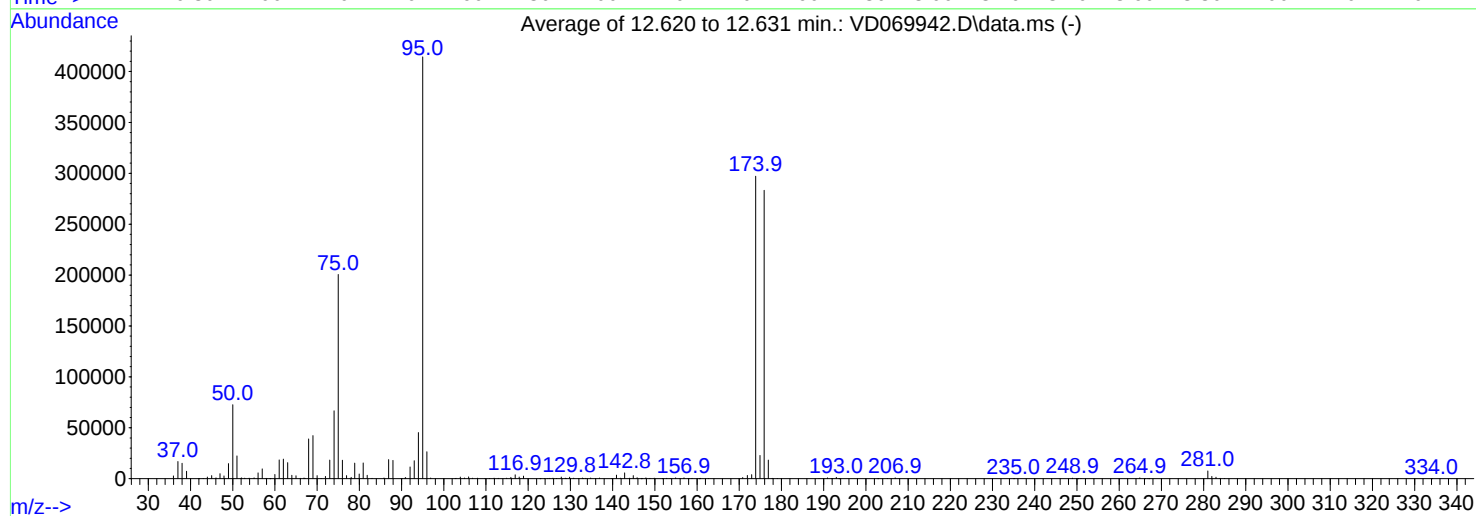


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080221\
 Data File : VD069942.D
 Acq On : 02 Aug 2021 08:22
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D072221S.M
 Title : SW846 8260
 Last Update : Fri Jul 23 04:51:13 2021

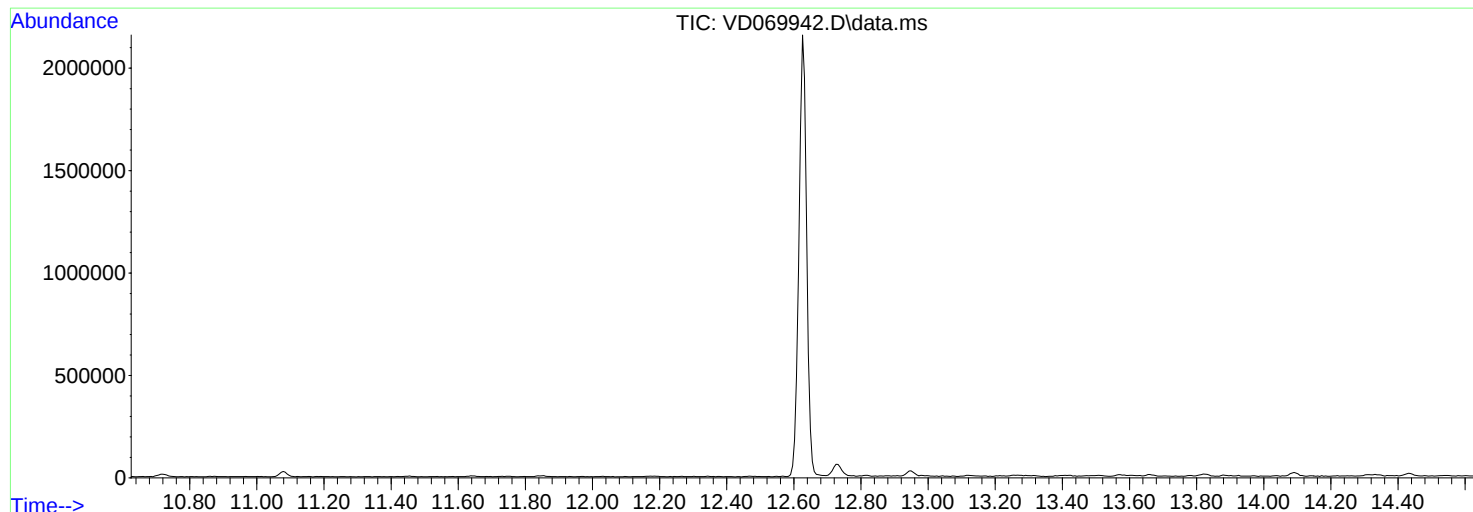

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	72579	PASS
75	95	30	60	48.4	200512	PASS
95	95	100	100	100.0	414400	PASS
96	95	5	9	6.4	26440	PASS
173	174	0.00	2	1.3	4006	PASS
174	95	50	100	71.7	297152	PASS
175	174	5	9	7.7	22803	PASS
176	174	95	101	95.3	283243	PASS
177	176	5	9	6.5	18317	PASS