

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080222\
 Data File : VD073925.D
 Acq On : 02 Aug 2022 14:28
 Operator : VA/SY
 Sample : N3996-01
 Misc : 5.33G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 MH-CS

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D080122S.M
 Title : SW846 8260

Signal : TIC: VD073925.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.073	24	26	31	rBV3	818	1512	1.45%	0.223%
2	2.215	45	50	52	rBV2	3399	4909	4.72%	0.725%
3	2.256	54	57	58	rVV3	1697	1929	1.85%	0.285%
4	2.315	63	67	69	rVV3	2663	4588	4.41%	0.678%
5	2.338	69	71	72	rVV	2463	2378	2.29%	0.351%
6	2.368	74	76	80	rVV2	3184	4370	4.20%	0.646%
7	2.403	80	82	83	rVV2	1863	1639	1.58%	0.242%
8	2.421	83	85	88	rVB2	1435	1512	1.45%	0.223%
9	2.485	94	96	97	rBV2	1820	1176	1.13%	0.174%
10	2.603	114	116	117	rVV2	1877	1269	1.22%	0.188%
11	2.626	118	120	122	rVV3	2329	2772	2.66%	0.410%
12	2.644	122	123	125	rVV	3370	2000	1.92%	0.296%
13	2.662	125	126	129	rVB2	2673	1771	1.70%	0.262%
14	2.691	129	131	132	rBV2	1924	1185	1.14%	0.175%
15	2.726	135	137	139	rBV2	1549	1296	1.25%	0.192%
16	2.773	142	145	147	rBV2	2995	3184	3.06%	0.471%
17	3.762	309	313	314	rBV2	928	1086	1.04%	0.160%
18	4.926	508	511	512	rVV2	1555	1241	1.19%	0.183%
19	4.962	512	517	523	rVB3	2522	5789	5.56%	0.855%
20	7.061	871	874	879	rVB2	944	1340	1.29%	0.198%
21	7.161	889	891	892	rBV	1570	1176	1.13%	0.174%
22	7.191	892	896	900	rVB2	2649	5088	4.89%	0.752%
23	7.903	1009	1017	1024	rBV2	18148	44205	42.48%	6.532%
24	7.967	1024	1028	1038	rVB2	20488	42739	41.07%	6.316%
25	8.326	1080	1089	1097	rVB2	18553	43050	41.37%	6.362%
26	8.855	1169	1179	1190	rVB2	35937	73414	70.55%	10.849%
27	10.332	1422	1430	1439	rVB	58173	103053	99.03%	15.228%
28	10.502	1456	1459	1463	rVB2	1454	1975	1.90%	0.292%
29	10.773	1504	1505	1511	rVB2	910	1123	1.08%	0.166%
30	11.067	1551	1555	1558	rBV3	1365	1474	1.42%	0.218%
31	11.632	1644	1651	1660	rVB	60588	104060	100.00%	15.377%
32	12.620	1812	1819	1825	rVB	46303	76708	73.72%	11.335%
33	12.944	1871	1874	1877	rVB2	1022	1360	1.31%	0.201%
34	13.561	1971	1979	1986	rVB	62611	102937	98.92%	15.211%
35	13.708	1999	2004	2007	rBV3	662	1154	1.11%	0.171%
36	13.785	2014	2017	2020	rBV3	938	1260	1.21%	0.186%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080222\
 Data File : VD073925.D
 Acq On : 02 Aug 2022 14:28
 Operator : VA/SY
 Sample : N3996-01
 Misc : 5.33G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 MH-CS

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D080122S.M
 Title : SW846 8260

37	13.938	2038	2043	2045	rBV	977	1365	1.31%	0.202%
38	14.508	2136	2140	2142	rBV2	1105	1435	1.38%	0.212%
39	14.885	2200	2204	2206	rBV3	1279	1279	1.23%	0.189%
40	14.949	2212	2215	2217	rBV2	1688	1196	1.15%	0.177%
41	15.043	2226	2231	2232	rBV2	1143	1230	1.18%	0.182%
42	15.155	2247	2250	2253	rVB2	1273	1605	1.54%	0.237%
43	15.414	2292	2294	2296	rBV	1326	1231	1.18%	0.182%
44	15.502	2306	2309	2310	rVB2	1436	1139	1.09%	0.168%
45	15.543	2313	2316	2318	rBV	1175	1121	1.08%	0.166%
46	15.579	2320	2322	2325	rVV3	956	1274	1.22%	0.188%
47	15.879	2370	2373	2375	rBV2	843	1084	1.04%	0.160%
48	15.926	2379	2381	2387	rVB2	894	1373	1.32%	0.203%
49	16.026	2394	2398	2400	rVB2	1092	1536	1.48%	0.227%
50	16.255	2434	2437	2439	rBV2	1756	1619	1.56%	0.239%
51	16.337	2449	2451	2453	rBV2	1415	1159	1.11%	0.171%
52	16.414	2461	2464	2466	rBV2	2083	2349	2.26%	0.347%
53	16.467	2472	2473	2476	rBV3	1681	1215	1.17%	0.180%
54	16.596	2493	2495	2499	rBV3	1387	1780	1.71%	0.263%




Sum of corrected areas: 676712

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080222\
Data File : VD073925.D
Acq On : 02 Aug 2022 14:28
Operator : VA/SY
Sample : N3996-01
Misc : 5.33G/5.00ml/MSVOA_D/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
MH-CS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D080122S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

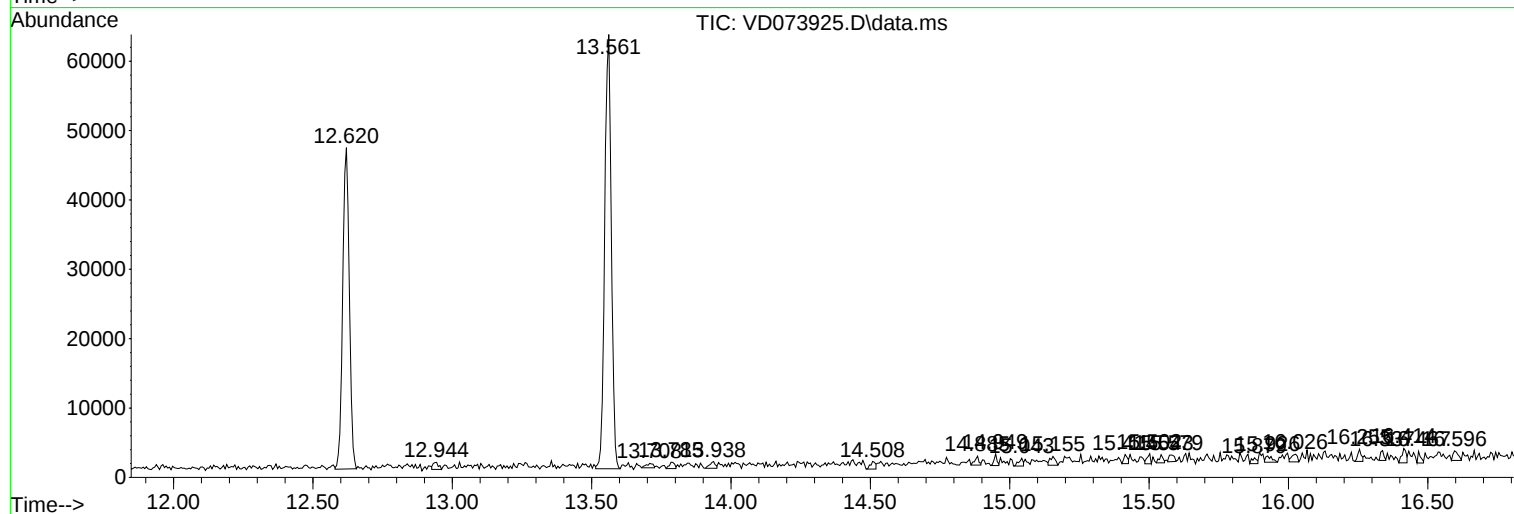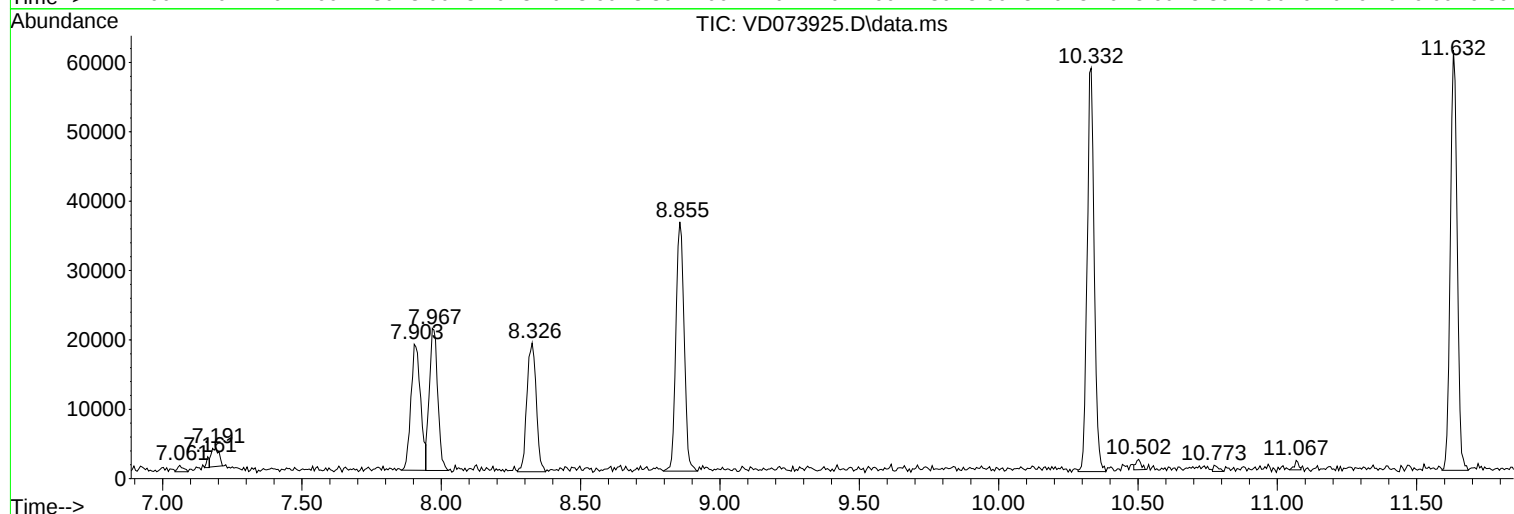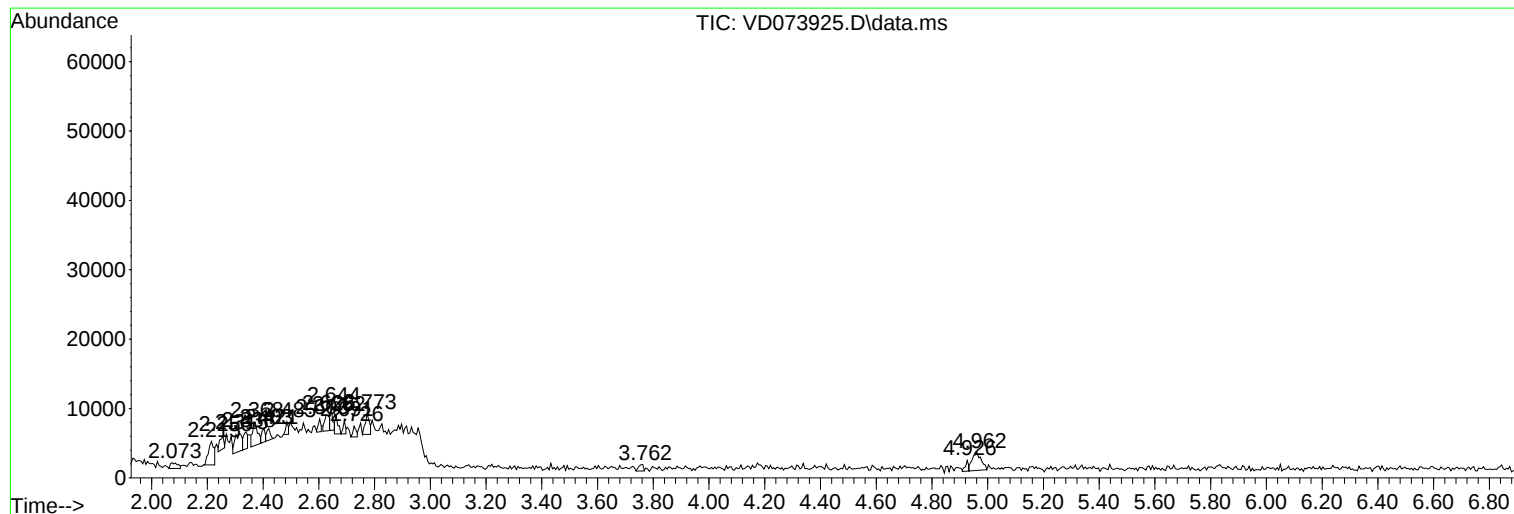

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080222\
Data File : VD073925.D
Acq On : 02 Aug 2022 14:28
Operator : VA/SY
Sample : N3996-01
Misc : 5.33G/5.00ml/MSVOA_D/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
MH-CS










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D080122S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 unknown2.368 Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.368	5.11 ug/l	4370	Pentafluorobenzene	7.973

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrazolo[1,5-a]pyrimidine, 5,7-...	149	C6H7N5	003210-44-4	17
2			N-Acrylonitril-2,2-dimethylaziri...	122	C7H10N2	077376-91-1	9
3			Dipropargyl sulfide	110	C6H6S	013702-09-5	9
4			3-Methyl-4-nitro-5-(1-pyrazolyl)...	193	C7H7N5O2	292855-42-6	9
5			1H-Pyrazole-5-carboxylic acid, 3...	171	C5H5N3O4	1000318-77-7	9

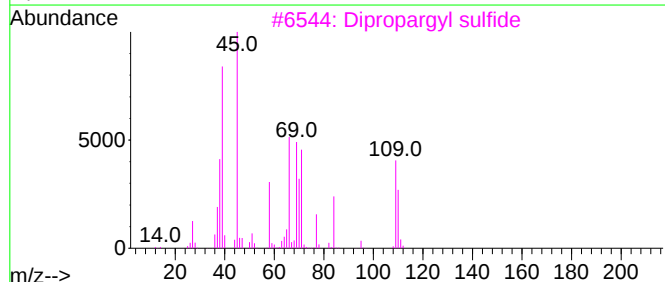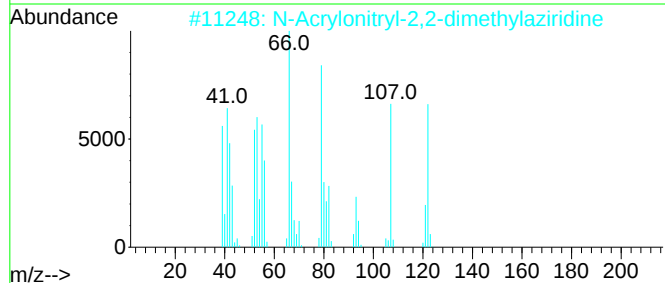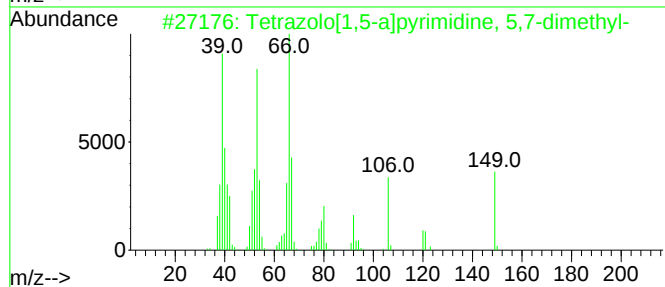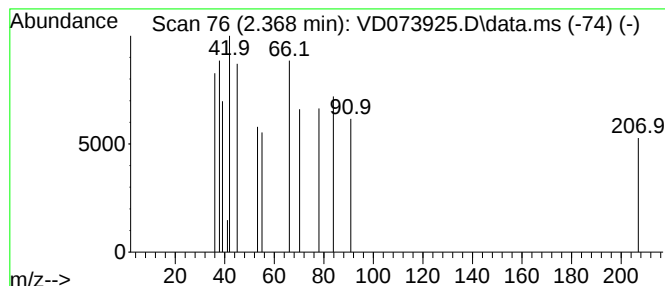

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080222\
Data File : VD073925.D
Acq On : 02 Aug 2022 14:28
Operator : VA/SY
Sample : N3996-01
Misc : 5.33G/5.00ml/MSVOA_D/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
MH-CS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D080122S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown2.368	2.368	5.1	ug/l	4370	1	7.973	42739	50.0