
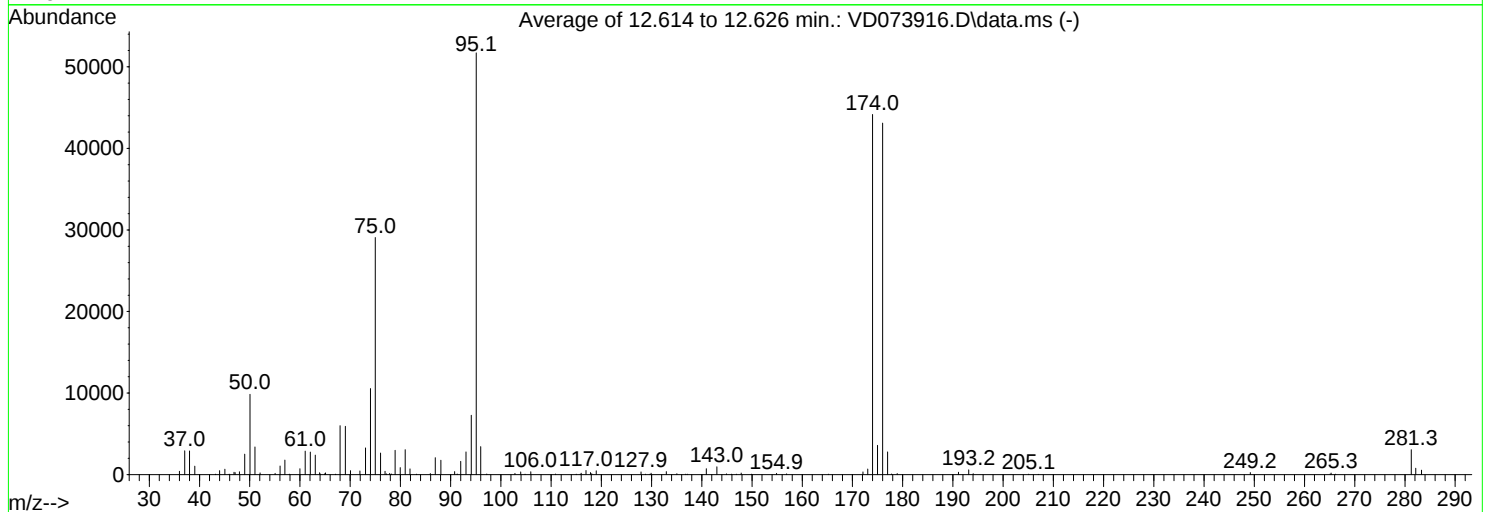


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD080222\  
Data File : VD073916.D  
Acq On : 02 Aug 2022 08:55  
Operator : VA/SY  
Sample : BFB  
Misc : 5.00G/5.00ml/MSVOA\_D/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D080122S.M  
Title : SW846 8260  
Last Update : Tue Aug 02 05:13:57 2022

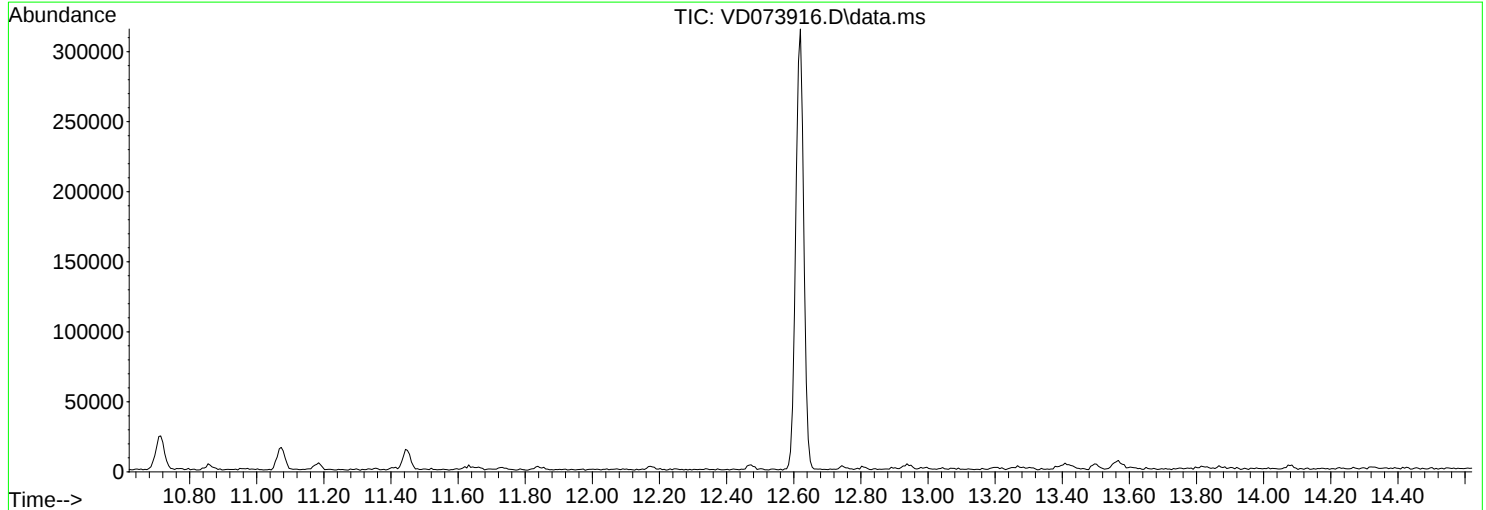

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1809

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 19.1  | 9857  | PASS      |
| 75     | 95      | 30     | 60     | 56.2  | 29075 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 51712 | PASS      |
| 96     | 95      | 5      | 9      | 6.7   | 3439  | PASS      |
| 173    | 174     | 0.00   | 2      | 1.6   | 693   | PASS      |
| 174    | 95      | 50     | 100    | 85.4  | 44165 | PASS      |
| 175    | 174     | 5      | 9      | 8.1   | 3591  | PASS      |
| 176    | 174     | 95     | 101    | 97.6  | 43104 | PASS      |
| 177    | 176     | 5      | 9      | 6.4   | 2778  | PASS      |