

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080223\
 Data File : VD076904.D
 Acq On : 02 Aug 2023 18:06
 Operator : KP/SY
 Sample : 03886-01
 Misc : 5.01G/5.0ml/MSVOA_D/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 500-1A-1B

Quant Time: Aug 03 01:25:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D071423S.M
 Quant Title : SW846 8260
 QLast Update : Mon Jul 17 08:07:52 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.875	168	155158	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.775	114	307084	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	294287	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	126305	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	82993	53.703	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	107.400%
35) Dibromofluoromethane	7.804	113	99681	51.655	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	103.320%
50) Toluene-d8	10.269	98	385615	55.859	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	111.720%
62) 4-Bromofluorobenzene	12.569	95	109317	48.950	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	97.900%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080223\
Data File : VD076904.D
Acq On : 02 Aug 2023 18:06
Operator : KP/SY
Sample : 03886-01
Misc : 5.01G/5.0ml/MSVOA_D/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
500-1A-1B

Quant Time: Aug 03 01:25:36 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D071423S.M
Quant Title : SW846 8260
QLast Update : Mon Jul 17 08:07:52 2023
Response via : Initial Calibration




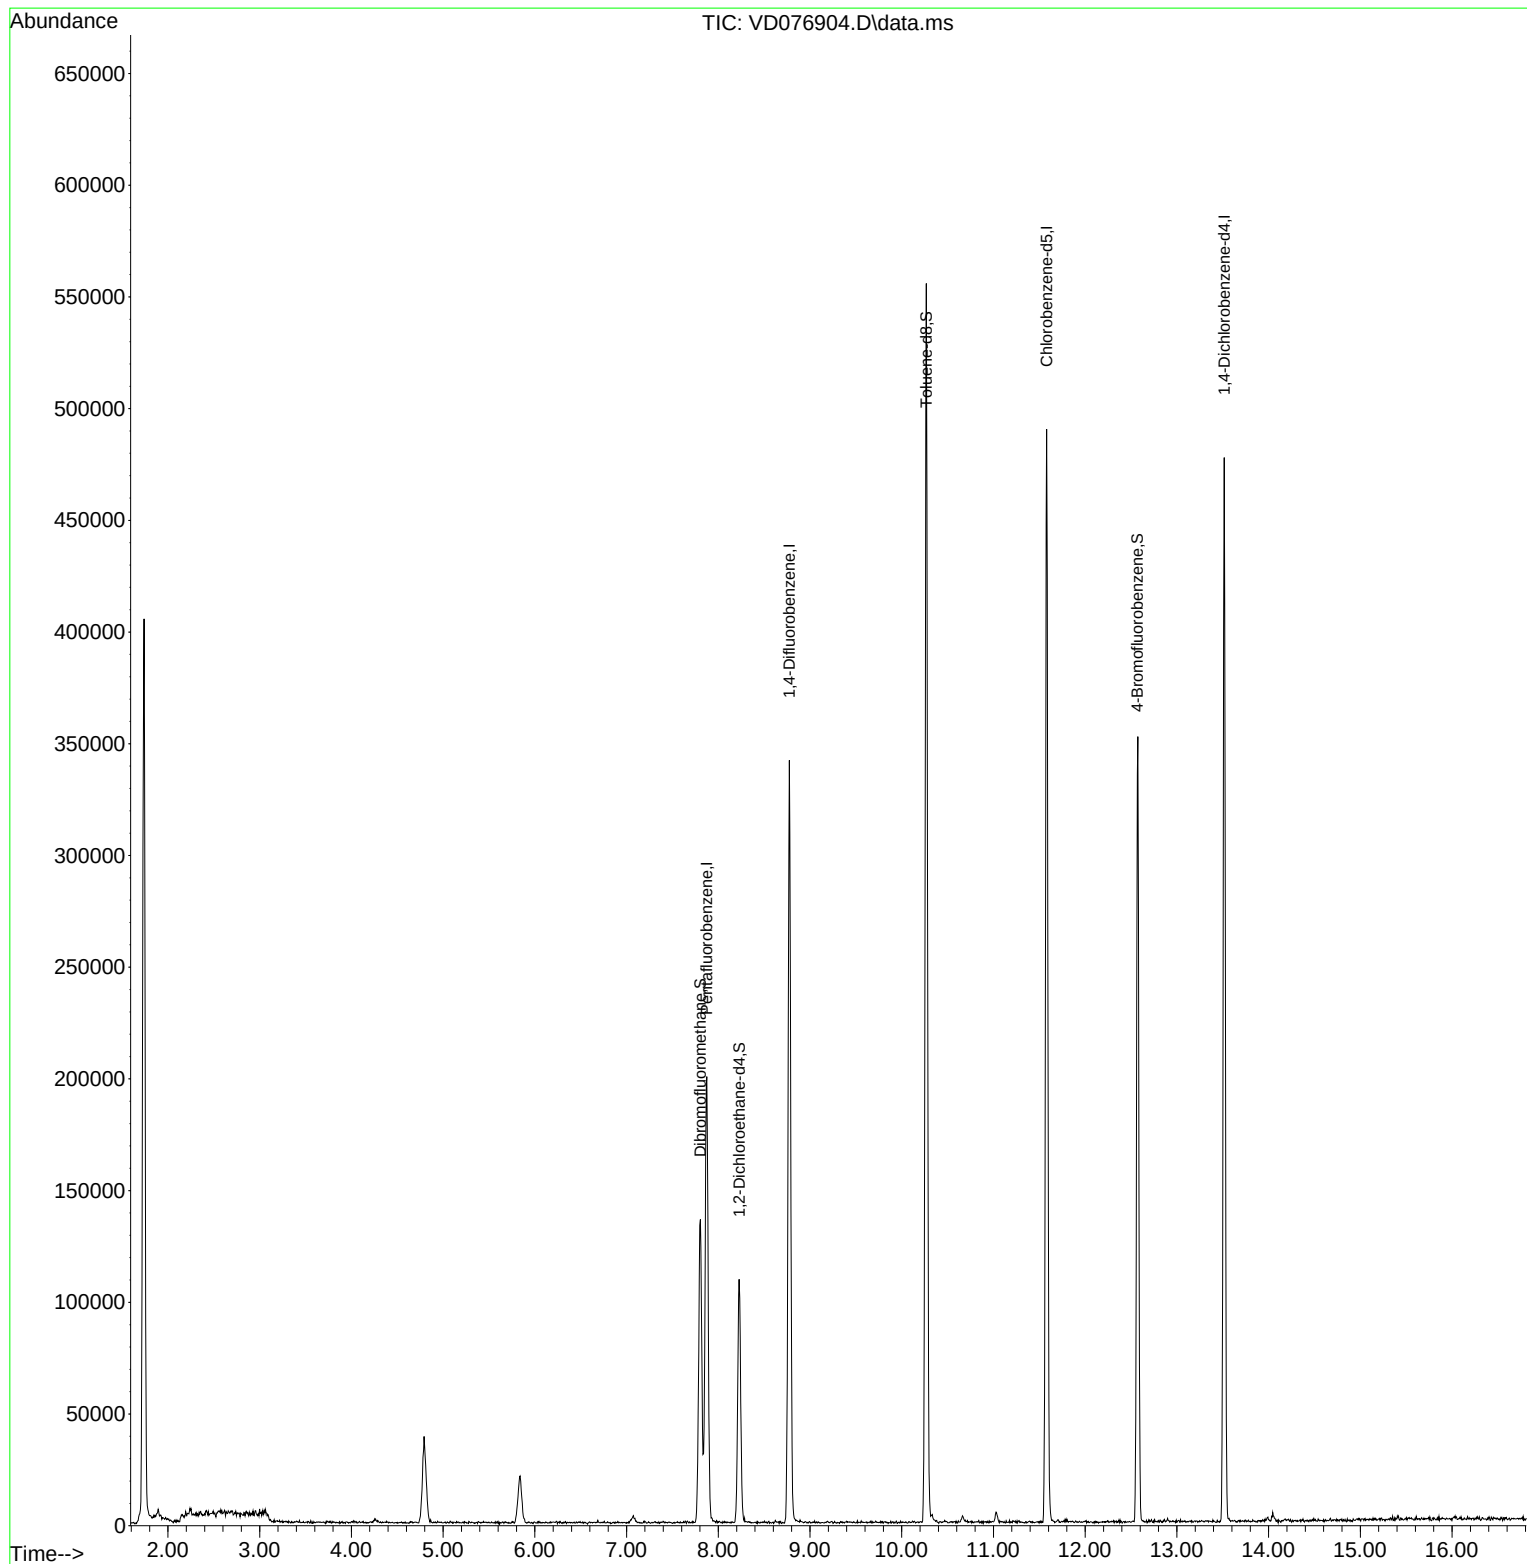


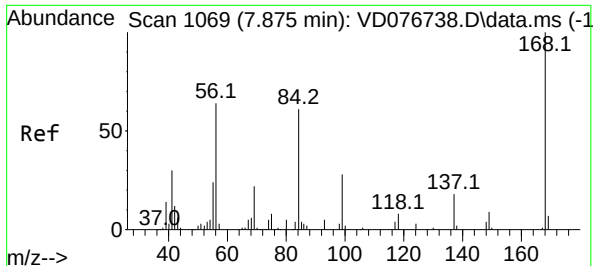

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1069
Delta R.T. -0.000 min
Lab File: VD076904.D
Acq: 02 Aug 2023 18:06




Instrument :
MSVOA_D
ClientSampleId :
500-1A-1B


Tgt Ion:168 Resp: 155158
Ion Ratio Lower Upper
168 100
99 55.1 36.7 55.1

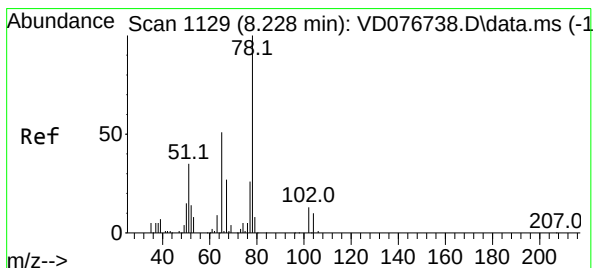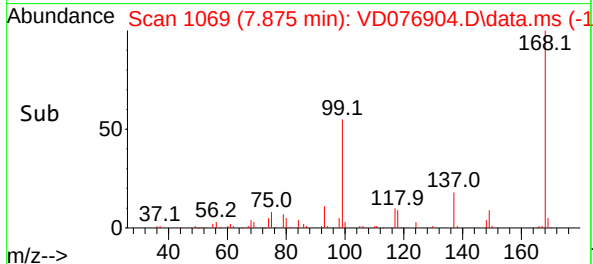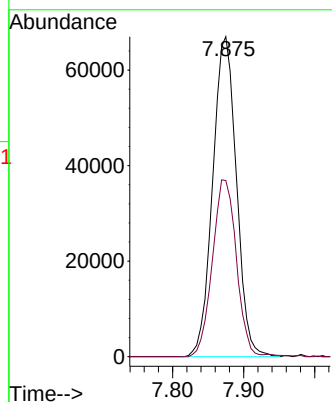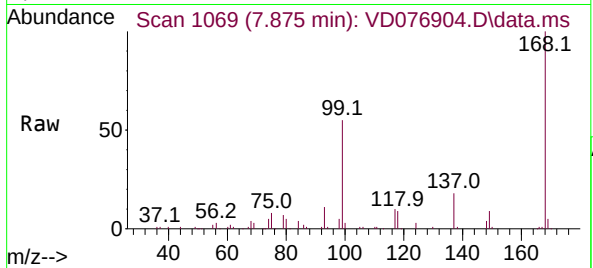

#33
1,2-Dichloroethane-d4
Concen: 53.703 ug/l
RT: 8.228 min Scan# 1129
Delta R.T. -0.000 min
Lab File: VD076904.D
Acq: 02 Aug 2023 18:06

Tgt Ion: 65 Resp: 82993
Ion Ratio Lower Upper
65 100
67 54.4 0.0 115.0

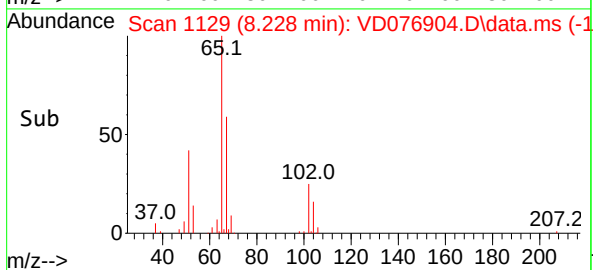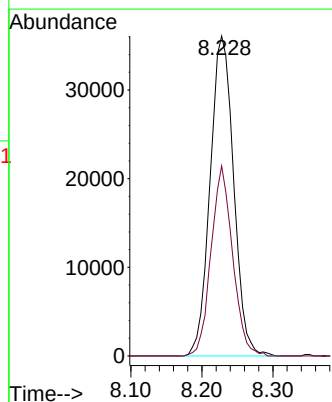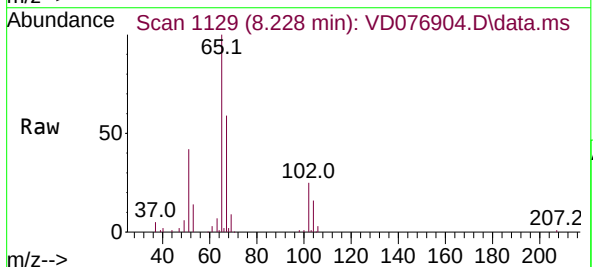

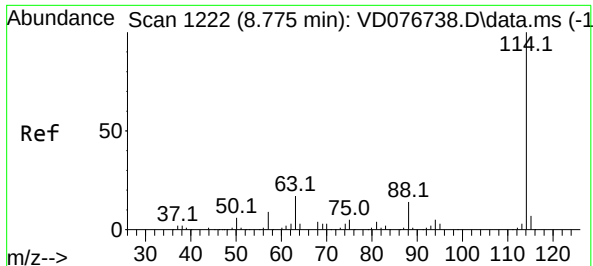

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.775 min Scan# 11

Delta R.T. -0.000 min

Lab File: VD076904.D

Acq: 02 Aug 2023 18:06

Instrument :

MSVOA_D

ClientSampleId :

500-1A-1B





Tgt Ion:114 Resp: 307084

Ion Ratio Lower Upper

114 100

63 17.8 0.0 33.4

88 13.8 0.0 26.2

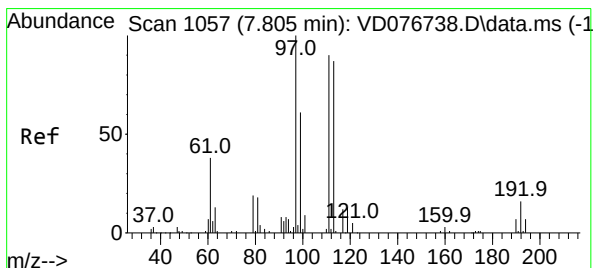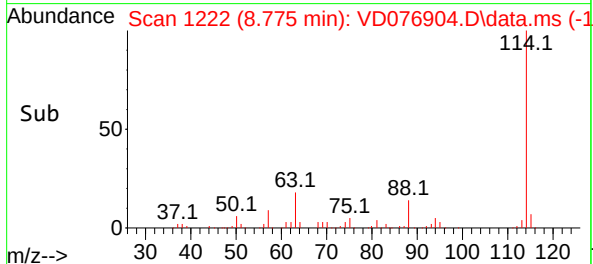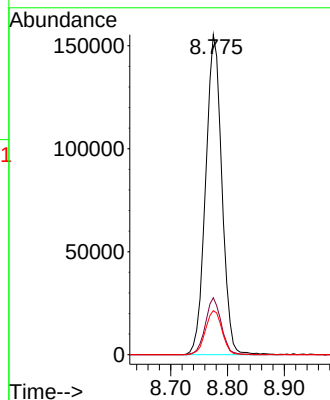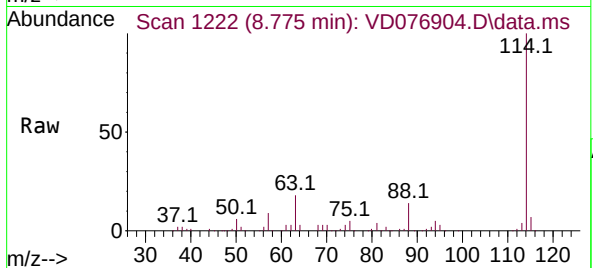

#35

Dibromofluoromethane

Concen: 51.655 ug/l

RT: 7.804 min Scan# 1057

Delta R.T. -0.001 min

Lab File: VD076904.D

Acq: 02 Aug 2023 18:06




Tgt Ion:113 Resp: 99681


Ion Ratio Lower Upper

113 100

111 103.5 84.7 127.1

192 18.2 16.8 25.2


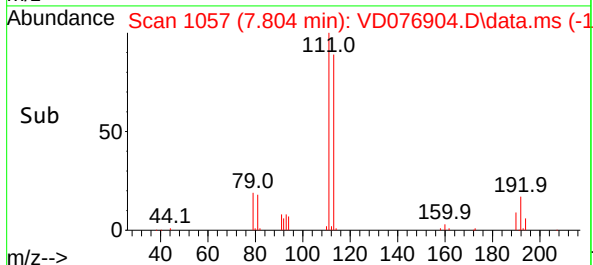
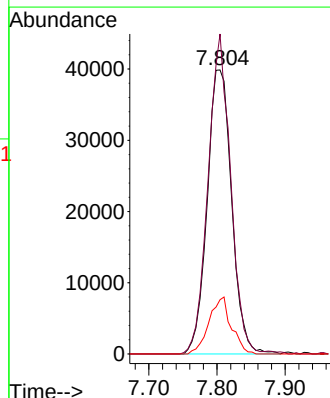
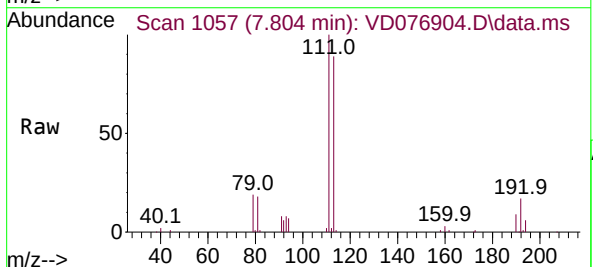


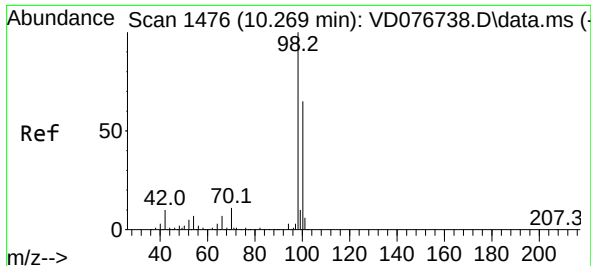

#50
Toluene-d8
Concen: 55.859 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. -0.000 min
Lab File: VD076904.D
Acq: 02 Aug 2023 18:06




Instrument :
MSVOA_D
ClientSampleId :
500-1A-1B


Tgt Ion: 98 Resp: 385615
Ion Ratio Lower Upper
98 100
100 64.3 50.3 75.5

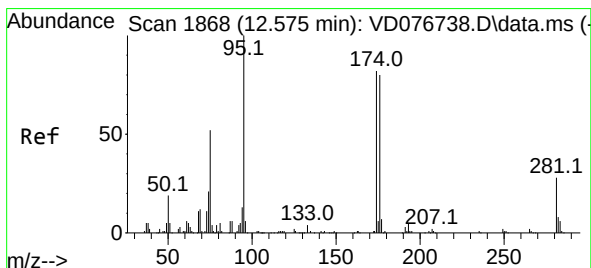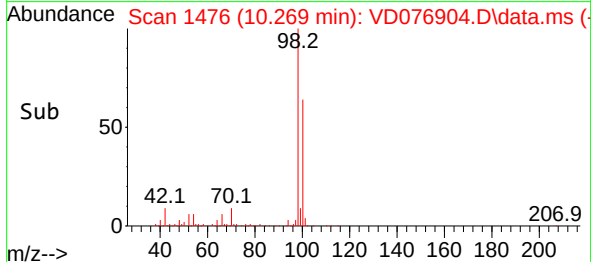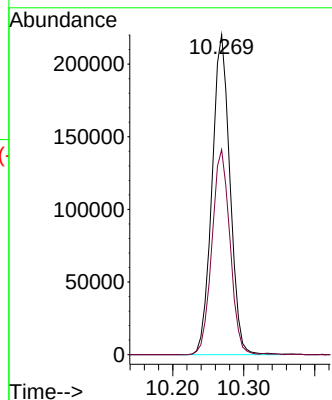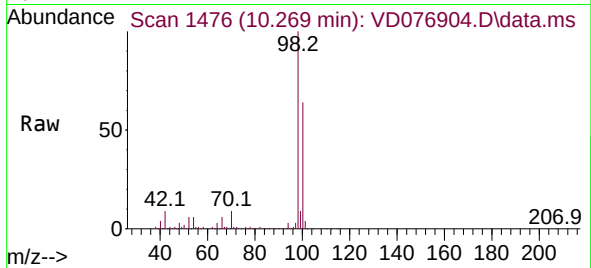

#62
4-Bromofluorobenzene
Concen: 48.950 ug/l
RT: 12.569 min Scan# 1867
Delta R.T. -0.006 min
Lab File: VD076904.D
Acq: 02 Aug 2023 18:06

Tgt Ion: 95 Resp: 109317
Ion Ratio Lower Upper
95 100
174 85.4 0.0 201.8
176 83.4 0.0 191.8


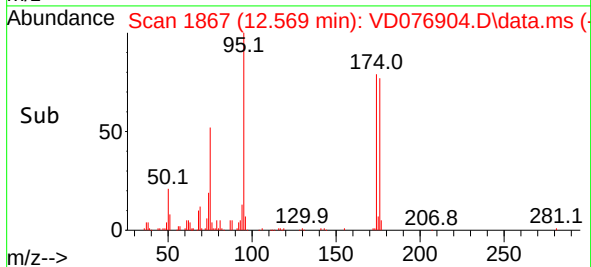
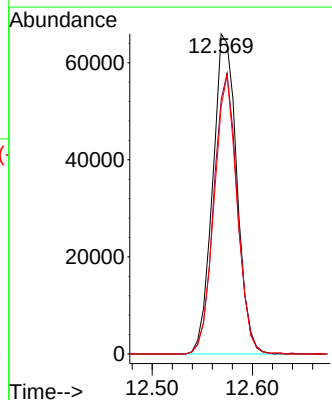
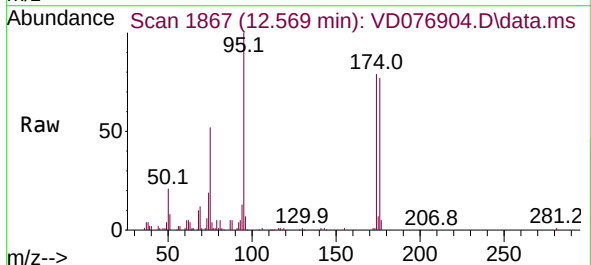


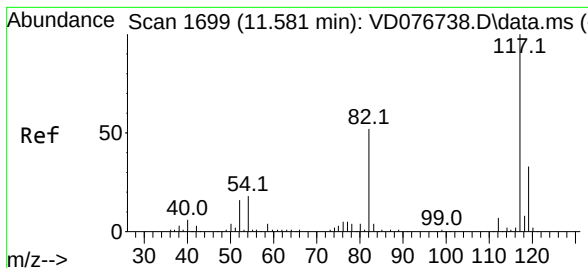

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 117
Delta R.T. -0.000 min
Lab File: VD076904.D
Acq: 02 Aug 2023 18:06

Instrument :
MSVOA_D
ClientSampleId :
500-1A-1B

Tgt Ion:117 Resp: 294287
Ion Ratio Lower Upper
117 100
82 53.3 38.3 57.5
119 33.6 25.0 37.4

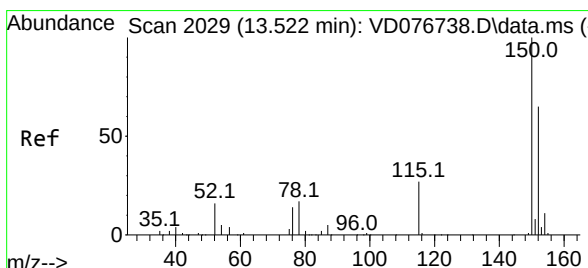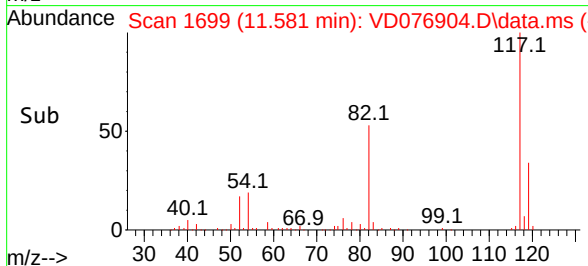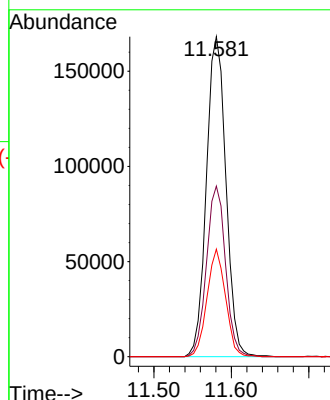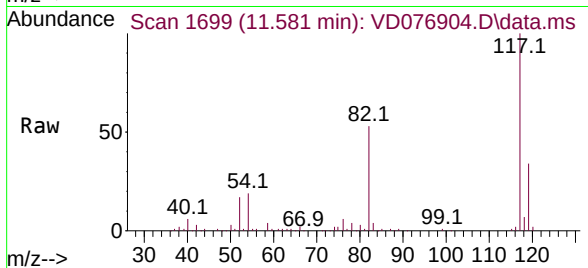

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. -0.006 min
Lab File: VD076904.D
Acq: 02 Aug 2023 18:06

Tgt Ion:152 Resp: 126305
Ion Ratio Lower Upper
152 100
115 57.5 27.1 81.3
150 154.0 0.0 353.6

