
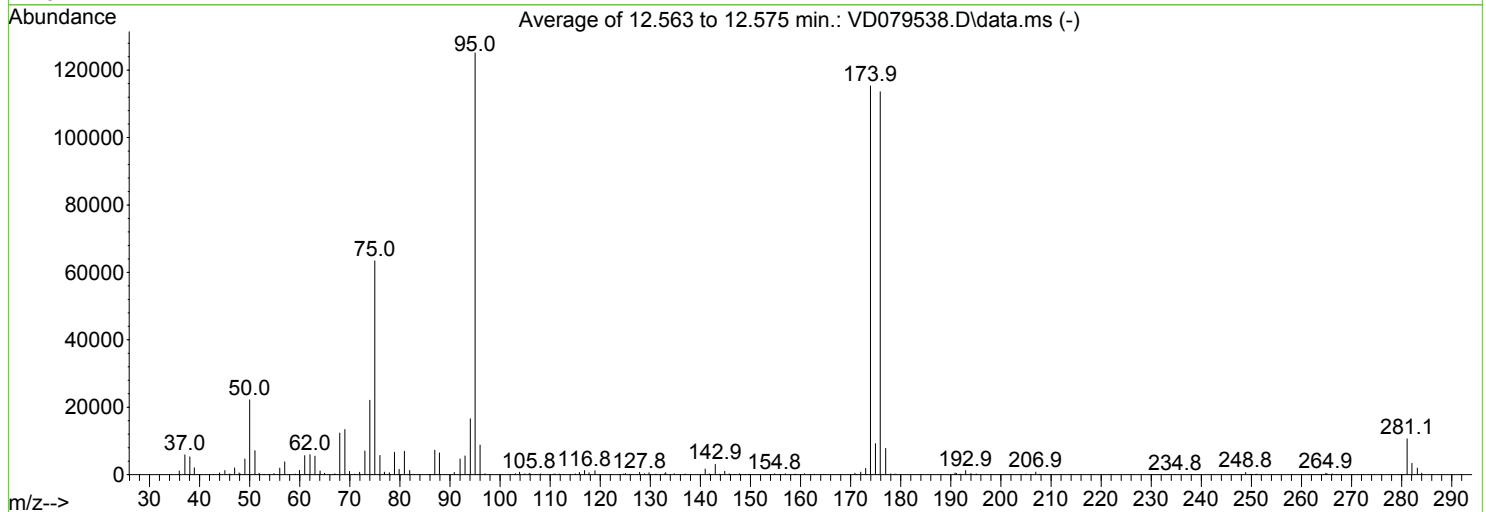


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080224\
Data File : VD079538.D
Acq On : 02 Aug 2024 10:13
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D072924S.M
Title : SW846 8260
Last Update : Tue Jul 30 03:50:47 2024

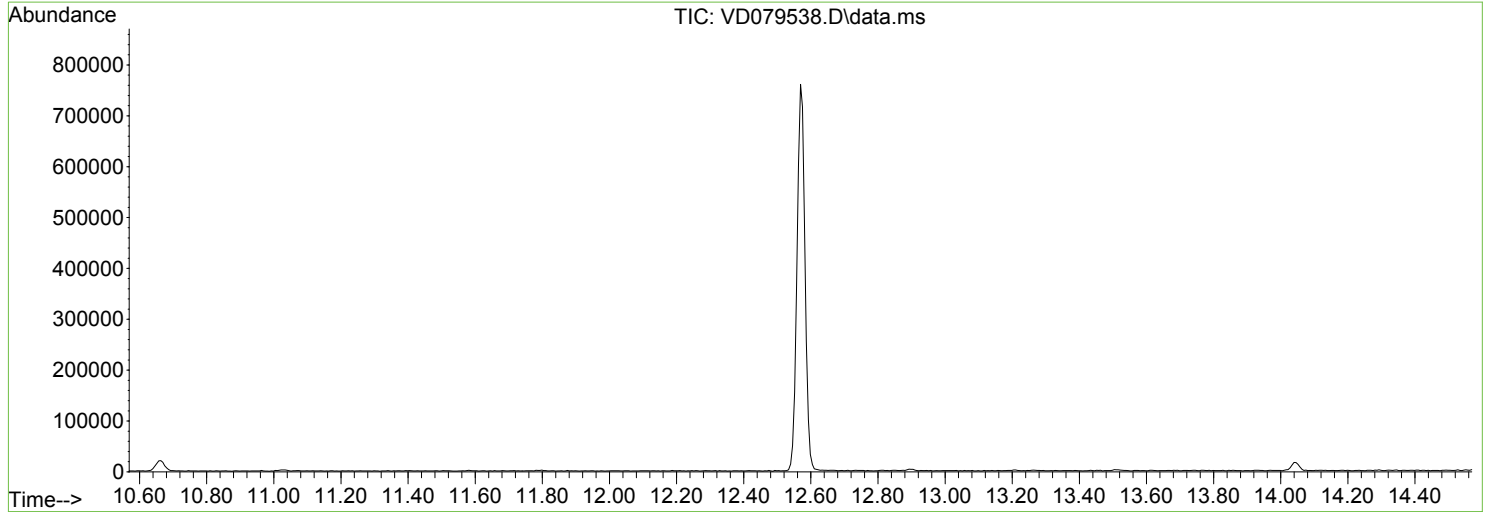

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1858

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.7	22205	PASS
75	95	30	60	50.7	63429	PASS
95	95	100	100	100.0	125144	PASS
96	95	5	9	7.0	8798	PASS
173	174	0.00	2	1.6	1844	PASS
174	95	50	100	92.1	115307	PASS
175	174	5	9	8.0	9232	PASS
176	174	95	101	98.5	113621	PASS
177	176	5	9	6.9	7811	PASS