
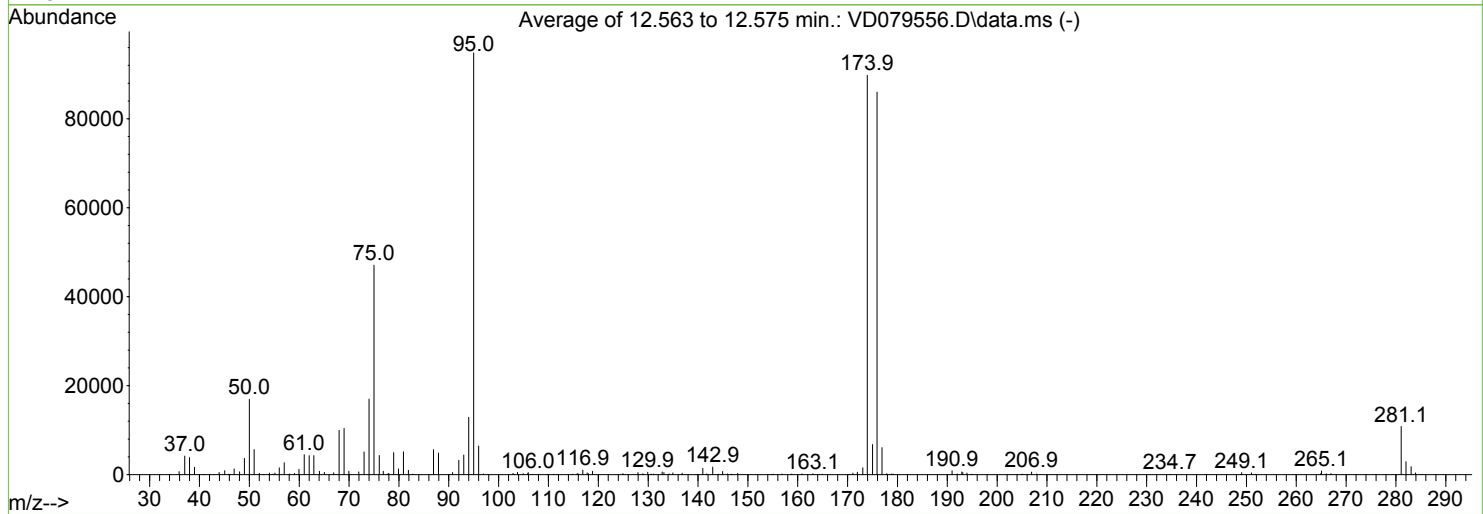


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080224\
Data File : VD079556.D
Acq On : 02 Aug 2024 22:07
Operator : RP/MD
Sample : BFB
Misc : 5.01G/5.0ml/MSVOA_D/SOIL/A
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D072924S.M
Title : SW846 8260
Last Update : Tue Jul 30 03:50:47 2024

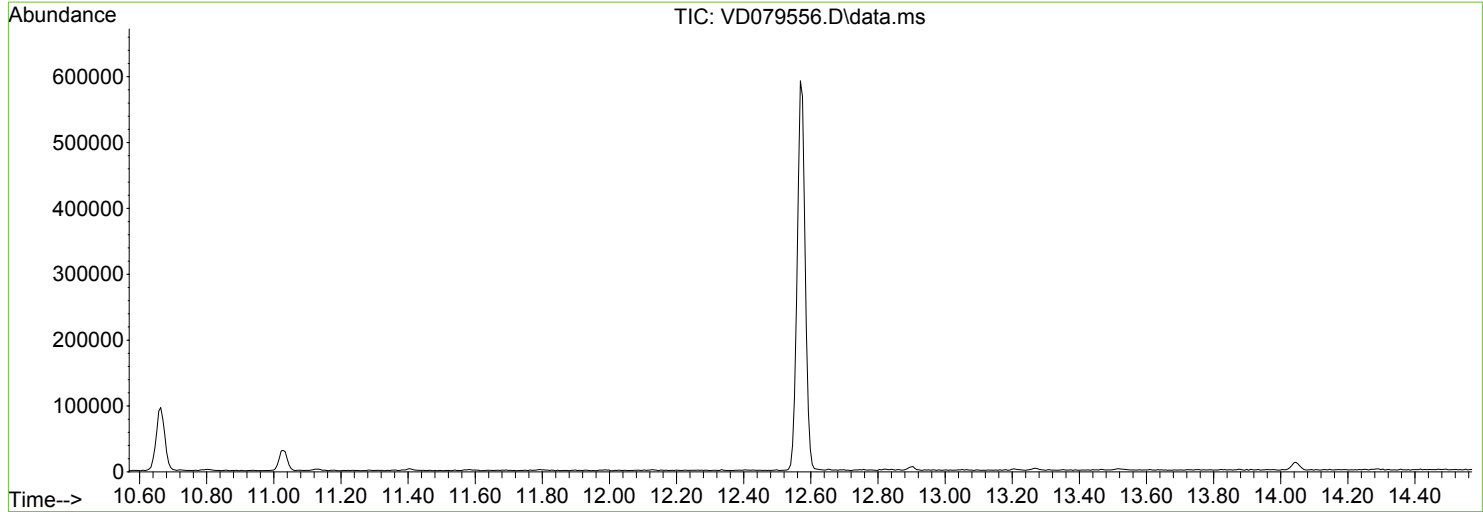

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1858

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.9	16936	PASS
75	95	30	60	49.6	47075	PASS
95	95	100	100	100.0	94829	PASS
96	95	5	9	6.8	6451	PASS
173	174	0.00	2	1.7	1554	PASS
174	95	50	100	94.7	89797	PASS
175	174	5	9	7.5	6759	PASS
176	174	95	101	95.8	86005	PASS
177	176	5	9	7.1	6071	PASS