


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD080319\  
Data File : VD063352.D  
Acq On : 3 Aug 2019 9:23  
Operator : VA/AP  
Sample : BFB  
Misc : 5.00µl/5ml/MSVOA D/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_D\METHOD\82D072919S.M  
Title : SW846 8260  
Last Update : Tue Jul 30 03:04:50 2019

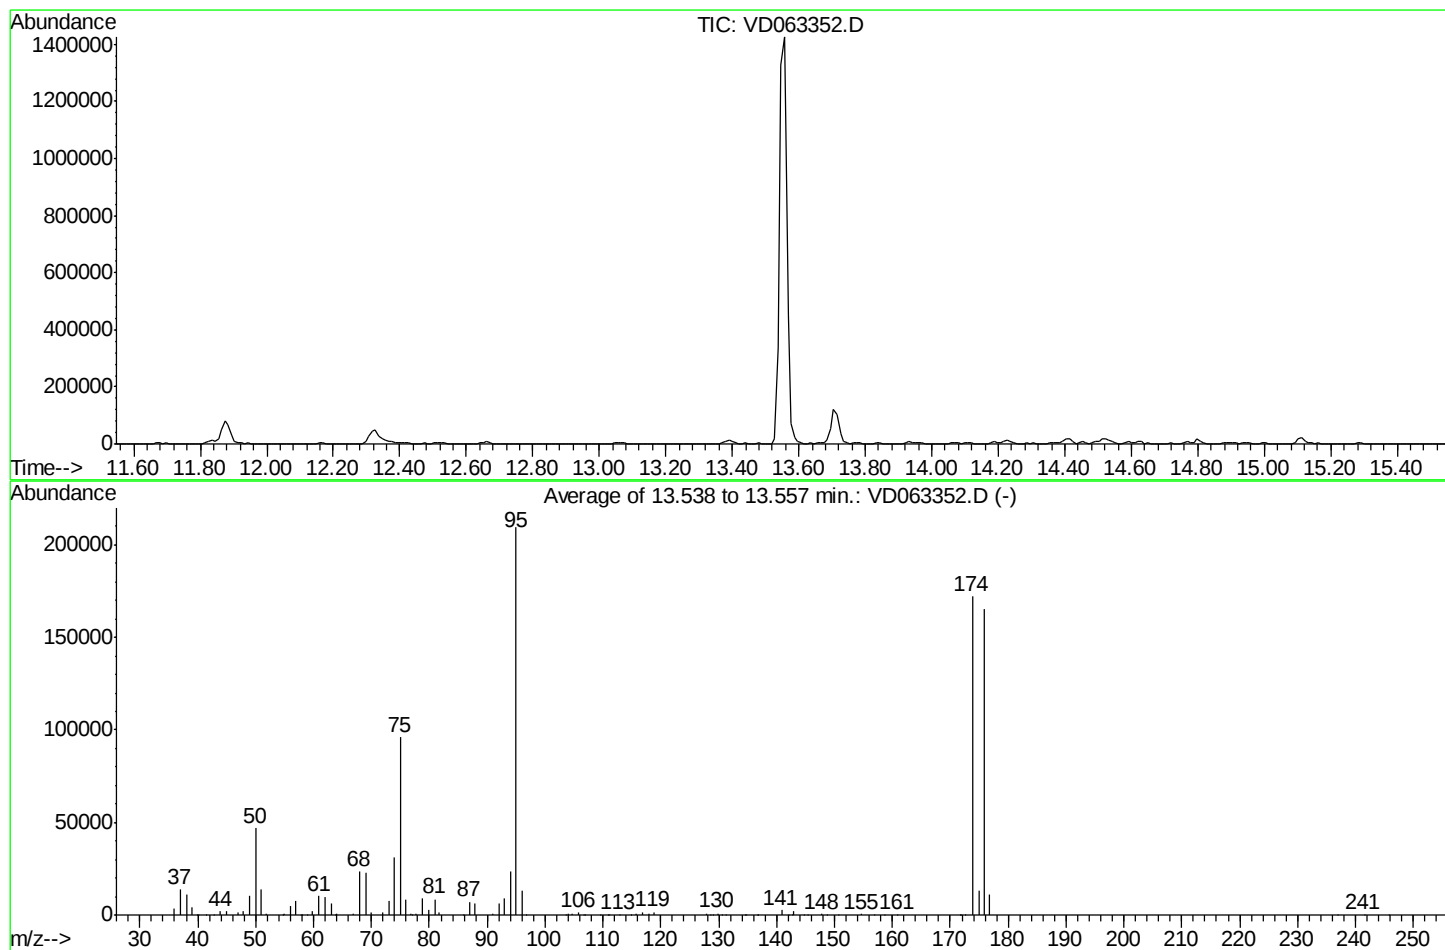

AutoFind: Scans 1230, 1231, 1232; Background Corrected with Scan 1226

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 22.3      | 46712   | PASS             |
| 75          | 95           | 30           | 60           | 45.8      | 95872   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 209456  | PASS             |
| 96          | 95           | 5            | 9            | 6.3       | 13141   | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 82.1      | 172018  | PASS             |
| 175         | 174          | 5            | 9            | 7.5       | 12907   | PASS             |
| 176         | 174          | 95           | 101          | 96.1      | 165293  | PASS             |
| 177         | 176          | 5            | 9            | 6.9       | 11391   | PASS             |