
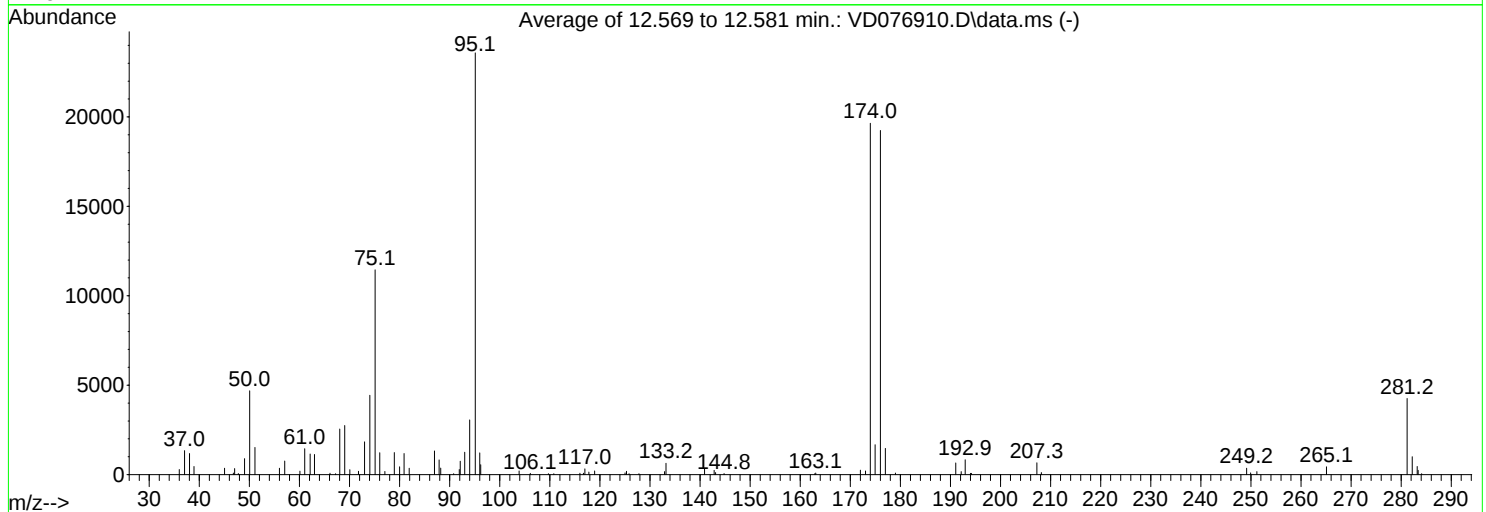


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080323\
Data File : VD076910.D
Acq On : 03 Aug 2023 09:34
Operator : KP/SY
Sample : BFB153
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB153

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM080323SMA.M
Title : SFAM01.0
Last Update : Fri Aug 04 02:21:25 2023

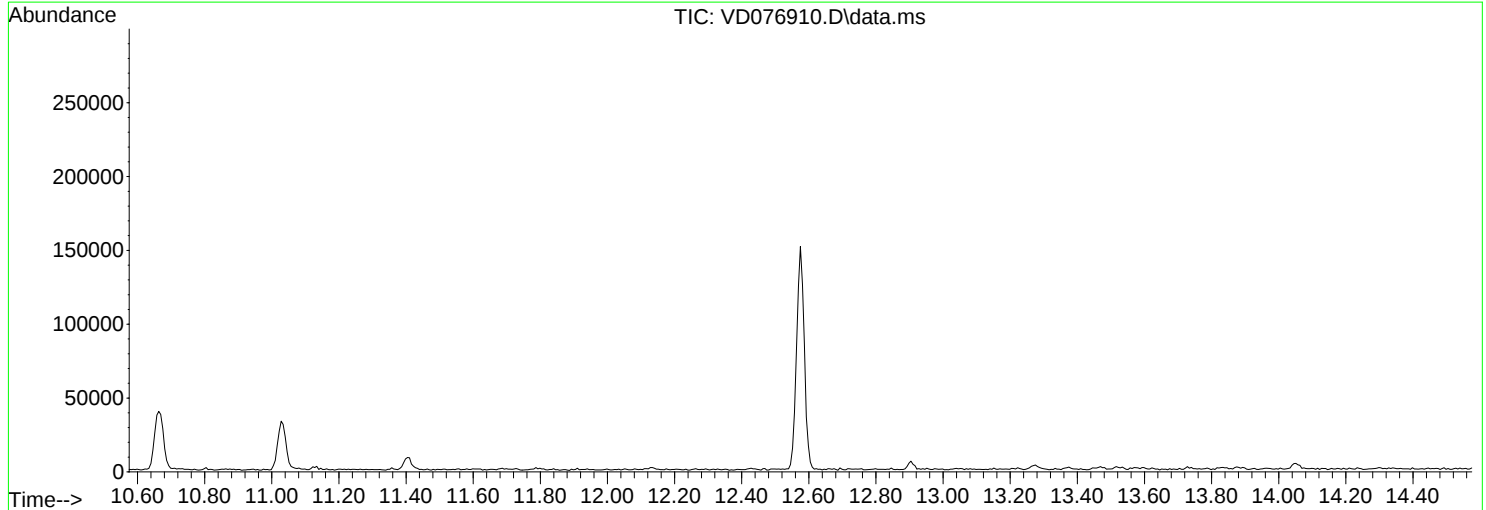

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1861

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	4685	PASS
75	95	30	80	48.6	11454	PASS
95	95	100	100	100.0	23581	PASS
96	95	5	9	5.2	1219	PASS
173	174	0.00	2	1.0	202	PASS
174	95	50	120	83.3	19645	PASS
175	174	5	9	8.5	1672	PASS
176	174	95	105	97.9	19237	PASS
177	176	5	10	7.6	1470	PASS

Scan 1861 (12.534 min): VD076910.D\data.ms
BFB153

m/z	Abundance
40.00	1027.0
44.10	1002.0

Instrument :
MSVOA_D
ClientSampleId :
BFB153

m/z	Abundance
36.10	346.0
37.10	1496.0
38.10	1219.0
38.90	400.0
40.00	909.0
44.10	1013.0
45.10	198.0
47.10	650.0
49.10	779.0
50.00	4749.0
51.10	1264.0
56.10	302.0
57.00	904.0
60.10	243.0
61.10	897.0
62.10	1267.0
63.00	994.0
67.20	169.0
68.00	2042.0
69.10	2627.0
70.10	334.0
73.10	1665.0
74.10	4409.0
75.10	10892.0
76.10	1085.0
77.00	337.0
79.00	1054.0
80.00	519.0
80.90	987.0
81.90	383.0
87.00	1259.0
87.90	1360.0
91.90	871.0
93.00	1432.0
94.00	3205.0
95.10	23576.0
96.00	1467.0
103.90	335.0
106.10	214.0
117.00	408.0
119.00	243.0
125.80	174.0
132.90	502.0
142.80	258.0
171.90	246.0
174.00	18248.0
175.00	1567.0
176.00	18584.0
177.00	1245.0
191.00	443.0
192.90	813.0
207.20	463.0
249.20	176.0
265.00	286.0
281.20	3274.0
282.20	630.0
283.20	588.0

Instrument :
MSVOA_D
ClientSampleId :
BFB153

m/z	Abundance
35.90	260.0
37.10	1382.0
38.00	1365.0
39.00	618.0
39.90	521.0
44.20	946.0
45.00	409.0
47.00	370.0
49.00	1092.0
50.10	5072.0
51.10	2236.0
55.90	407.0
57.10	692.0
60.20	190.0
61.00	2145.0
62.10	989.0
63.00	1390.0
66.10	237.0
68.00	2799.0
69.10	2590.0
70.00	298.0
71.80	290.0
72.90	1658.0
74.00	5292.0
75.10	12588.0
76.00	1563.0
77.10	193.0
78.90	1712.0
80.00	354.0
81.00	1535.0
81.90	528.0
86.90	1670.0
87.90	1111.0
90.80	161.0
92.10	1157.0
92.90	1000.0
94.00	3399.0
95.10	27000.0
96.00	2189.0
103.80	279.0
109.70	163.0
110.80	161.0
116.00	249.0
116.70	254.0
117.00	222.0
117.80	420.0
118.90	371.0
125.30	565.0
127.80	164.0
133.20	816.0
140.90	538.0
142.80	473.0
162.90	154.0
172.00	205.0
173.10	409.0
174.00	21832.0
175.00	1669.0
176.00	21520.0
177.00	1532.0
179.00	278.0
191.00	829.0
192.20	177.0
192.90	821.0
194.00	206.0
207.30	721.0
208.20	196.0
249.10	497.0
249.90	153.0
251.20	260.0
265.10	303.0
281.20	4938.0
282.30	1107.0
283.40	718.0

Instrument :
MSVOA_D
ClientSampleId :
BFB153

m/z	Abundance
36.00	253.0
37.00	1147.0
38.10	970.0
39.00	355.0
40.10	1145.0
44.10	790.0
45.00	463.0
46.80	260.0
47.80	199.0
49.10	820.0
50.10	4233.0
51.10	1060.0
56.00	360.0
57.00	690.0
60.00	160.0
61.10	1310.0
62.20	1213.0
63.00	1000.0
68.10	2814.0
69.00	3017.0
70.00	193.0
71.80	279.0
73.00	2179.0
74.10	3598.0
75.10	10882.0
76.10	1024.0
78.90	940.0
80.00	457.0
80.80	1028.0
82.00	150.0
86.90	1046.0
88.20	1105.0
92.10	1098.0
93.10	1331.0
94.00	2583.0
95.10	20168.0
96.20	1675.0
117.00	349.0
125.00	298.0
133.20	1090.0
140.90	418.0
143.10	345.0
144.80	183.0
163.10	271.0
172.10	307.0
172.90	196.0
174.00	18856.0
174.90	1780.0
176.00	17608.0
177.00	1634.0
191.10	695.0
192.10	342.0
193.00	855.0
194.20	212.0
207.20	815.0
208.10	156.0
249.10	414.0
250.00	155.0
251.20	240.0
265.10	723.0
281.20	4575.0
282.10	1282.0
283.20	781.0
284.10	156.0

Instrument :
MSVOA_D
ClientSampleId :
BFB153