
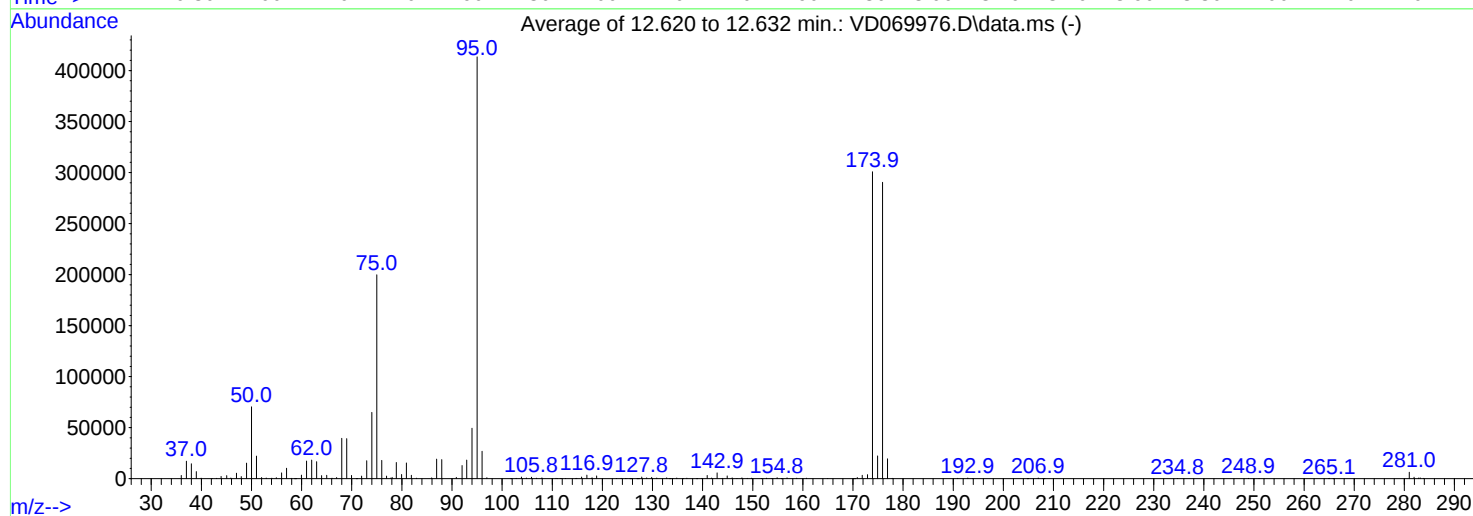


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080421\
 Data File : VD069976.D
 Acq On : 04 Aug 2021 08:59
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D072221S.M
 Title : SW846 8260
 Last Update : Fri Jul 23 04:51:13 2021

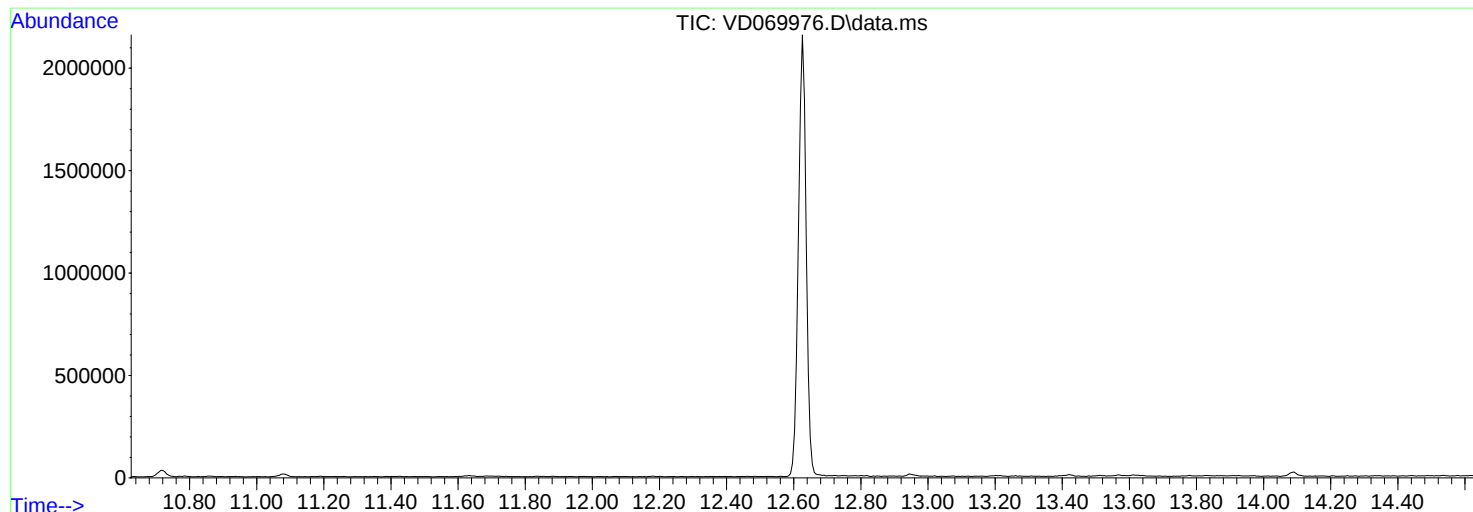

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	70448	PASS
75	95	30	60	48.3	199829	PASS
95	95	100	100	100.0	413440	PASS
96	95	5	9	6.5	26829	PASS
173	174	0.00	2	1.3	4008	PASS
174	95	50	100	72.8	300843	PASS
175	174	5	9	7.4	22317	PASS
176	174	95	101	96.6	290496	PASS
177	176	5	9	6.7	19512	PASS