

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080422\
 Data File : VD073955.D
 Acq On : 04 Aug 2022 16:11
 Operator : VA/SY
 Sample : N3962-06
 Misc : 3.71G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 RVE-192

Quant Time: Aug 05 07:53:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D080122S.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 02 05:13:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.973	168	120534	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.856	114	202906	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.632	117	175876	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	67208	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.320	65	59115	60.588	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	121.180%
35) Dibromofluoromethane	7.909	113	61609	48.869	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	97.740%
50) Toluene-d8	10.326	98	167057	39.339	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	78.680%
62) 4-Bromofluorobenzene	12.620	95	56420	36.128	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	72.260%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080422\
Data File : VD073955.D
Acq On : 04 Aug 2022 16:11
Operator : VA/SY
Sample : N3962-06
Misc : 3.71G/5.00ml/MSVOA_D/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
RVE-192


Quant Time: Aug 05 07:53:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D080122S.M
Quant Title : SW846 8260
QLast Update : Tue Aug 02 05:13:57 2022
Response via : Initial Calibration

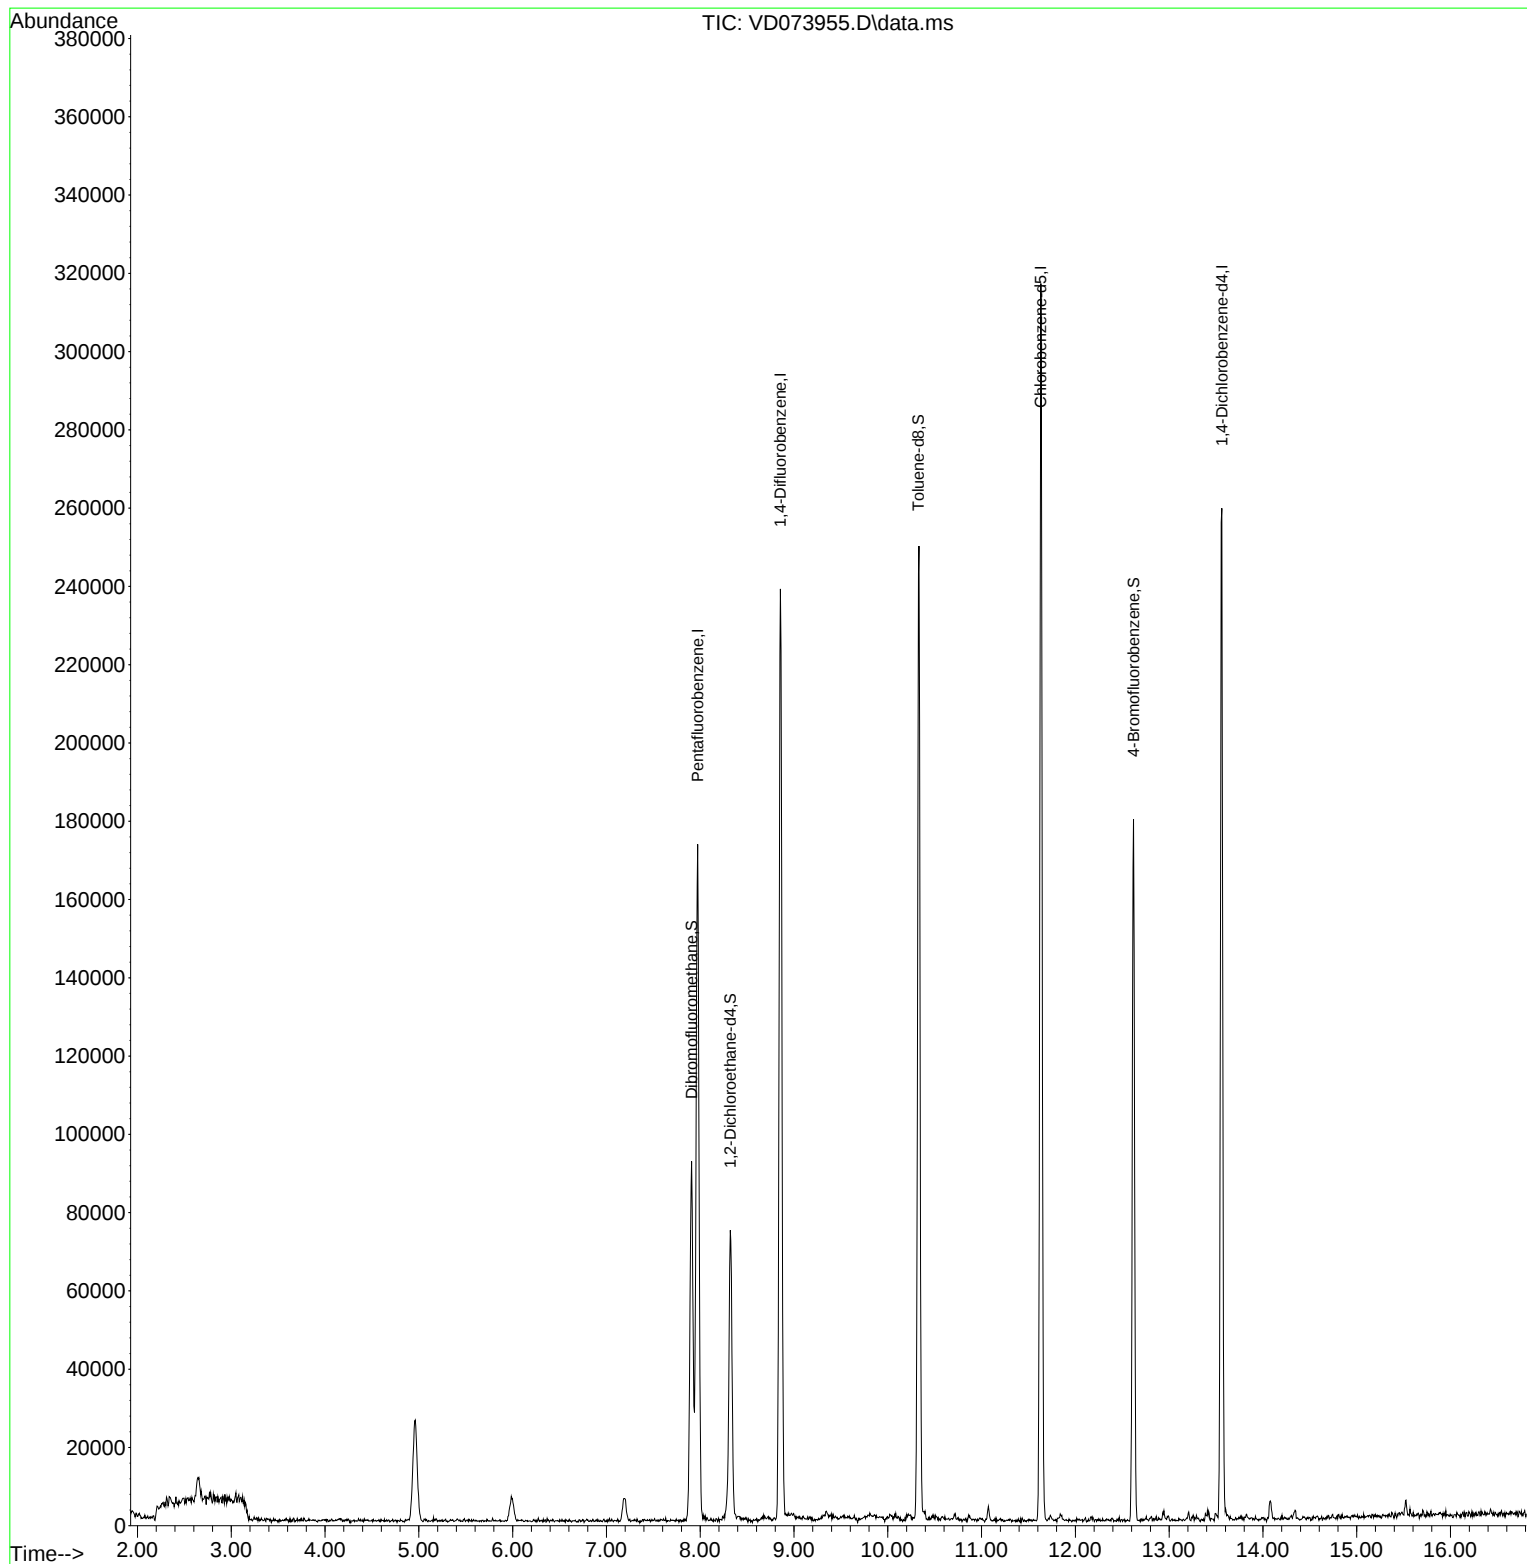



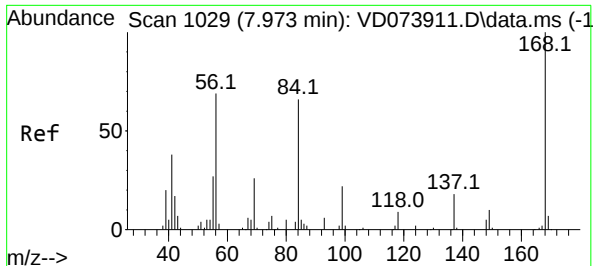


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.973 min Scan# 1029
Delta R.T. 0.000 min
Lab File: VD073955.D
Acq: 04 Aug 2022 16:11

Instrument :
MSVOA_D
ClientSampleId :
RVE-192



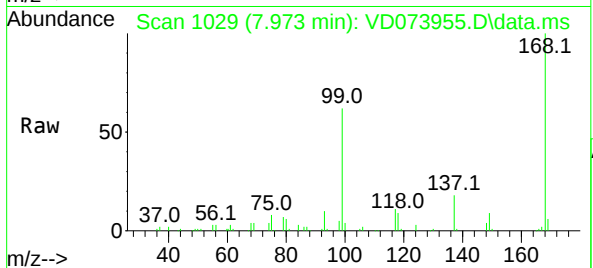



Tgt Ion:168 Resp: 120534
Ion Ratio Lower Upper
168 100
99 61.9 52.2 78.4

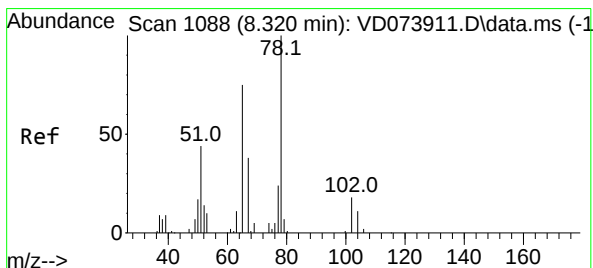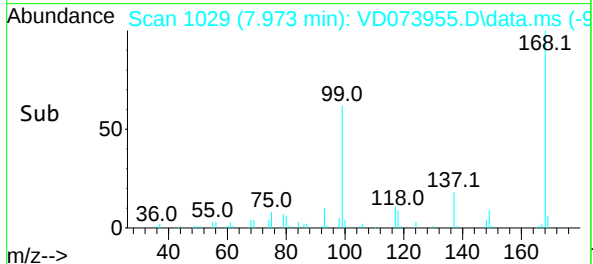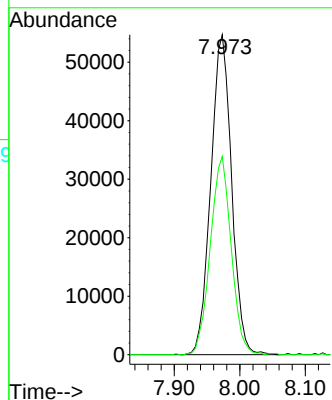

#33
1,2-Dichloroethane-d4
Concen: 60.588 ug/l
RT: 8.320 min Scan# 1088
Delta R.T. 0.000 min
Lab File: VD073955.D
Acq: 04 Aug 2022 16:11

Tgt Ion: 65 Resp: 59115
Ion Ratio Lower Upper
65 100
67 50.3 0.0 102.8

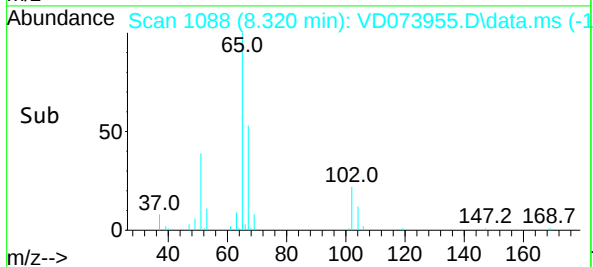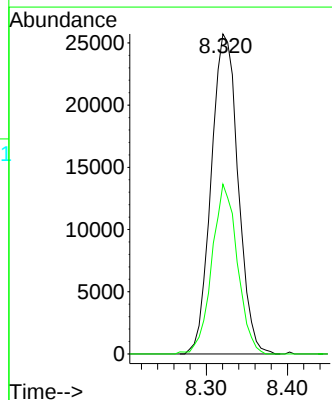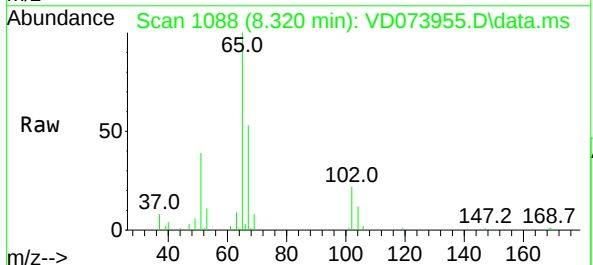

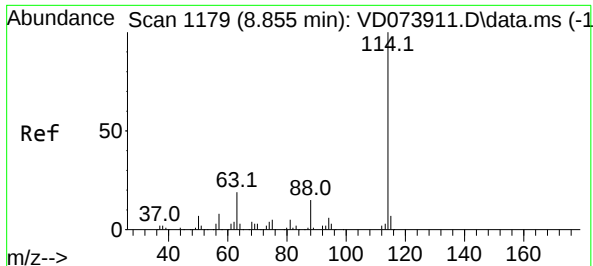

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.856 min Scan# 1179

Delta R.T. 0.000 min

Lab File: VD073955.D

Acq: 04 Aug 2022 16:11

Instrument :

MSVOA_D

ClientSampleId :

RVE-192





Tgt Ion:114 Resp: 202906

Ion Ratio Lower Upper

114 100

63 20.0 0.0 37.6

88 15.1 0.0 30.2

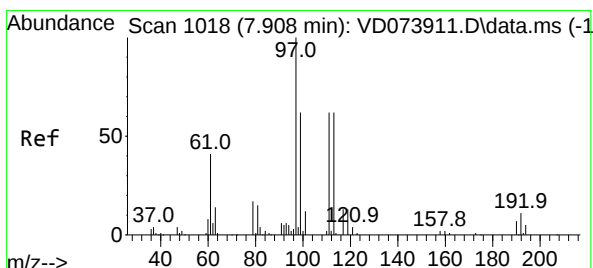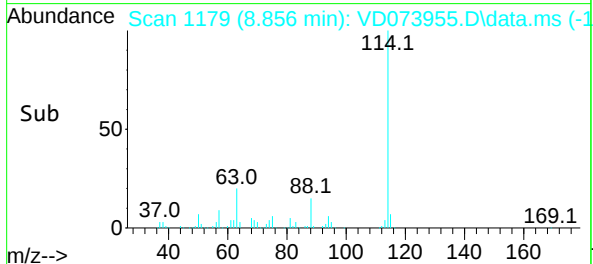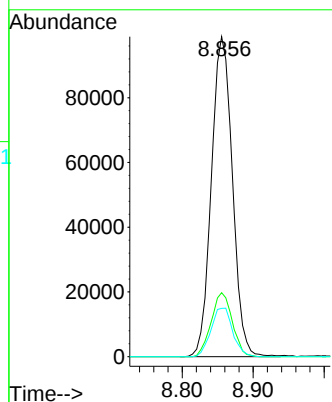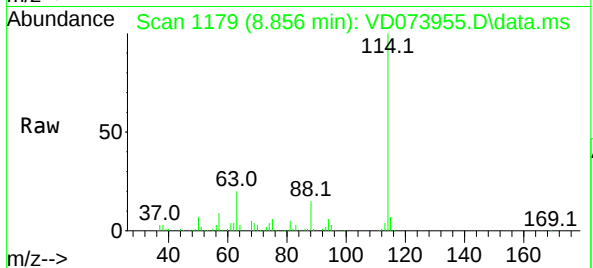

#35

Dibromofluoromethane

Concen: 48.869 ug/l

RT: 7.909 min Scan# 1018

Delta R.T. 0.000 min

Lab File: VD073955.D

Acq: 04 Aug 2022 16:11




Tgt Ion:113 Resp: 61609


Ion Ratio Lower Upper

113 100

111 104.8 83.7 125.5

192 18.7 15.0 22.6


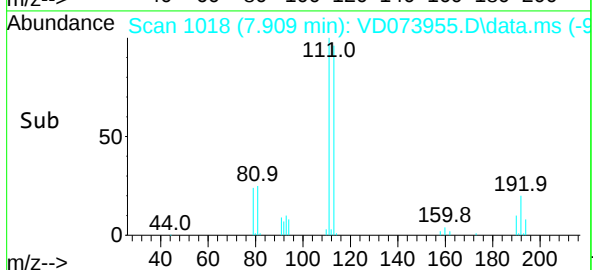
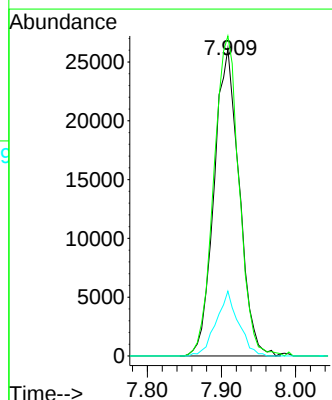
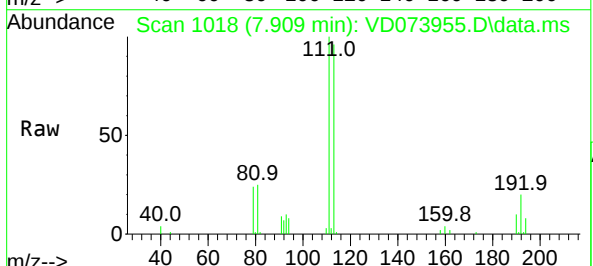


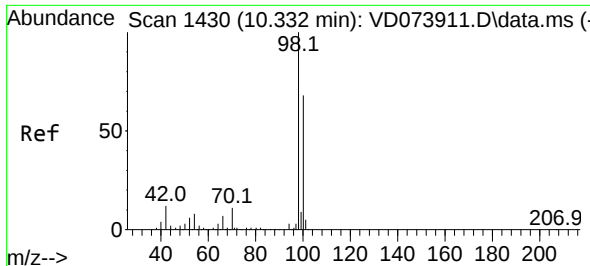

#50
Toluene-d8
Concen: 39.339 ug/l
RT: 10.326 min Scan# 1430
Delta R.T. -0.006 min
Lab File: VD073955.D
Acq: 04 Aug 2022 16:11




Instrument :
MSVOA_D
ClientSampleId :
RVE-192


Tgt Ion: 98 Resp: 167057
Ion Ratio Lower Upper
98 100
100 66.2 53.1 79.7

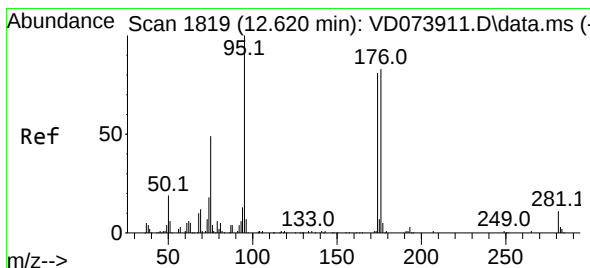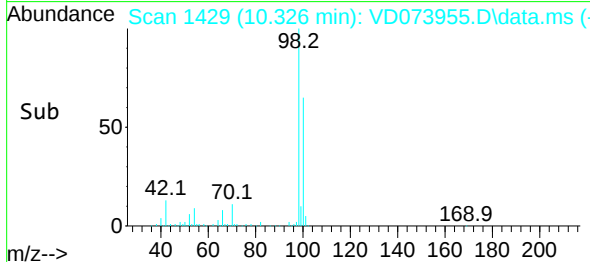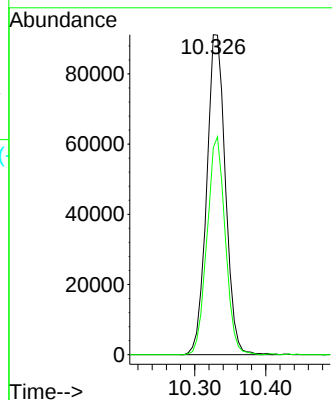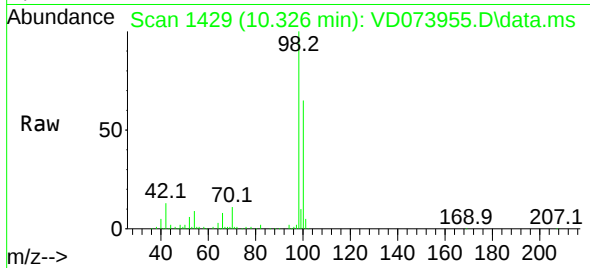

#62
4-Bromofluorobenzene
Concen: 36.128 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. 0.000 min
Lab File: VD073955.D
Acq: 04 Aug 2022 16:11

Tgt Ion: 95 Resp: 56420
Ion Ratio Lower Upper
95 100
174 81.5 0.0 164.2
176 76.8 0.0 161.4


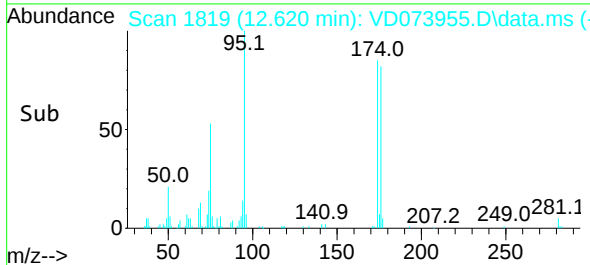
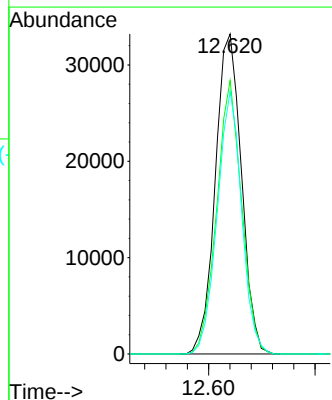
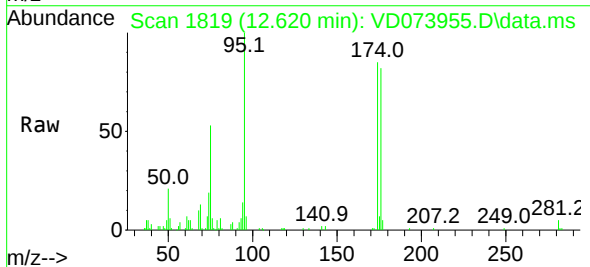


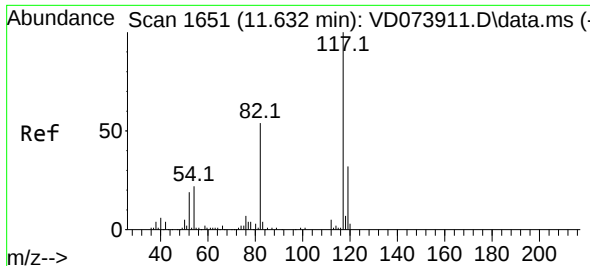

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.632 min Scan# 1651
Delta R.T. 0.000 min
Lab File: VD073955.D
Acq: 04 Aug 2022 16:11

Instrument :
MSVOA_D
ClientSampleId :
RVE-192

Tgt Ion:117 Resp: 175876
Ion Ratio Lower Upper
117 100
82 54.2 43.3 64.9
119 31.6 25.8 38.8

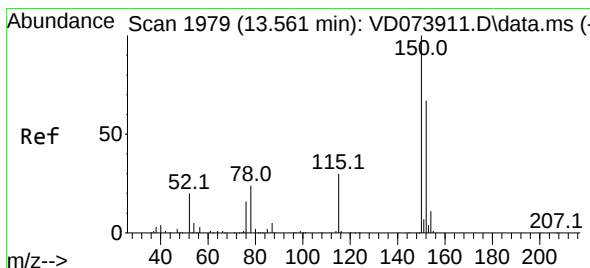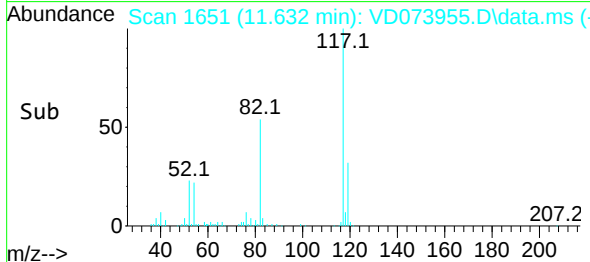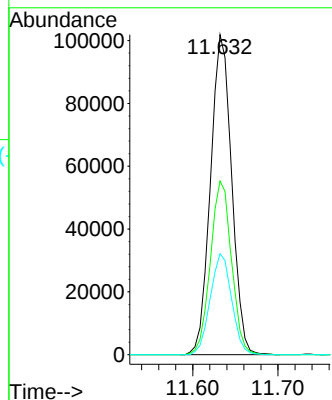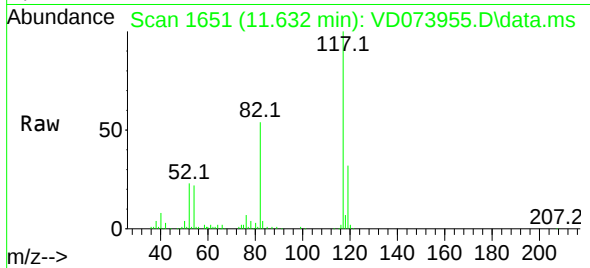

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. 0.000 min
Lab File: VD073955.D
Acq: 04 Aug 2022 16:11

Tgt Ion:152 Resp: 67208
Ion Ratio Lower Upper
152 100
115 59.9 29.1 87.3
150 155.8 0.0 338.2

