
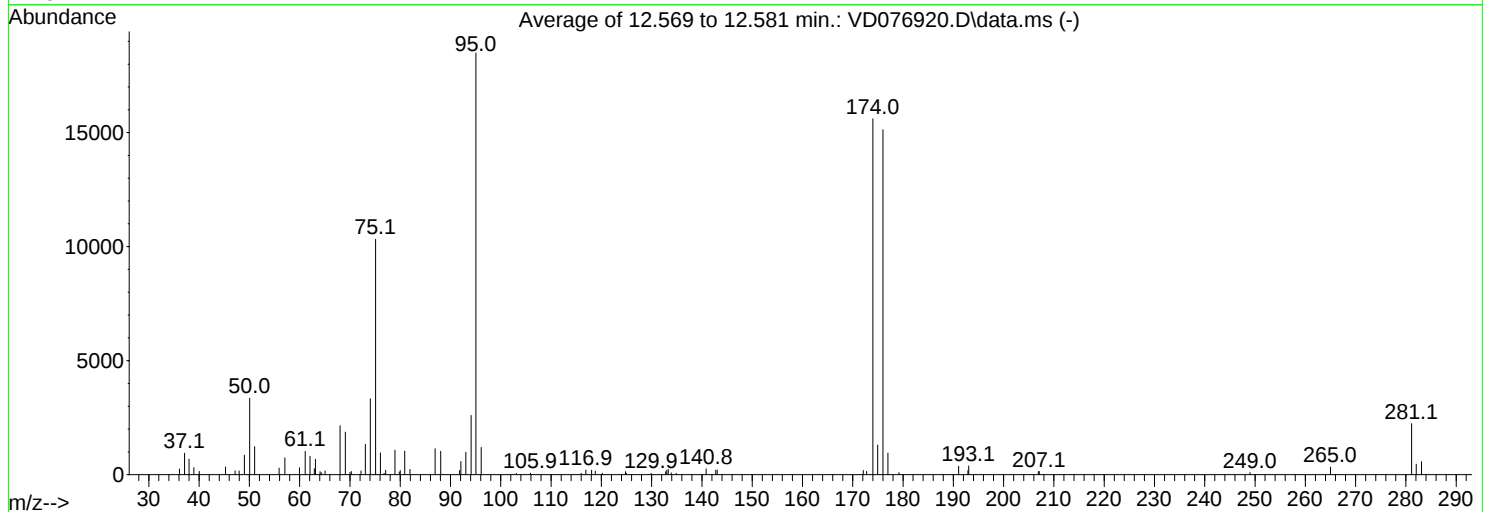


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080423\
Data File : VD076920.D
Acq On : 04 Aug 2023 10:58
Operator : KP/SY
Sample : BFB154
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB154

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM080323SMA.M
Title : SFAM01.0
Last Update : Fri Aug 04 02:21:25 2023

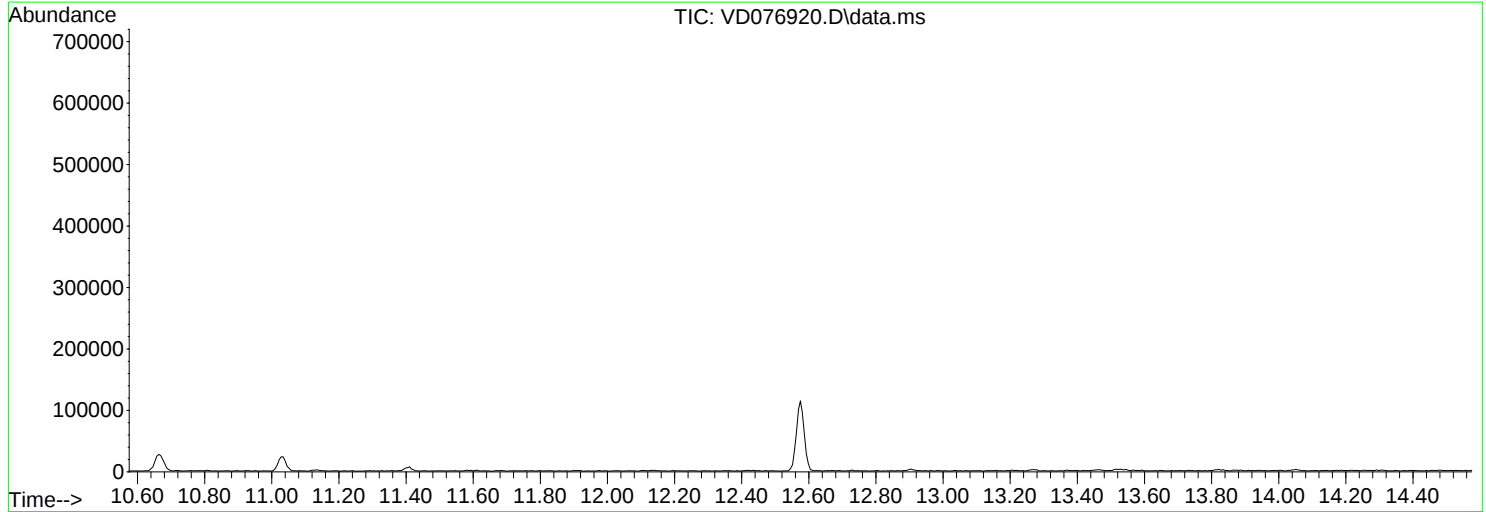

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1861

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.1	3357	PASS
75	95	30	80	55.8	10322	PASS
95	95	100	100	100.0	18499	PASS
96	95	5	9	6.4	1192	PASS
173	174	0.00	2	0.9	142	PASS
174	95	50	120	84.4	15609	PASS
175	174	5	9	8.3	1297	PASS
176	174	95	105	96.9	15131	PASS
177	176	5	10	6.3	946	PASS

Scan 1861 (12.534 min): VD076920.D\data.ms
BFB154

m/z	Abundance
40.10	780.0
43.90	835.0

Instrument :
MSVOA_D
ClientSampleId :
BFB154

m/z	Abundance
36.20	193.0
37.00	1295.0
38.00	789.0
39.10	310.0
40.10	1018.0
44.10	722.0
45.30	297.0
48.00	238.0
49.00	855.0
50.00	3806.0
51.10	1274.0
56.00	222.0
57.00	887.0
60.00	232.0
61.00	1059.0
62.10	786.0
63.20	534.0
64.10	215.0
68.10	2364.0
69.10	1802.0
70.30	175.0
73.00	1353.0
74.00	3715.0
75.10	10433.0
76.10	930.0
76.80	175.0
77.20	221.0
79.00	1060.0
79.80	326.0
80.90	928.0
82.00	400.0
87.00	1038.0
88.10	1161.0
91.80	539.0
92.20	412.0
93.10	914.0
94.00	2998.0
95.10	17680.0
96.10	1172.0
103.10	158.0
105.90	193.0
116.00	165.0
116.90	299.0
118.00	184.0
118.80	185.0
132.80	375.0
133.30	152.0
140.90	290.0
142.80	284.0
172.20	205.0
174.00	14636.0
174.90	1225.0
176.00	14254.0
177.00	694.0
191.10	240.0
192.90	521.0
206.90	151.0
264.90	325.0
281.10	1470.0
282.10	348.0
283.10	485.0

Instrument :
MSVOA_D
ClientSampleId :
BFB154

m/z	Abundance
36.00	183.0
37.10	896.0
38.00	849.0
38.90	291.0
40.10	814.0
44.00	852.0
45.20	449.0
47.20	265.0
49.00	809.0
50.10	3774.0
51.10	1276.0
55.90	416.0
57.10	638.0
59.90	245.0
61.10	940.0
62.00	958.0
62.90	771.0
63.20	668.0
64.00	192.0
65.00	290.0
68.10	1968.0
69.10	2279.0
70.00	300.0
72.20	257.0
73.10	1395.0
74.10	4074.0
75.10	11542.0
76.00	1072.0
78.90	1132.0
80.00	551.0
80.90	1299.0
86.90	1273.0
88.00	1031.0
92.00	809.0
93.10	1081.0
94.10	2911.0
95.10	21664.0
96.10	1411.0
118.10	239.0
118.80	280.0
120.20	181.0
124.80	394.0
133.30	536.0
133.90	239.0
134.90	175.0
140.90	267.0
142.70	297.0
143.10	239.0
172.00	338.0
172.70	238.0
174.00	16872.0
174.90	1508.0
176.00	16186.0
177.00	1204.0
191.10	436.0
193.10	614.0
207.10	420.0
265.00	212.0
281.20	2281.0
282.00	422.0
283.10	501.0

Instrument :
MSVOA_D
ClientSampleId :
BFB154

m/z	Abundance
36.10	363.0
37.20	639.0
38.10	403.0
38.90	318.0
40.00	924.0
44.10	811.0
45.20	265.0
47.10	248.0
47.90	242.0
49.00	910.0
50.10	2492.0
51.00	1134.0
55.80	225.0
57.10	695.0
60.00	424.0
61.20	1086.0
62.10	680.0
63.10	829.0
64.30	242.0
65.10	191.0
68.00	2117.0
69.10	1512.0
70.20	258.0
72.20	219.0
73.00	1220.0
74.00	2192.0
75.10	8991.0
76.10	870.0
77.00	365.0
79.00	1033.0
80.90	864.0
81.90	301.0
86.90	1096.0
88.10	889.0
92.10	508.0
93.00	957.0
94.20	1891.0
95.00	16152.0
96.10	994.0
116.90	322.0
118.00	162.0
125.00	153.0
129.90	172.0
133.00	596.0
140.80	203.0
143.00	367.0
172.80	189.0
174.00	15318.0
175.00	1157.0
176.00	14953.0
177.00	940.0
179.20	273.0
191.00	441.0
193.00	514.0
206.90	261.0
249.00	273.0
265.10	444.0
281.20	2971.0
282.10	594.0
283.10	715.0

Instrument :
MSVOA_D
ClientSampleId :
BFB154