


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD080519\
 Data File : VD063374.D
 Acq On : 5 Aug 2019 9:51
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D072919S.M
 Title : SW846 8260
 Last Update : Tue Jul 30 03:04:50 2019

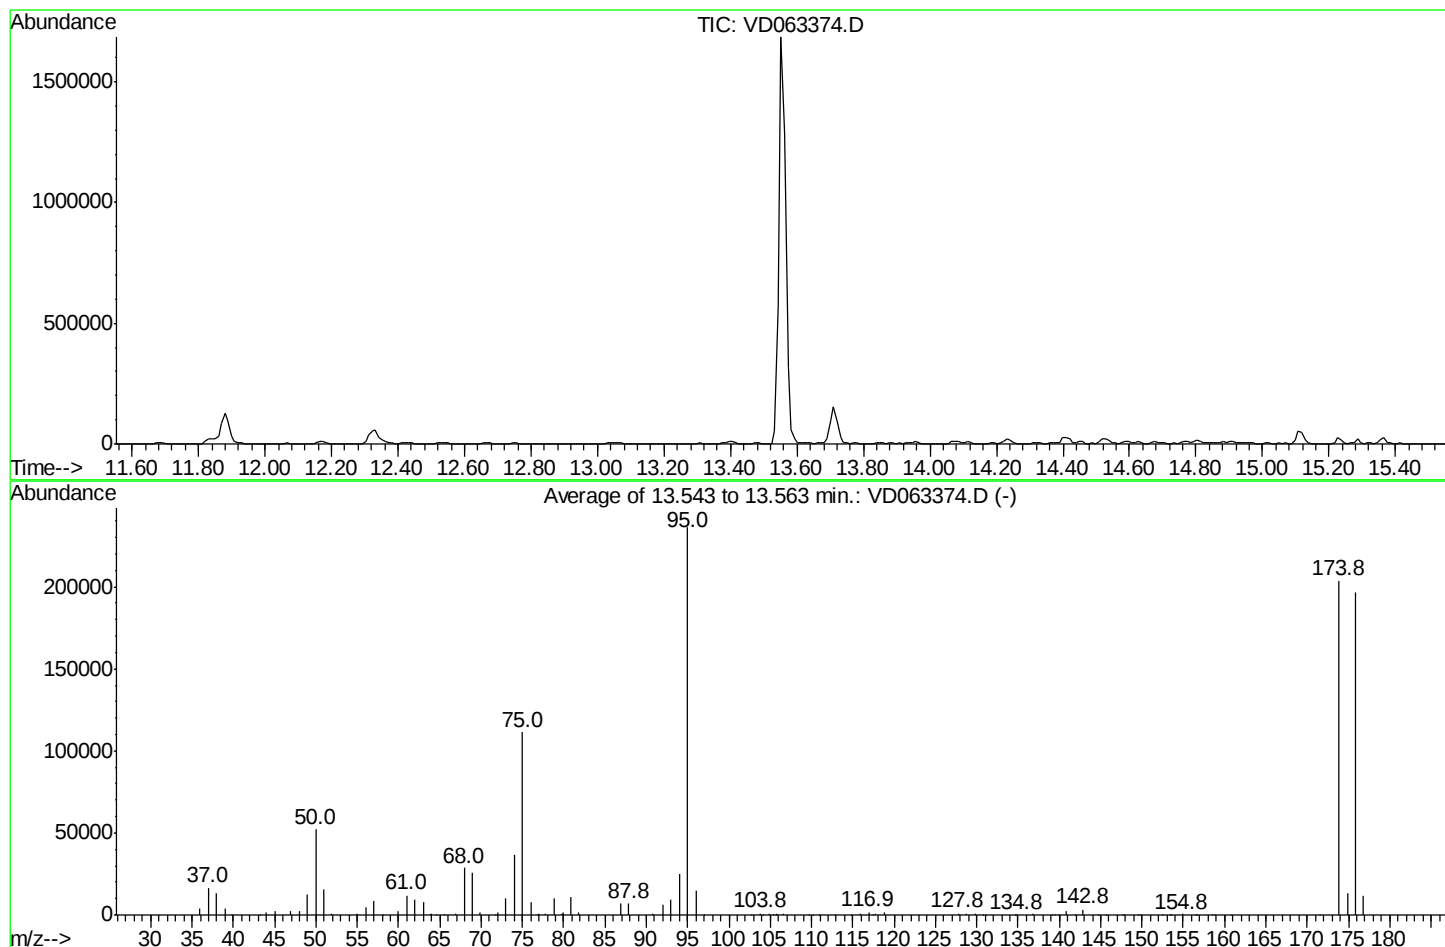

AutoFind: Scans 1231, 1232, 1233; Background Corrected with Scan 1226

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	51949	PASS
75	95	30	60	47.1	111349	PASS
95	95	100	100	100.0	236245	PASS
96	95	5	9	6.2	14691	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	86.2	203690	PASS
175	174	5	9	6.5	13221	PASS
176	174	95	101	96.5	196493	PASS
177	176	5	9	6.1	11907	PASS