


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD080619\
 Data File : VD063392.D
 Acq On : 6 Aug 2019 10:29
 Operator : JC/SY
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D072919S.M
 Title : SW846 8260
 Last Update : Tue Jul 30 03:04:50 2019

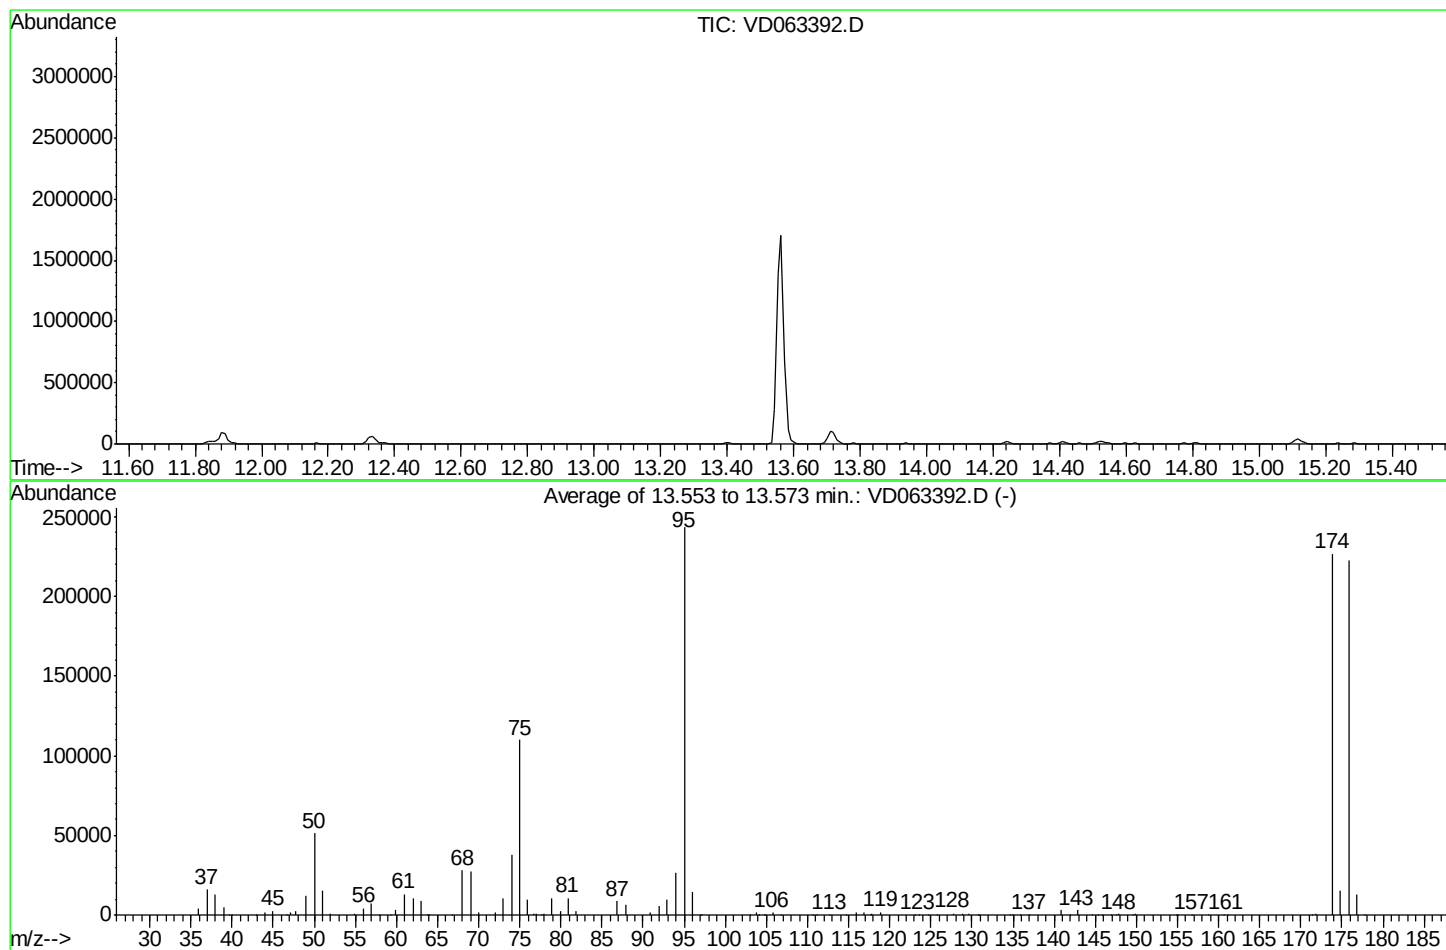

AutoFind: Scans 1301, 1302, 1303; Background Corrected with Scan 1296

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	51338	PASS
75	95	30	60	45.2	110066	PASS
95	95	100	100	100.0	243440	PASS
96	95	5	9	5.9	14387	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	93.3	227050	PASS
175	174	5	9	6.8	15435	PASS
176	174	95	101	98.2	223061	PASS
177	176	5	9	5.9	13099	PASS