


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD080718\  
Data File : VD059696.D  
Acq On : 7 Aug 2018 10:28  
Operator : VA/AP  
Sample : BFB  
Misc : 5.00µl/5ml/MSVOA D/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_D\METHOD\82D080618S.M  
Title : SW846 8260  
Last Update : Wed Aug 08 02:03:19 2018

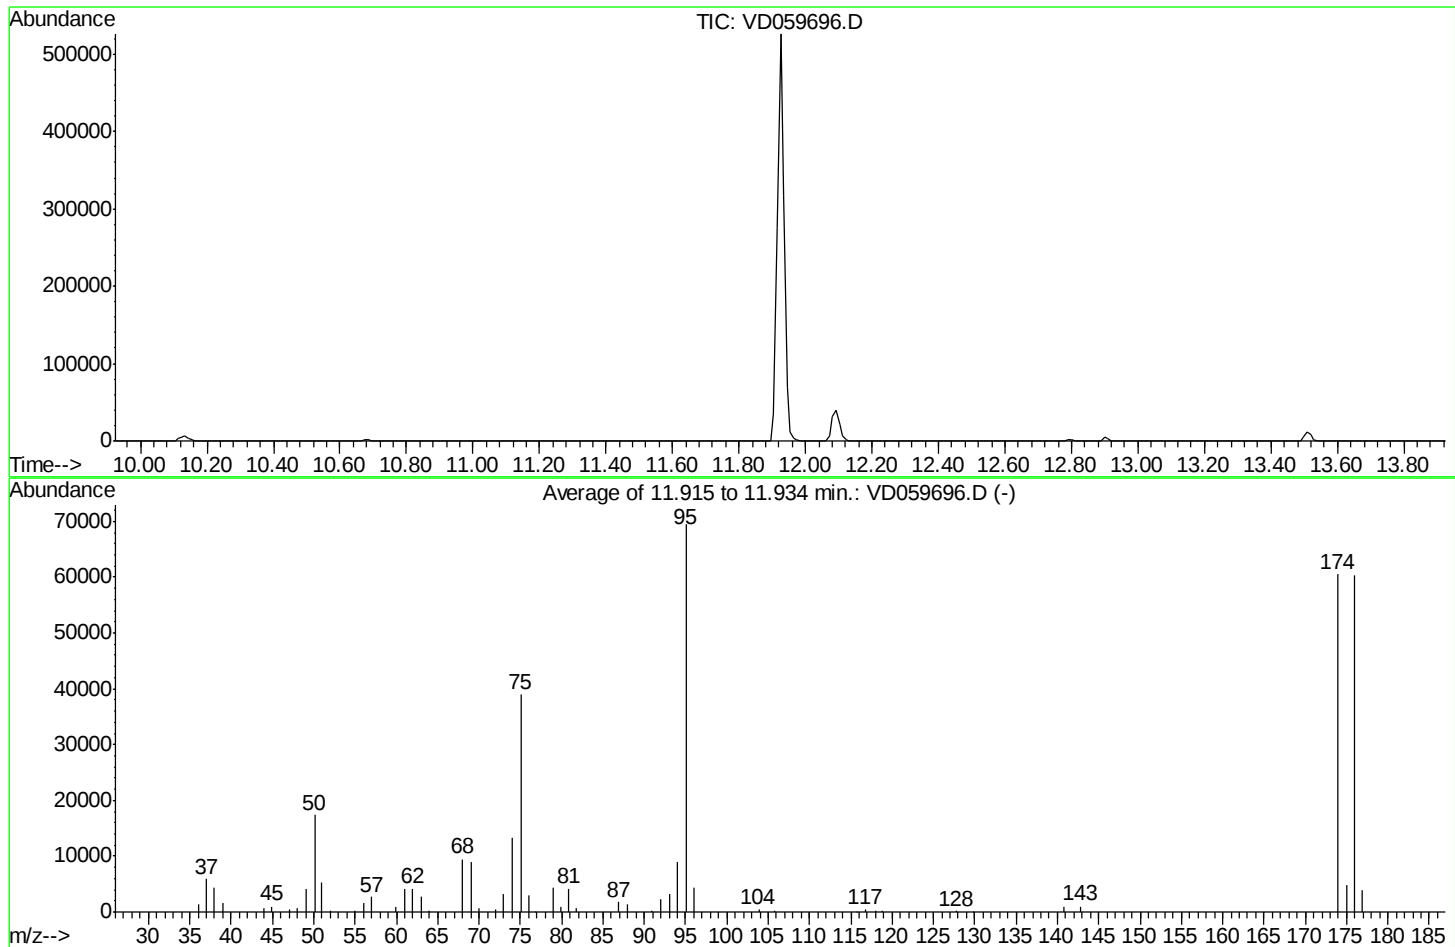

AutoFind: Scans 1188, 1189, 1190; Background Corrected with Scan 1184

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 25.1      | 17428   | PASS             |
| 75          | 95           | 30           | 60           | 56.0      | 38896   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 69466   | PASS             |
| 96          | 95           | 5            | 9            | 6.4       | 4461    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 87.2      | 60549   | PASS             |
| 175         | 174          | 5            | 9            | 8.0       | 4874    | PASS             |
| 176         | 174          | 95           | 101          | 99.5      | 60266   | PASS             |
| 177         | 176          | 5            | 9            | 6.4       | 3832    | PASS             |