
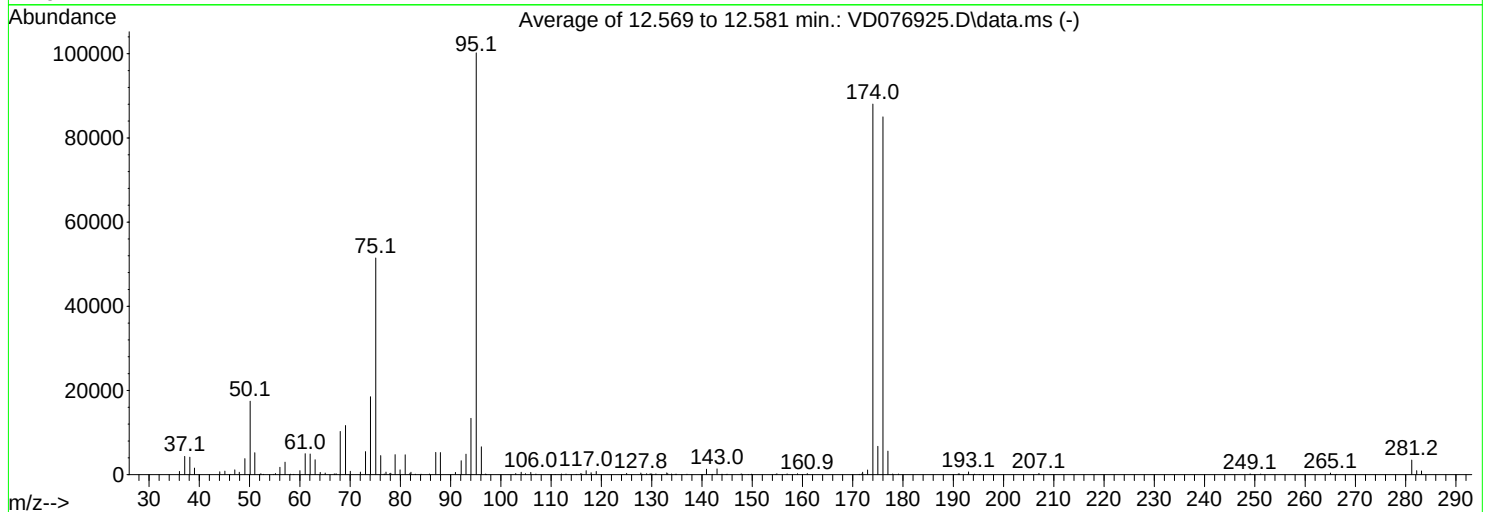


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080723\
Data File : VD076925.D
Acq On : 07 Aug 2023 11:02
Operator : KP/SY
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D071423S.M
Title : SW846 8260
Last Update : Mon Jul 17 08:07:52 2023

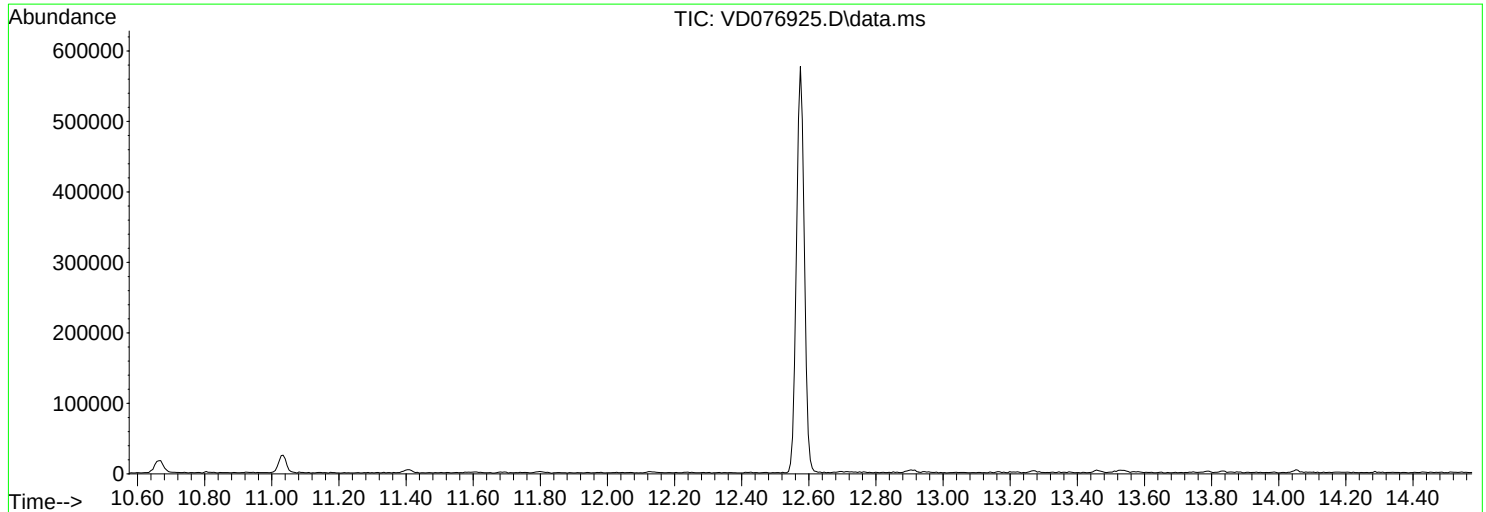

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.4	17456	PASS
75	95	30	60	51.4	51491	PASS
95	95	100	100	100.0	100213	PASS
96	95	5	9	6.6	6603	PASS
173	174	0.00	2	1.3	1121	PASS
174	95	50	100	87.8	88029	PASS
175	174	5	9	7.7	6749	PASS
176	174	95	101	96.5	84984	PASS
177	176	5	9	6.6	5578	PASS