


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD080819\
Data File : VD063429.D
Acq On : 8 Aug 2019 8:49
Operator : JC/SY
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D072919S.M
Title : SW846 8260
Last Update : Tue Jul 30 03:04:50 2019

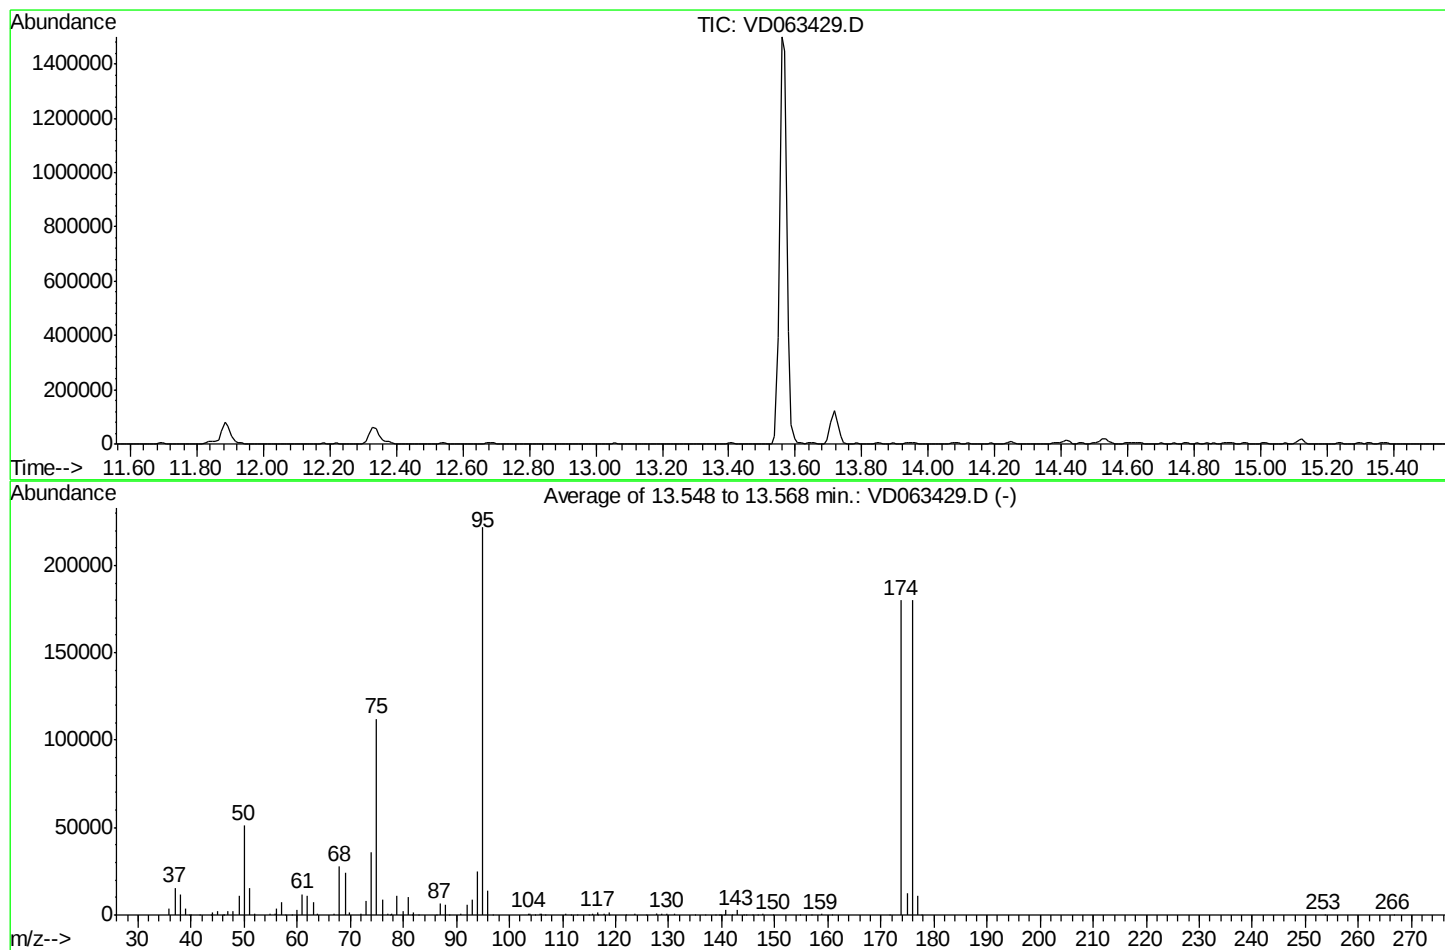

AutoFind: Scans 1231, 1232, 1233; Background Corrected with Scan 1227

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.1	51213	PASS
75	95	30	60	50.5	112085	PASS
95	95	100	100	100.0	221733	PASS
96	95	5	9	6.3	14027	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	81.2	180072	PASS
175	174	5	9	6.9	12457	PASS
176	174	95	101	100.0	180013	PASS
177	176	5	9	6.0	10835	PASS