
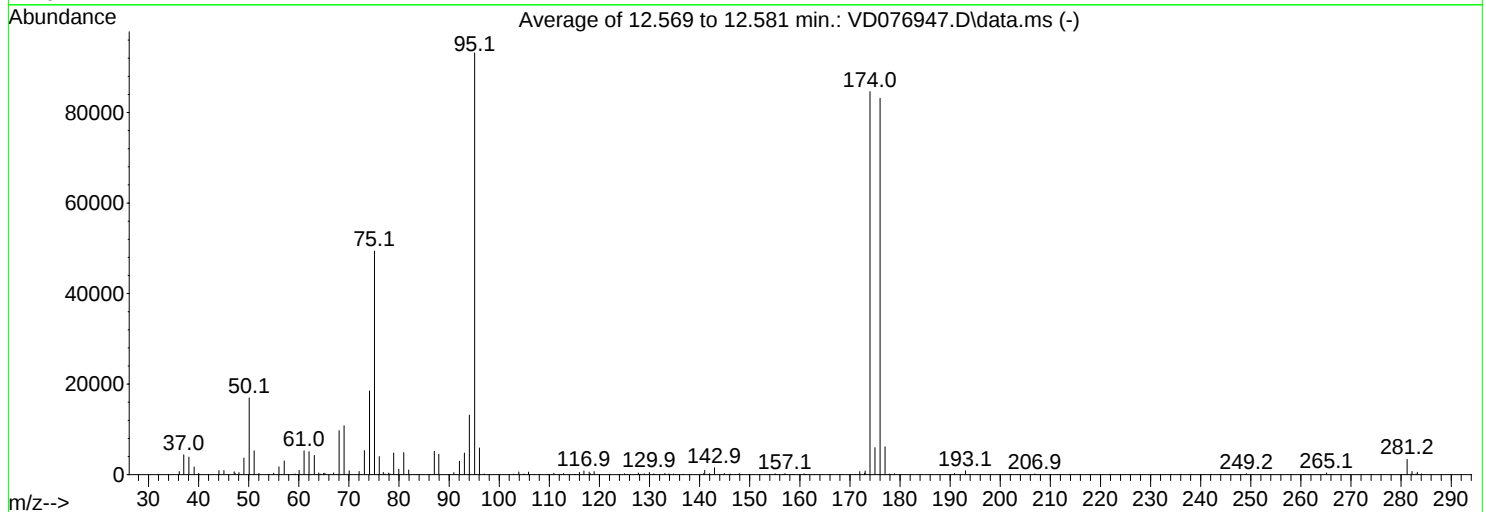


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080823\
Data File : VD076947.D
Acq On : 08 Aug 2023 09:19
Operator : KP/SY
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D080823S.M
Title : SW846 8260
Last Update : Wed Aug 09 07:25:36 2023

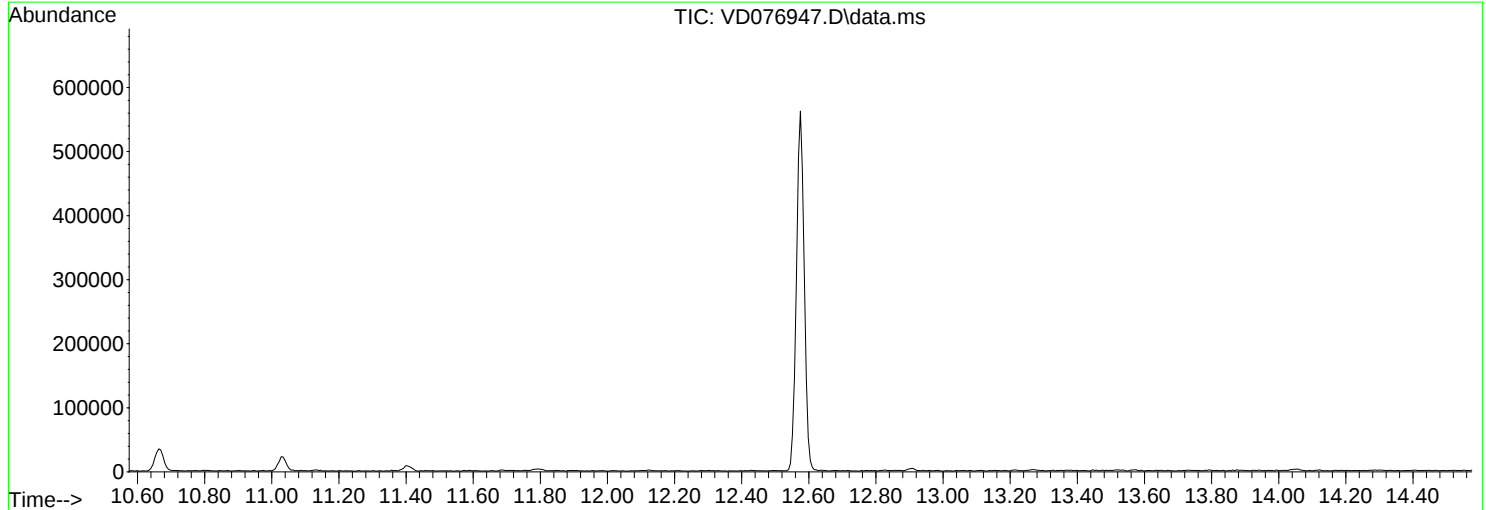


AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.2	16952	PASS
75	95	30	60	53.0	49373	PASS
95	95	100	100	100.0	93187	PASS
96	95	5	9	6.4	5922	PASS
173	174	0.00	2	1.0	821	PASS
174	95	50	100	90.8	84616	PASS
175	174	5	9	7.0	5961	PASS
176	174	95	101	98.2	83133	PASS
177	176	5	9	7.4	6156	PASS

Dichlorodifluoromethane

Response Ratio

Instrument :
MSVOA_D
ClientSampleId :
BFB

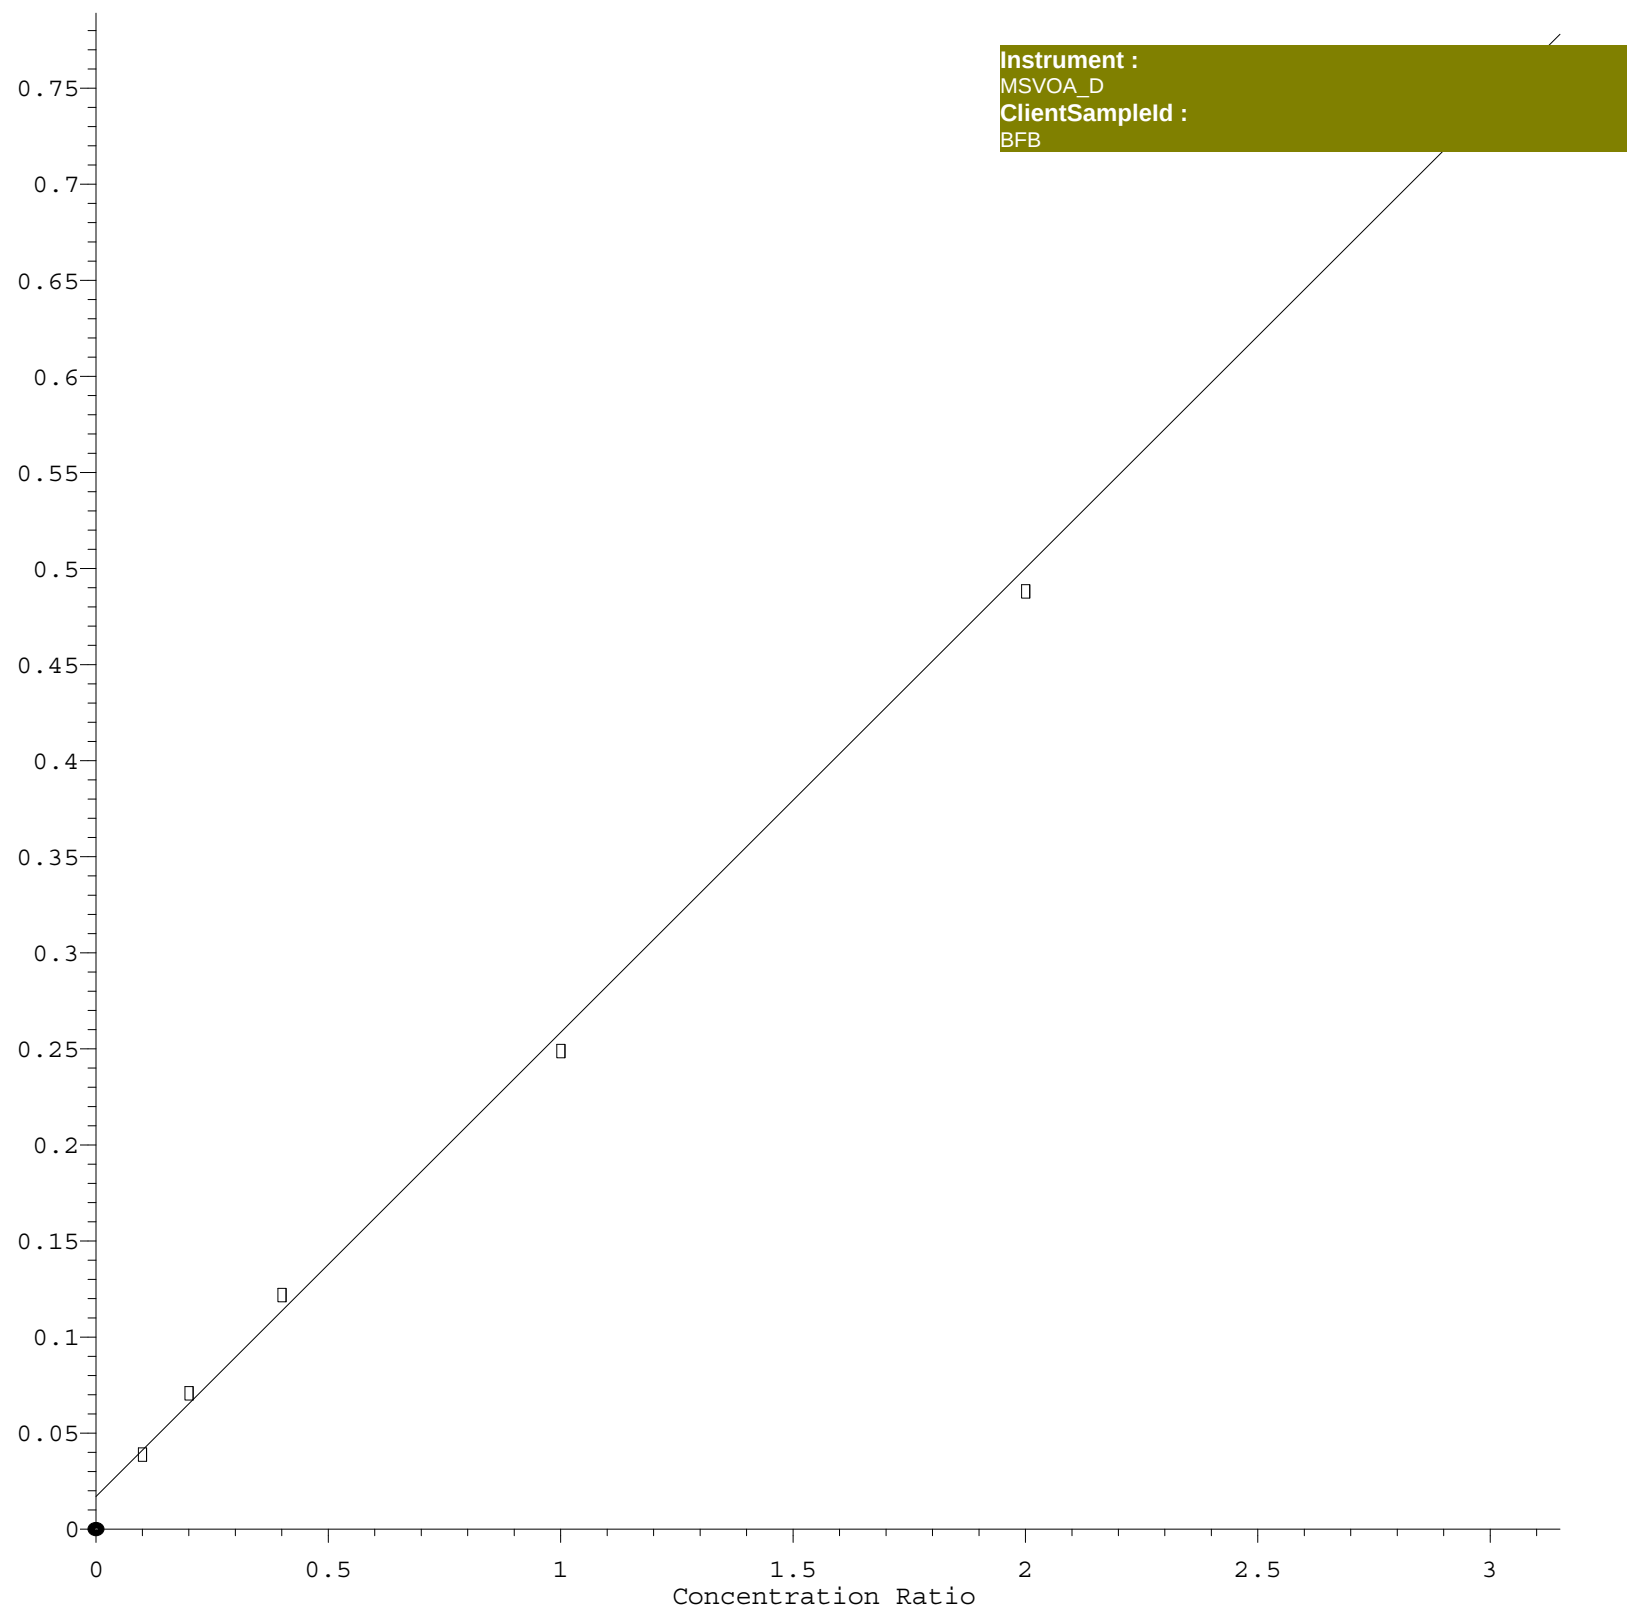

$$\text{Response} = 2.417\text{e-}001 * \text{Amt} + 1.677\text{e-}002$$

Coef of Det (r^2) = 0.998881 Curve Fit: Linear


Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D080823S.M

Calibration Table Last Updated: Wed Aug 09 07:25:36 2023

Tert butyl alcohol

Response Ratio


Instrument :
MSVOA_D
ClientSampleId :
BFB

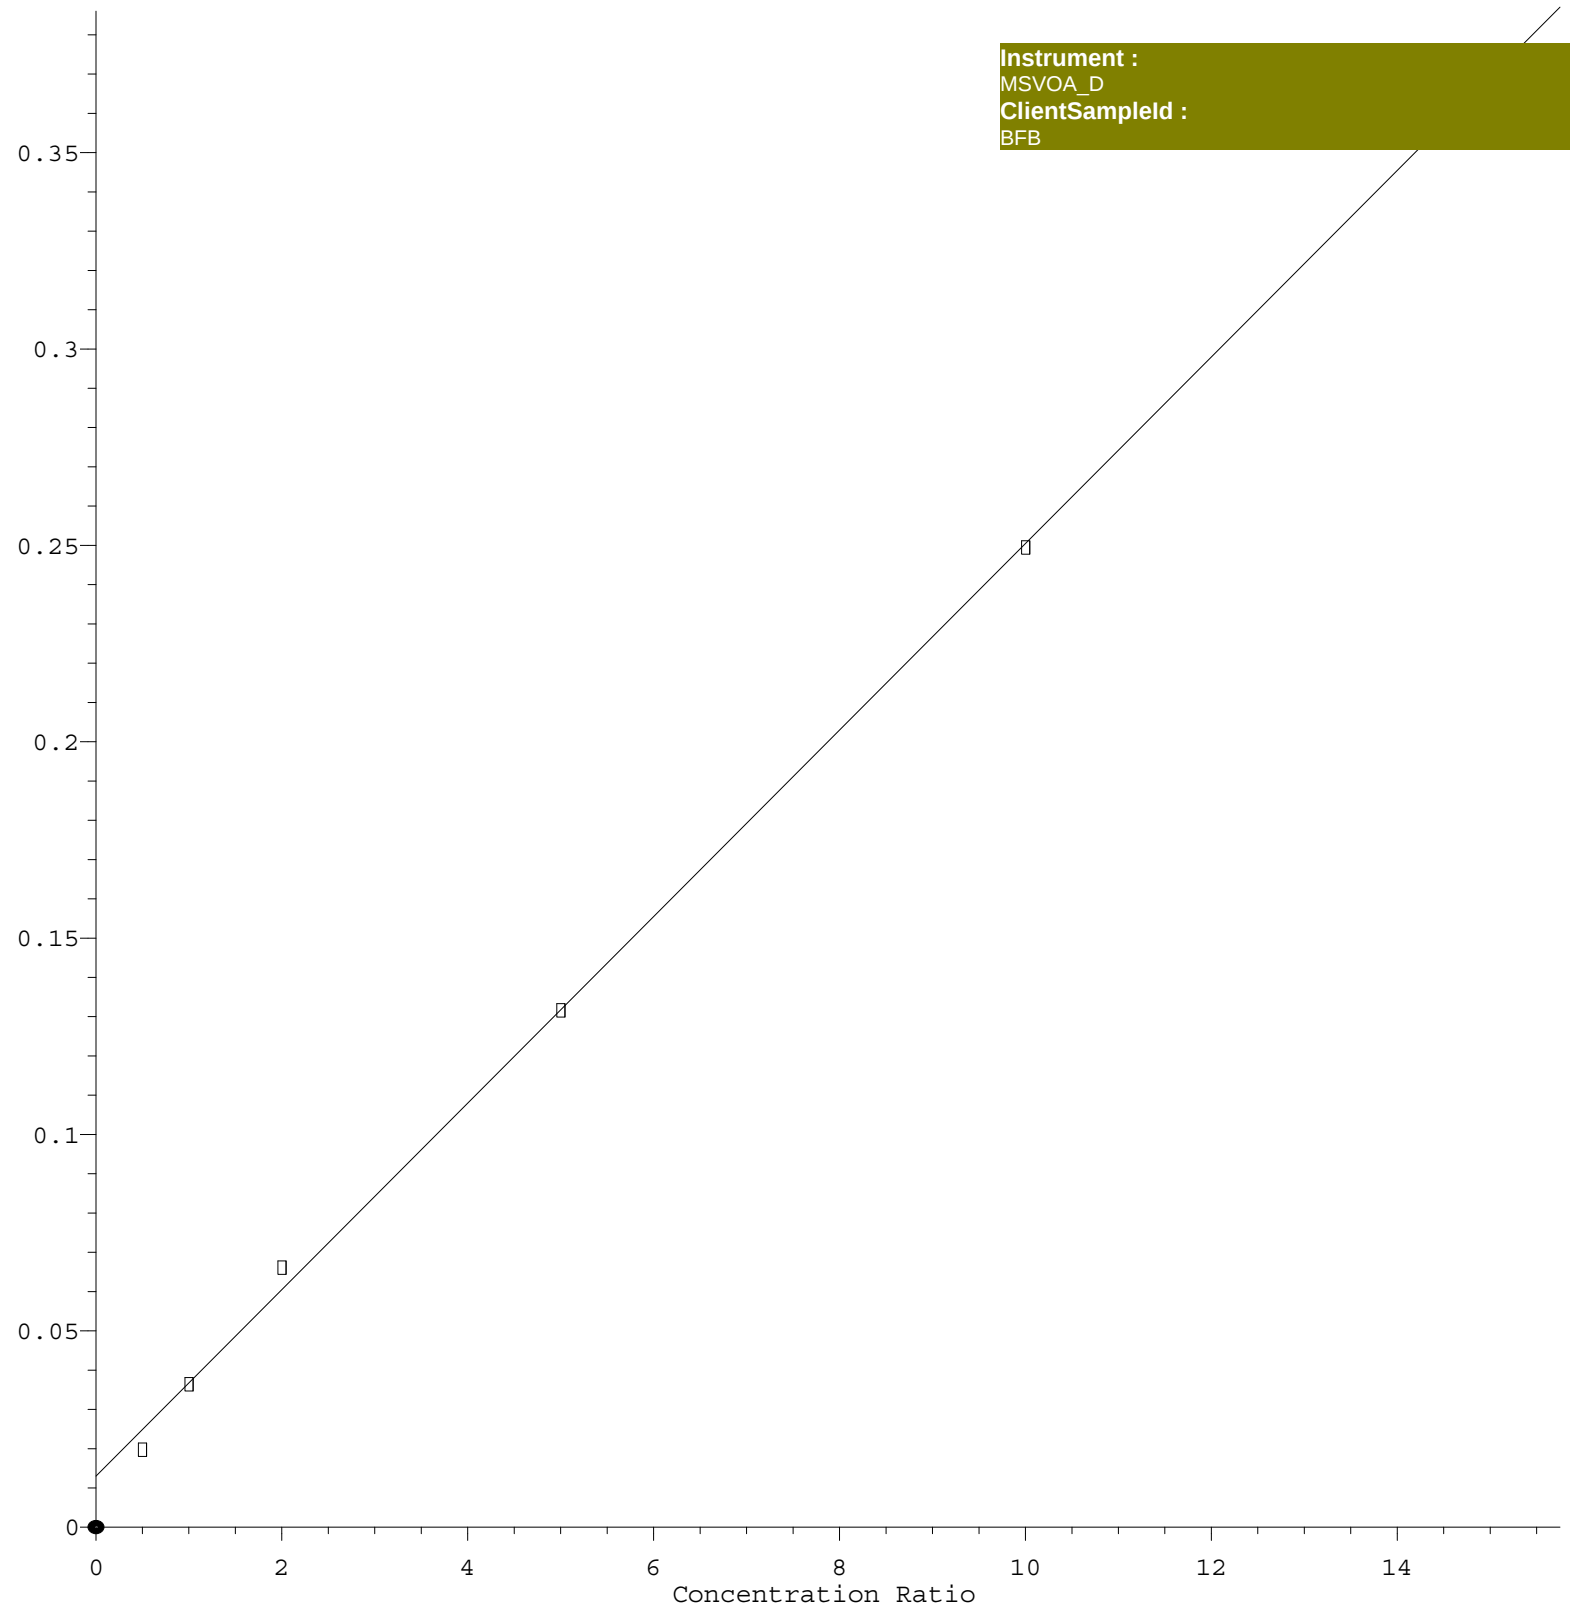

Response = 2.373e-002 * Amt + 1.280e-002
 Coef of Det (r^2) = 0.999380 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D080823S.M
 Calibration Table Last Updated: Wed Aug 09 07:25:36 2023

Acetone


Response Ratio

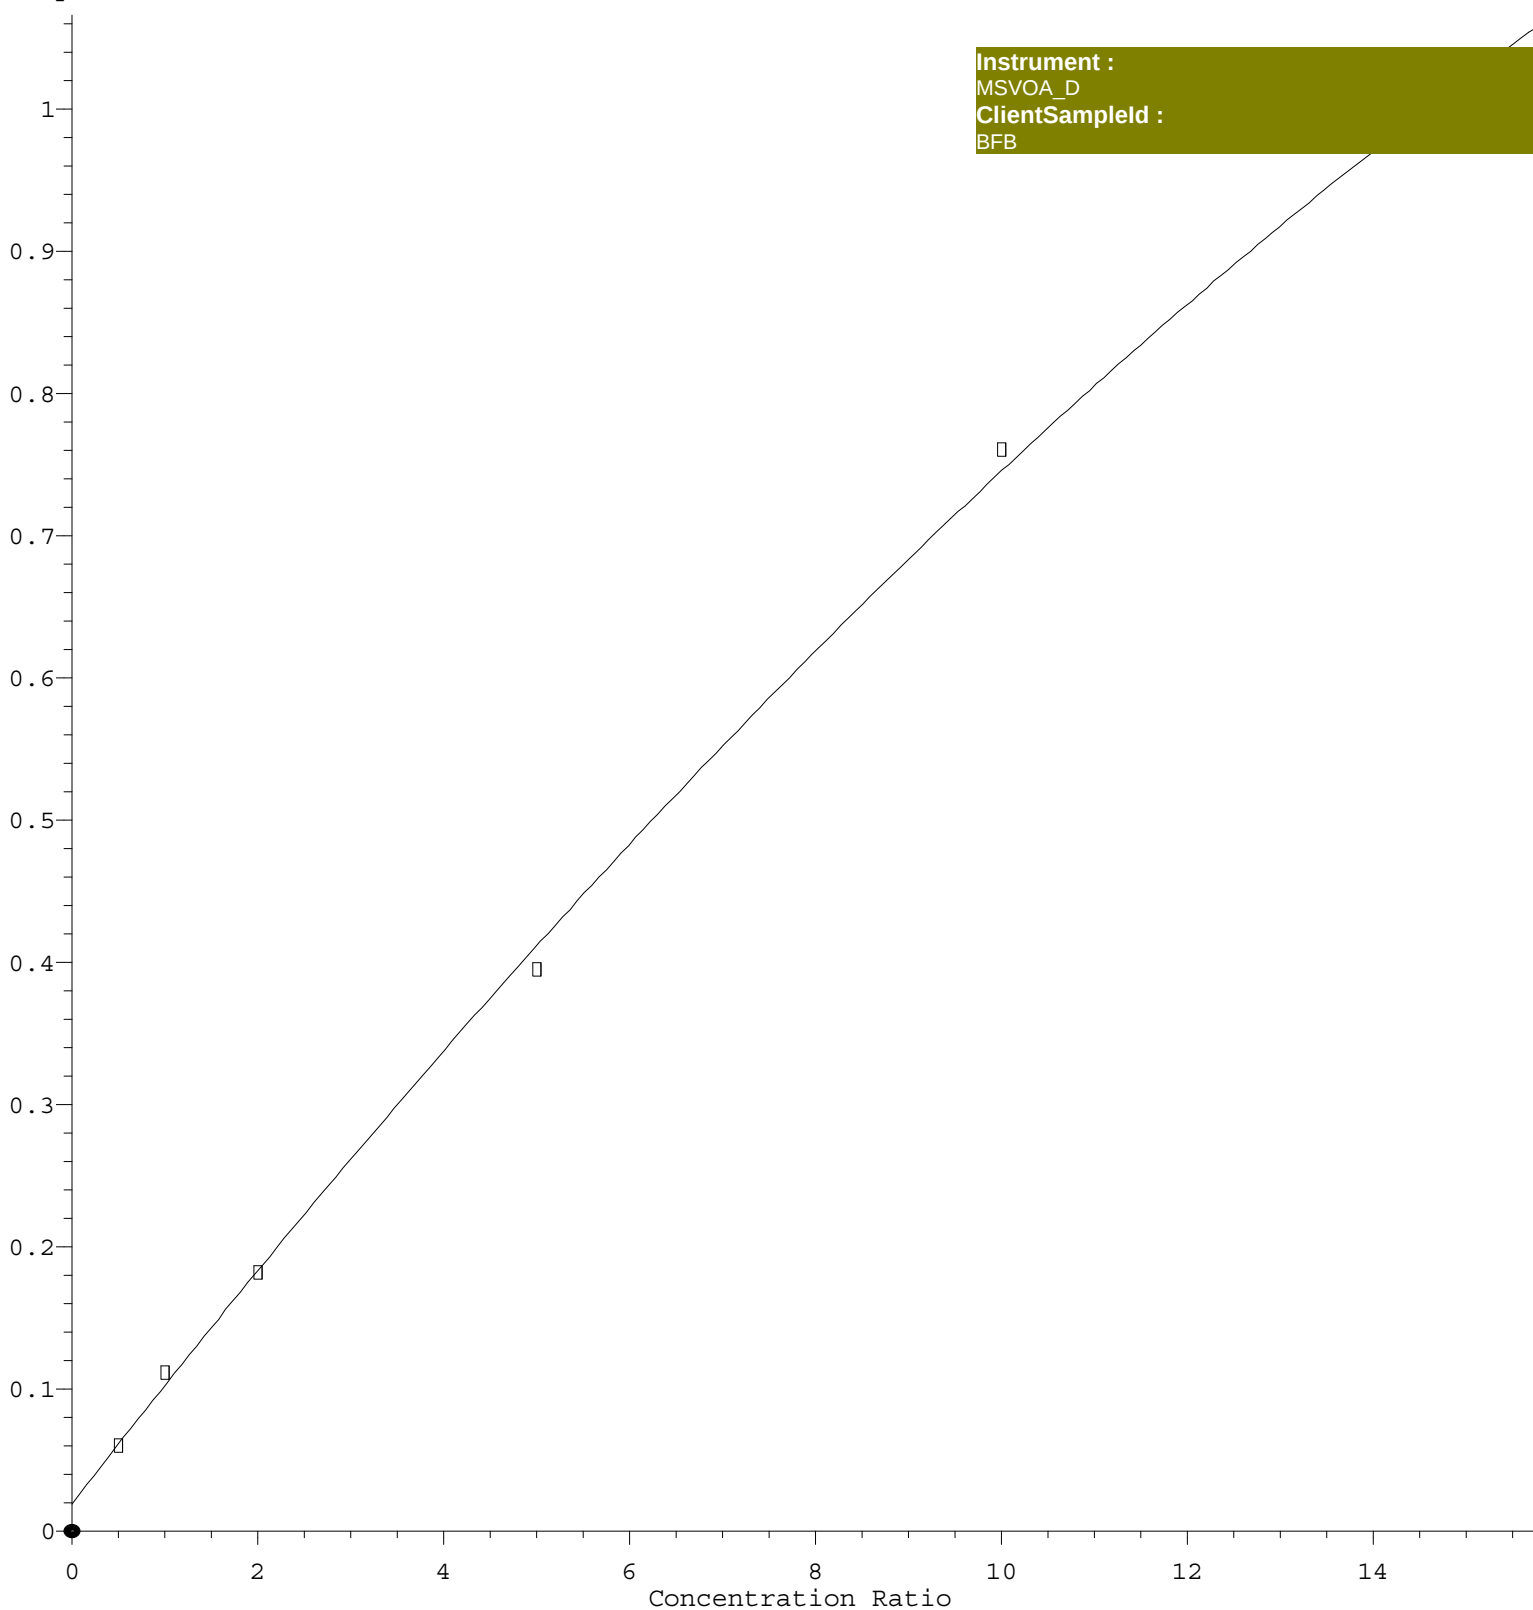

R = -1.168e-003 A*A + 8.429e-002 A + 1.942e-002
Coef of Det (r^2) = 0.999187 Curve Fit: Quadratic
Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D080823S.M
Calibration Table Last Updated: Wed Aug 09 07:25:36 2023

Methylene Chloride


Response Ratio

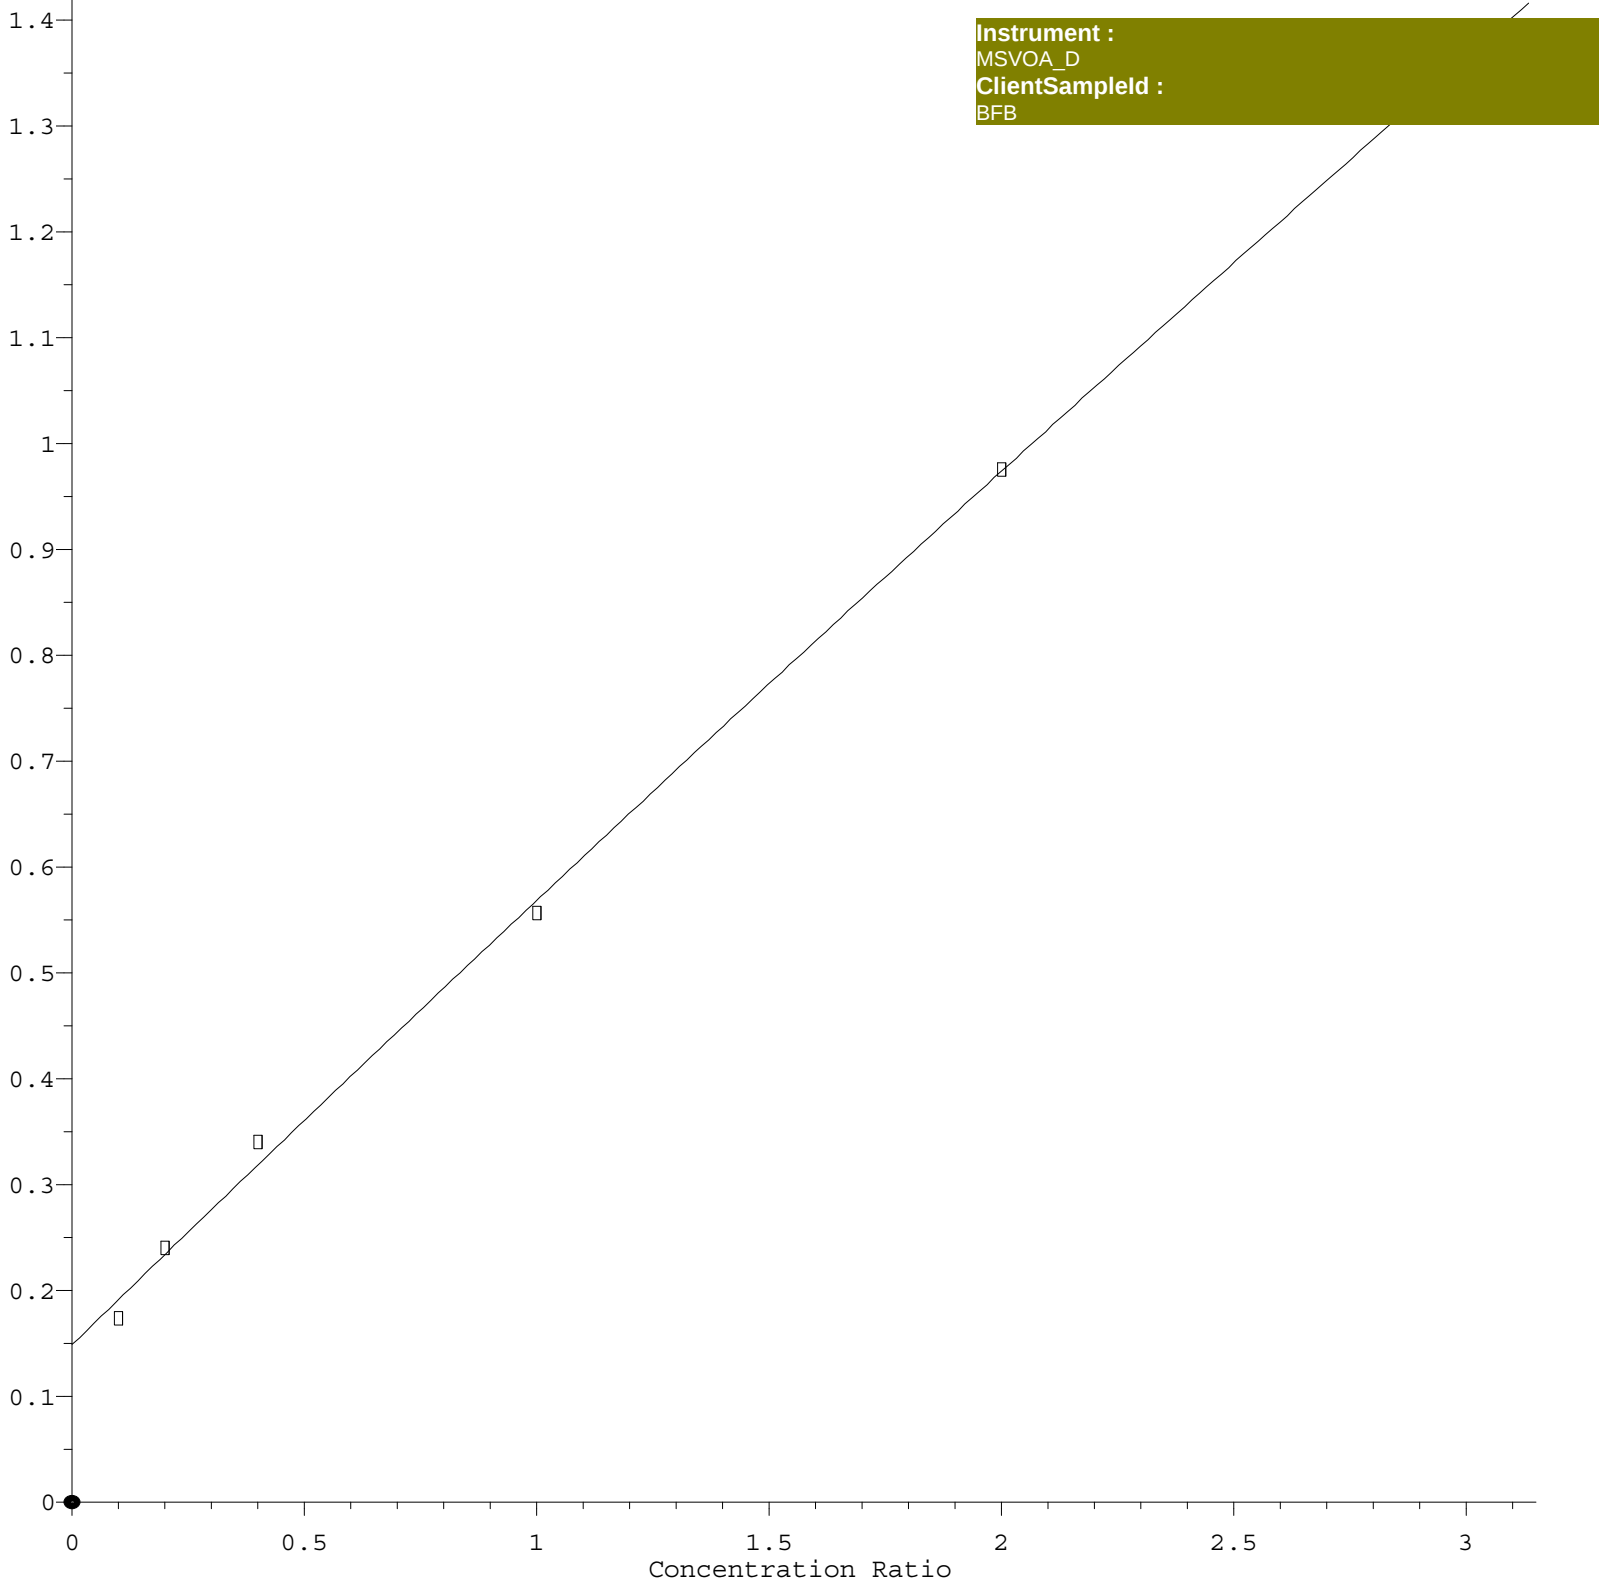

$R = -7.350e-003 A^2 + 4.272e-001 A + 1.487e-001$
 Coef of Det (r^2) = 0.999116 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D080823S.M
 Calibration Table Last Updated: Wed Aug 09 07:25:36 2023

Cyclohexane

Response Ratio

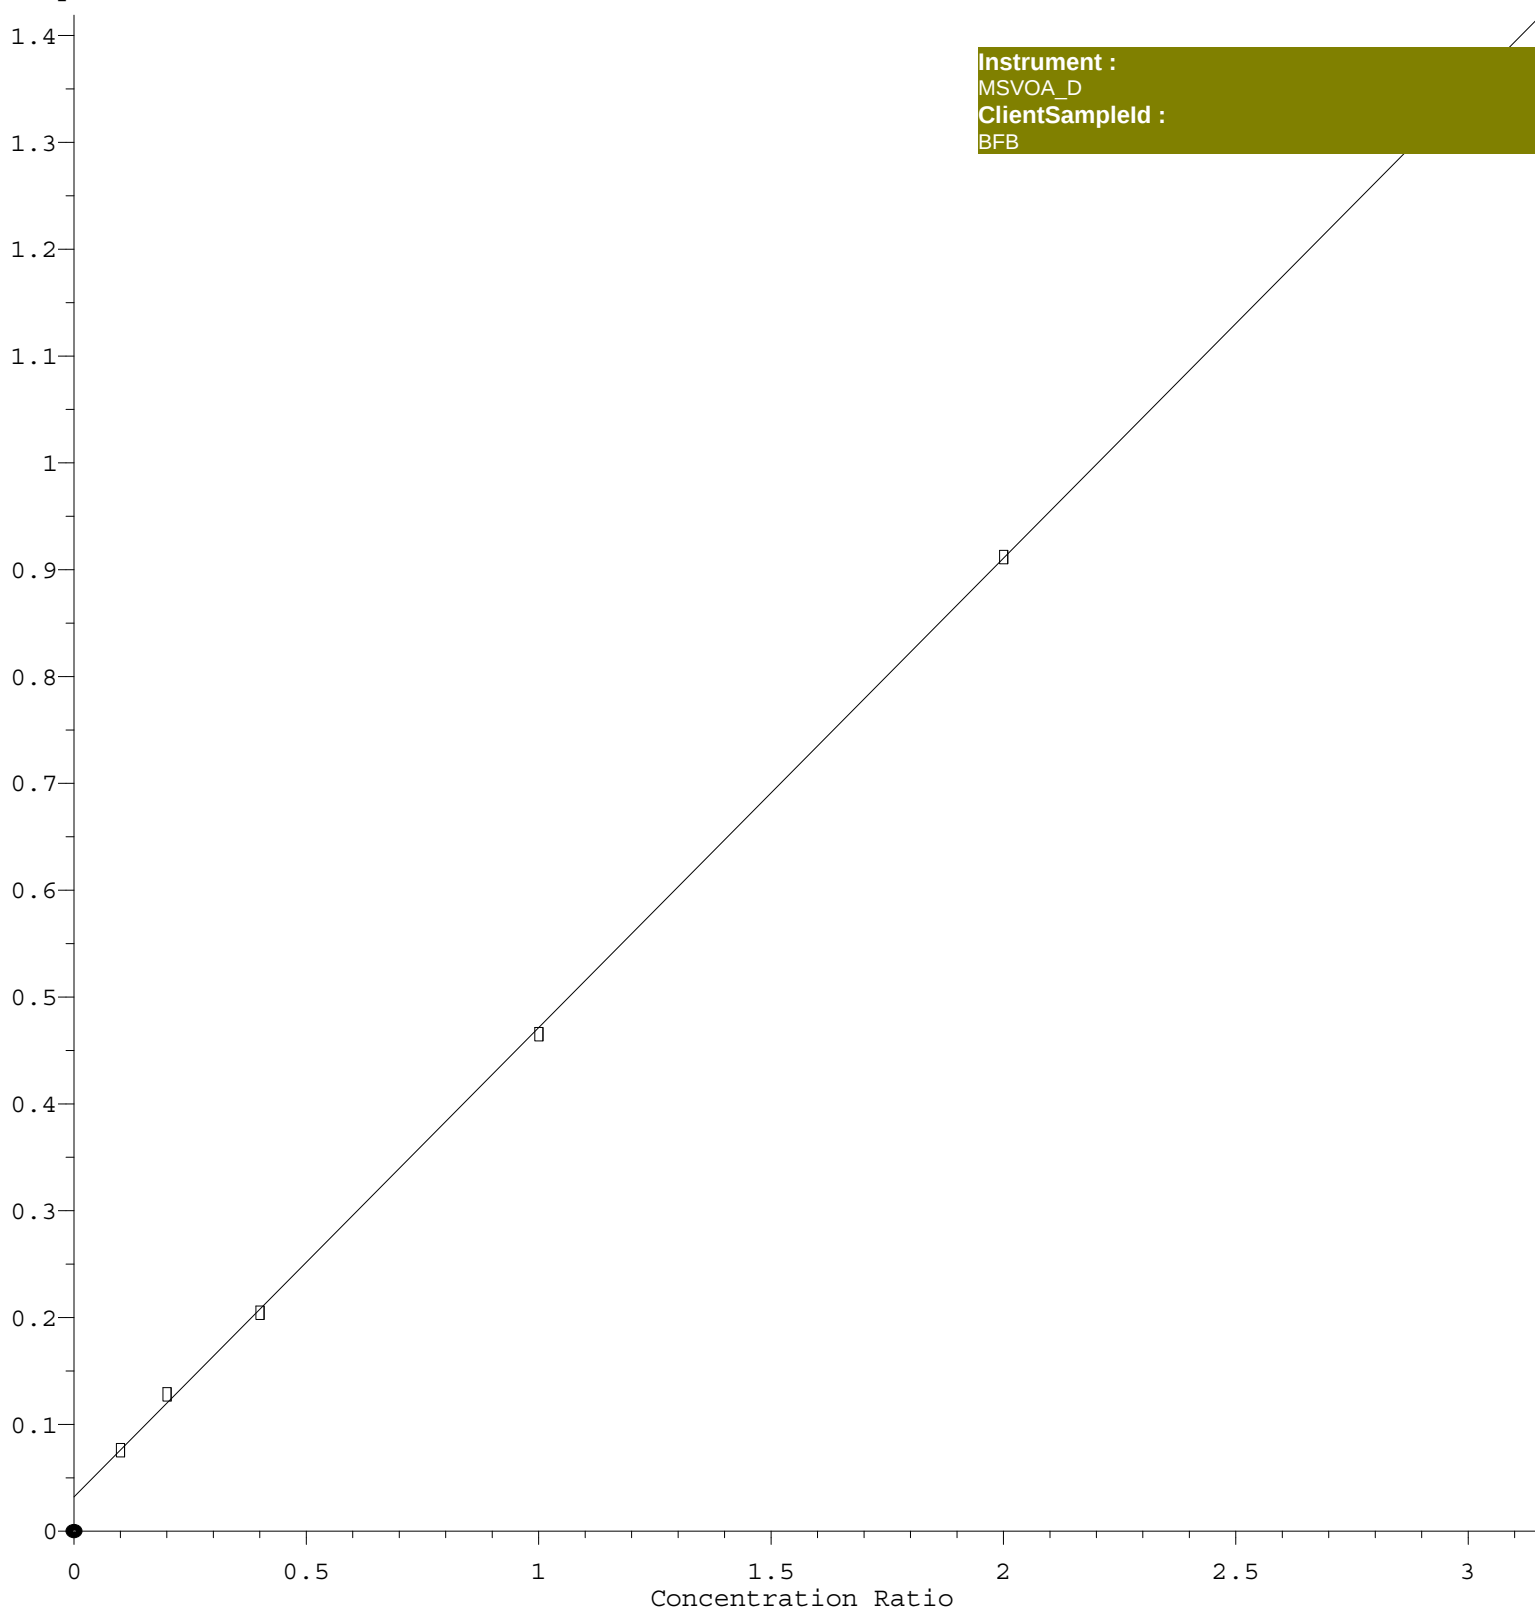

$$\text{Response} = 4.394\text{e-}001 * \text{Amt} + 3.225\text{e-}002$$

Coef of Det (r^2) = 0.999908 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D080823S.M

Calibration Table Last Updated: Wed Aug 09 07:25:36 2023