


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD080919\
Data File : VD063469.D
Acq On : 9 Aug 2019 12:33
Operator : JC/SY
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D080919S.M
Title : SW846 8260
Last Update : Sat Aug 10 06:42:47 2019

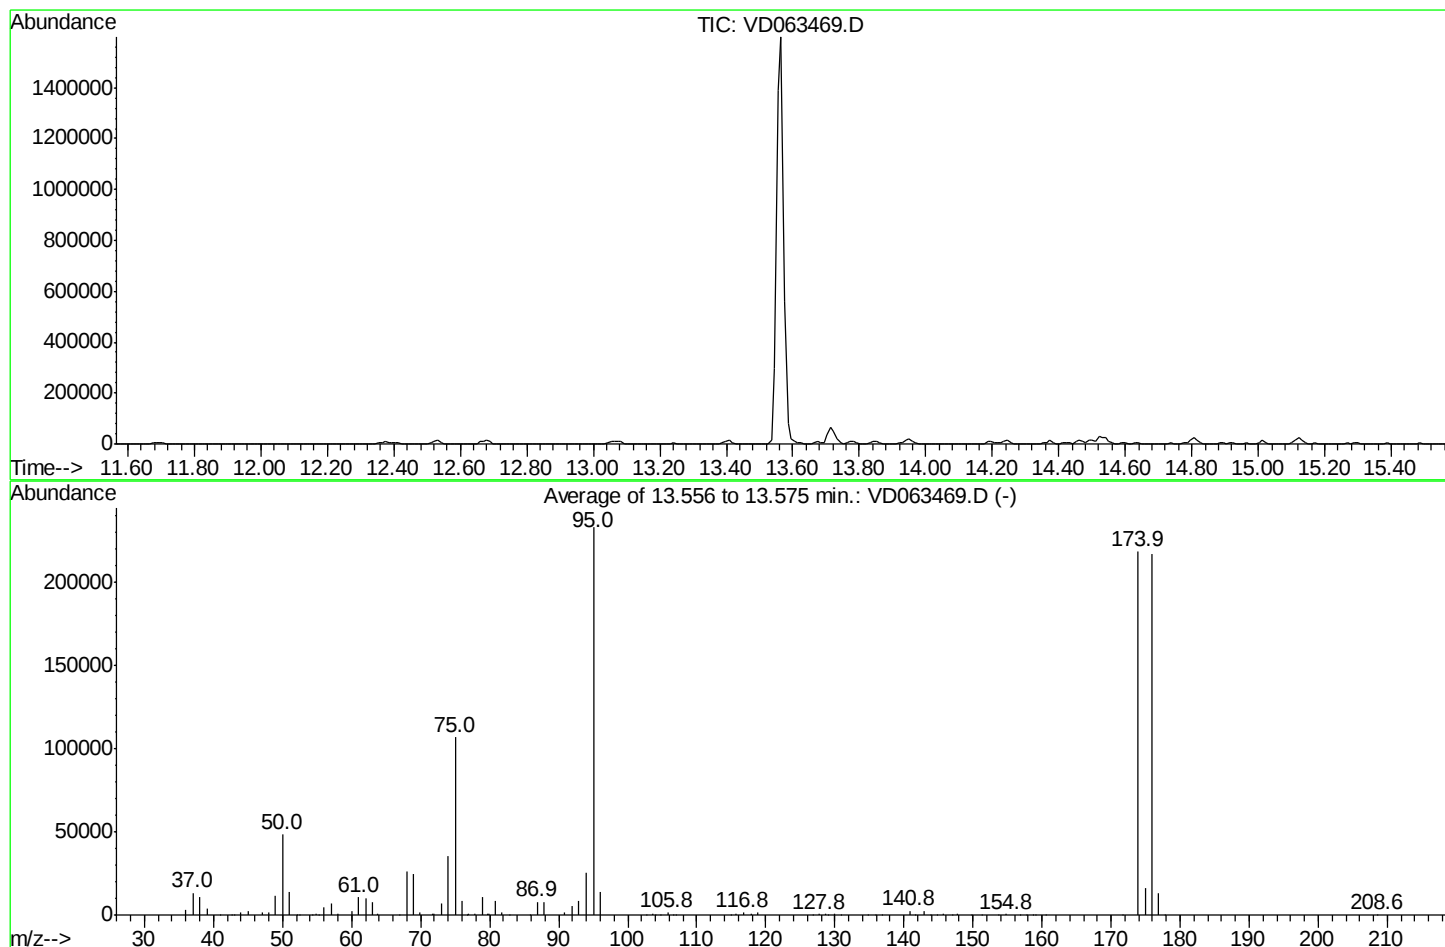

AutoFind: Scans 1232, 1233, 1234; Background Corrected with Scan 1227

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	48189	PASS
75	95	30	60	45.8	106602	PASS
95	95	100	100	100.0	232893	PASS
96	95	5	9	5.9	13670	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	93.7	218154	PASS
175	174	5	9	7.2	15800	PASS
176	174	95	101	99.4	216917	PASS
177	176	5	9	5.9	12797	PASS