

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080922\
 Data File : VD074011.D
 Acq On : 10 Aug 2022 02:54
 Operator : VA/SY
 Sample : N4046-15
 Misc : 6.87G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BEACONPOINT-BACKFILL-08

Quant Time: Aug 10 04:48:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D080922S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 10 01:05:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.973	168	89209	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.856	114	198763	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.632	117	214711	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	99462	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.320	65	69821	88.279	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 176.560%#	
35) Dibromofluoromethane	7.903	113	79225	65.249	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 130.500%	
50) Toluene-d8	10.332	98	257698	71.848	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 143.700%#	
62) 4-Bromofluorobenzene	12.620	95	90310	58.586	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 117.180%	


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080922\
Data File : VD074011.D
Acq On : 10 Aug 2022 02:54
Operator : VA/SY
Sample : N4046-15
Misc : 6.87G/5.00ml/MSVOA_D/SOIL
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BEACONPOINT-BACKFILL-08

Quant Time: Aug 10 04:48:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D080922S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 10 01:05:43 2022
Response via : Initial Calibration




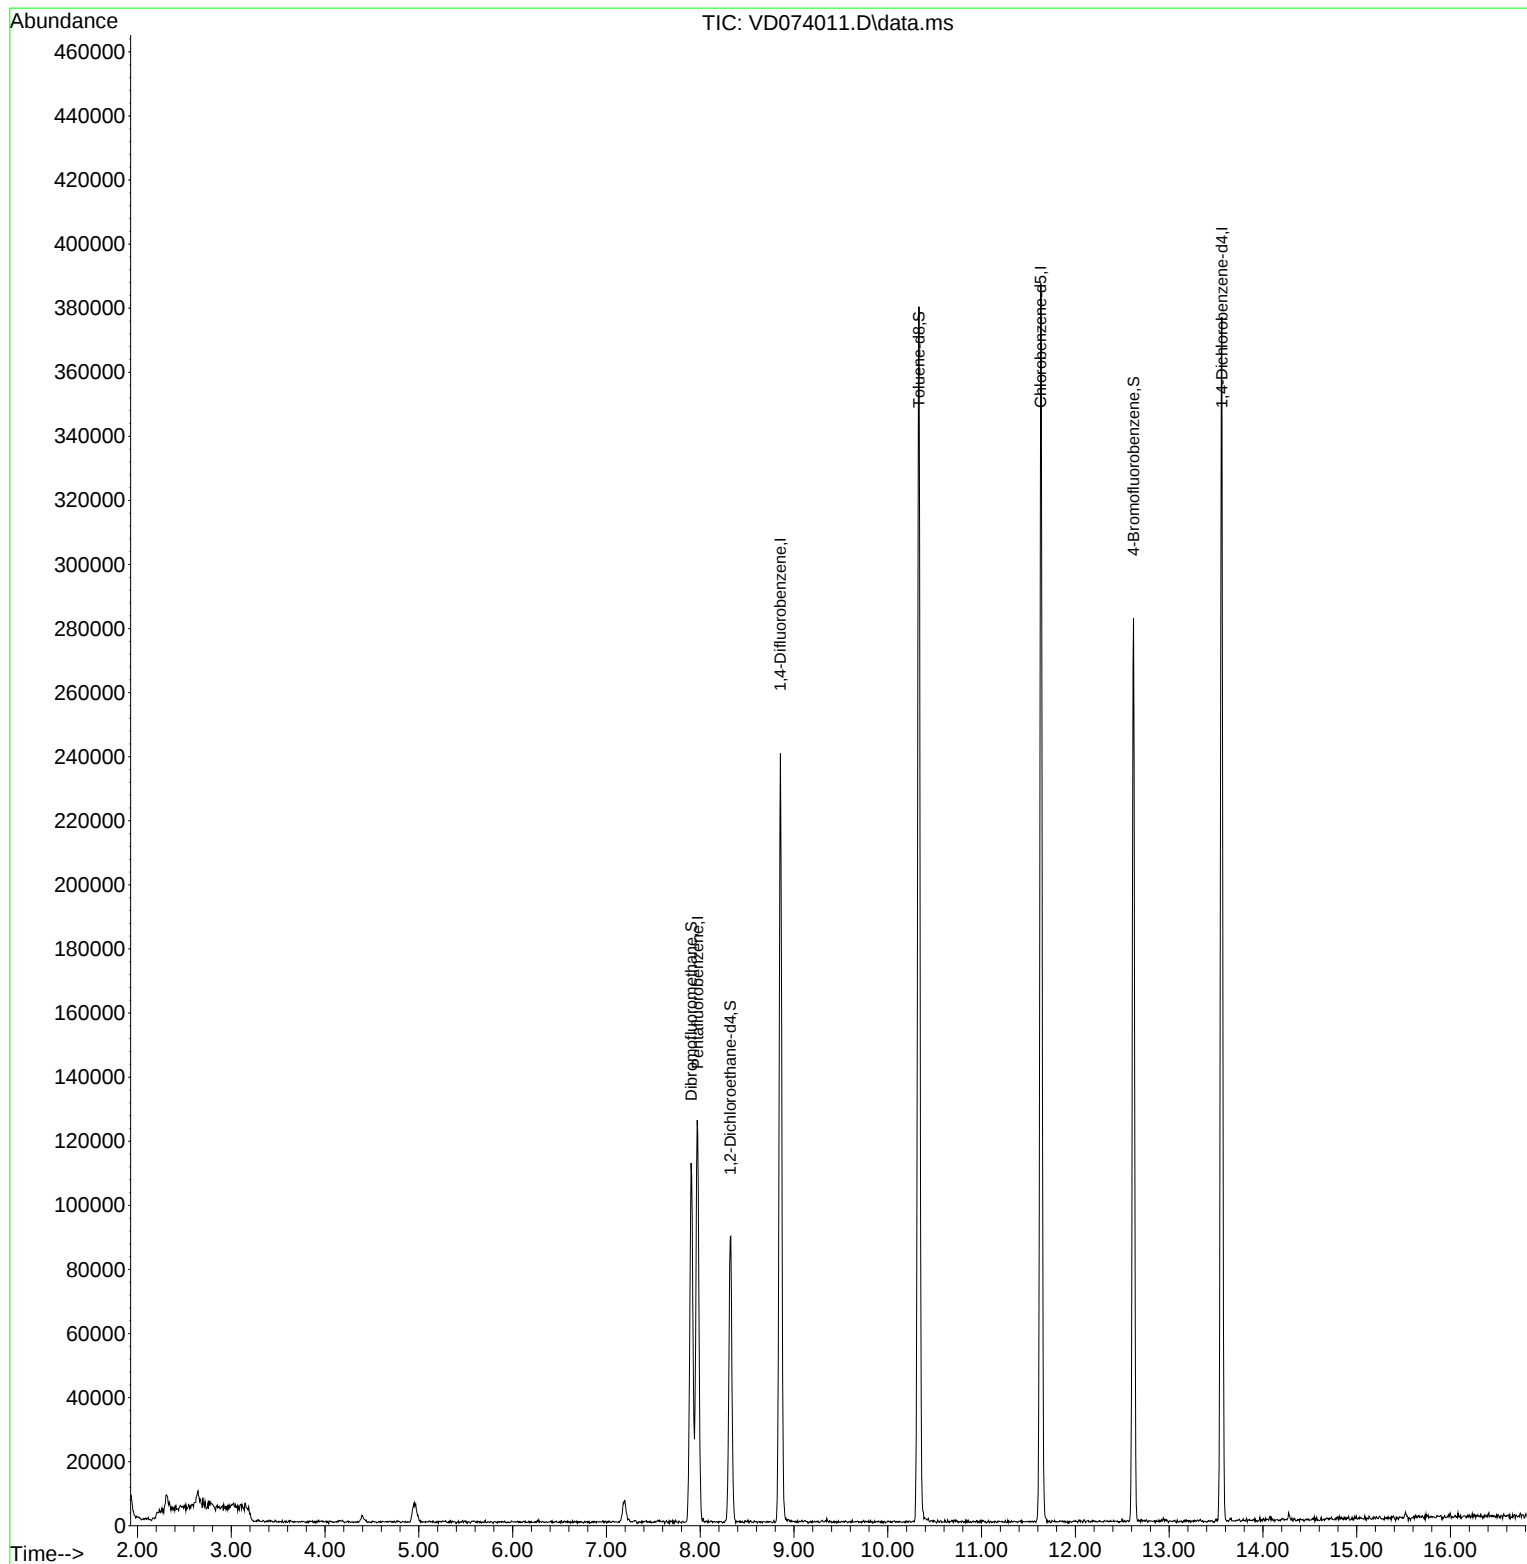


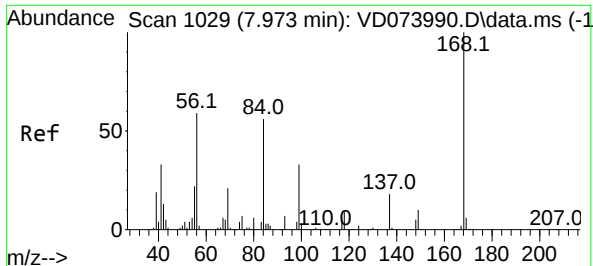

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.973 min Scan# 1029
Delta R.T. 0.000 min
Lab File: VD074011.D
Acq: 10 Aug 2022 02:54




Instrument :
MSVOA_D
ClientSampleId :
BEACONPOINT-BACKFILL-08


Tgt Ion:168 Resp: 89209
Ion Ratio Lower Upper
168 100
99 59.2 48.3 72.5

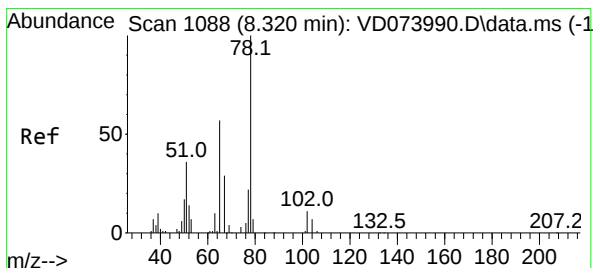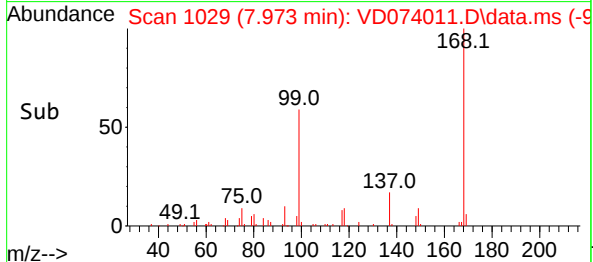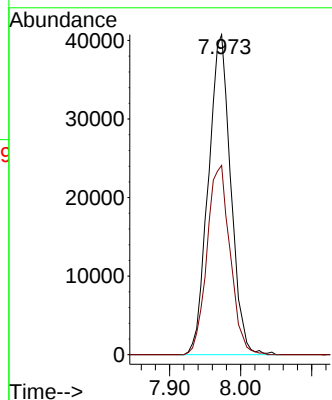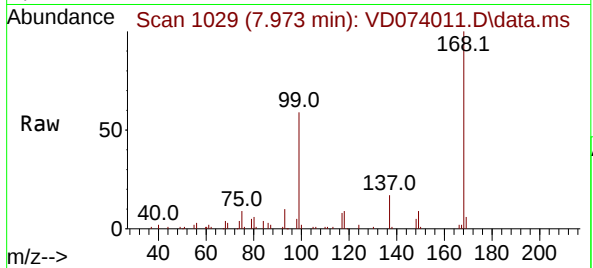

#33
1,2-Dichloroethane-d4
Concen: 88.279 ug/l
RT: 8.320 min Scan# 1088
Delta R.T. 0.000 min
Lab File: VD074011.D
Acq: 10 Aug 2022 02:54

Tgt Ion: 65 Resp: 69821
Ion Ratio Lower Upper
65 100
67 51.6 0.0 113.6

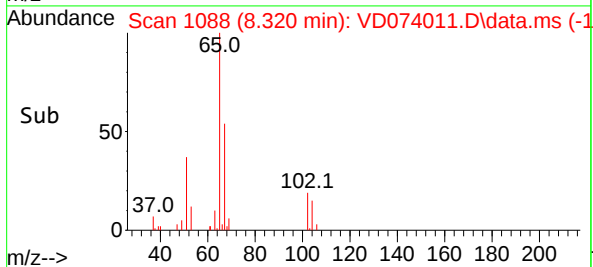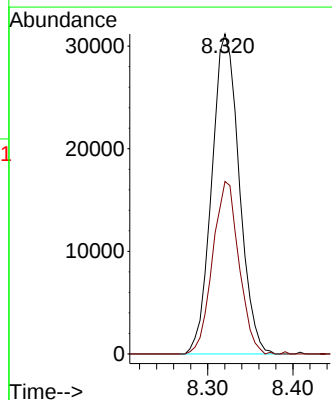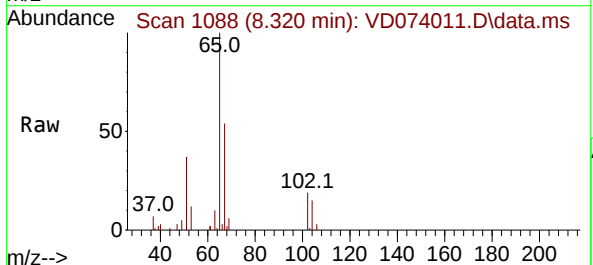

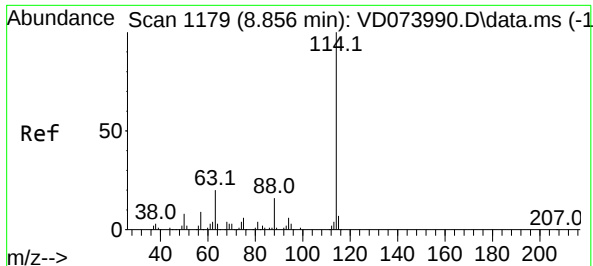

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.856 min Scan# 1179

Delta R.T. -0.000 min

Lab File: VD074011.D

Acq: 10 Aug 2022 02:54

Instrument :

MSVOA_D

ClientSampleId :

BEACONPOINT-BACKFILL-08





Tgt Ion:114 Resp: 198763

Ion Ratio Lower Upper

114 100

63 19.8 0.0 41.0

88 15.3 0.0 31.6

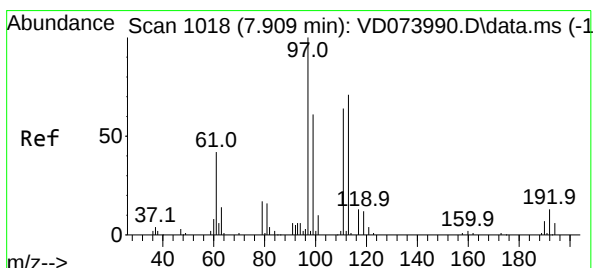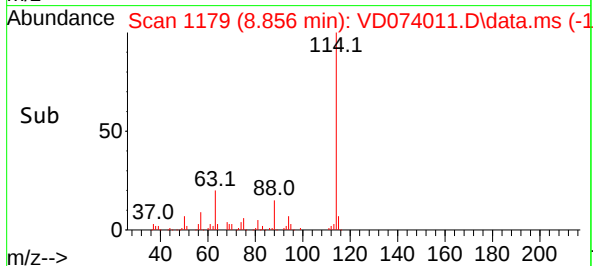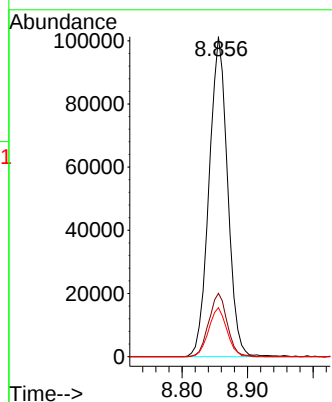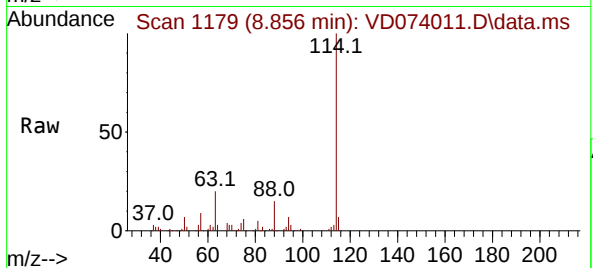

#35

Dibromofluoromethane

Concen: 65.249 ug/l

RT: 7.903 min Scan# 1017

Delta R.T. -0.006 min

Lab File: VD074011.D

Acq: 10 Aug 2022 02:54




Tgt Ion:113 Resp: 79225


Ion Ratio Lower Upper

113 100

111 99.7 80.0 120.0

192 18.2 14.2 21.4


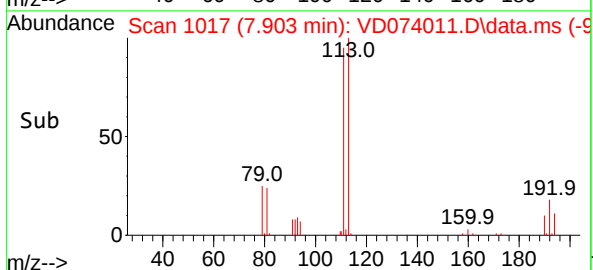
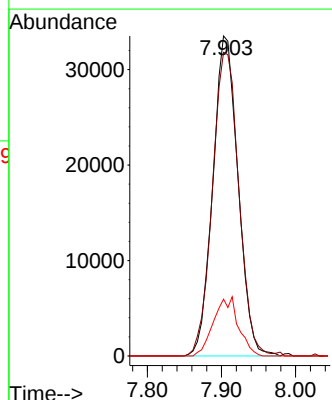
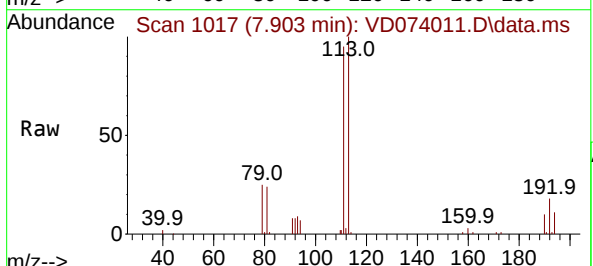


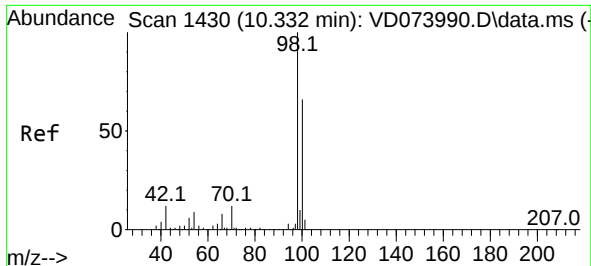

#50
Toluene-d8
Concen: 71.848 ug/l
RT: 10.332 min Scan# 1430
Delta R.T. -0.000 min
Lab File: VD074011.D
Acq: 10 Aug 2022 02:54




Instrument : MSVOA_D
ClientSampleId : BEACONPOINT-BACKFILL-08


Tgt Ion: 98 Resp: 257698
Ion Ratio Lower Upper
98 100
100 64.9 51.3 76.9

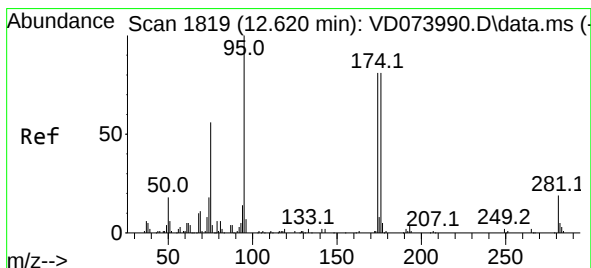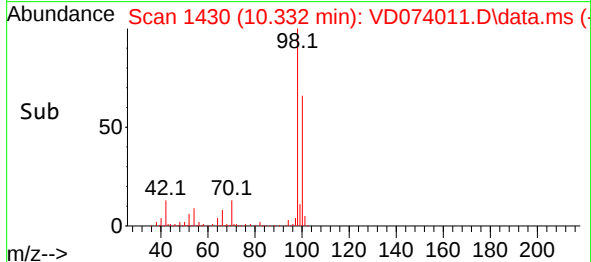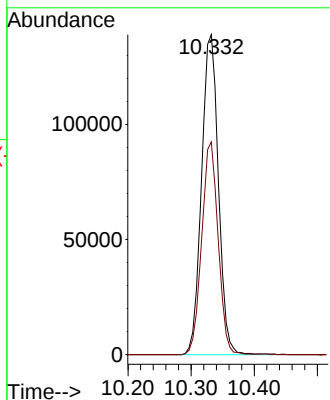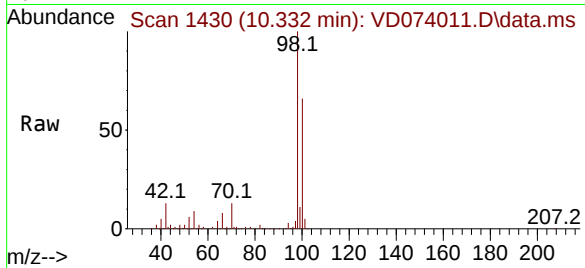

#62
4-Bromofluorobenzene
Concen: 58.586 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. 0.000 min
Lab File: VD074011.D
Acq: 10 Aug 2022 02:54

Tgt Ion: 95 Resp: 90310
Ion Ratio Lower Upper
95 100
174 80.4 0.0 162.6
176 76.1 0.0 160.0


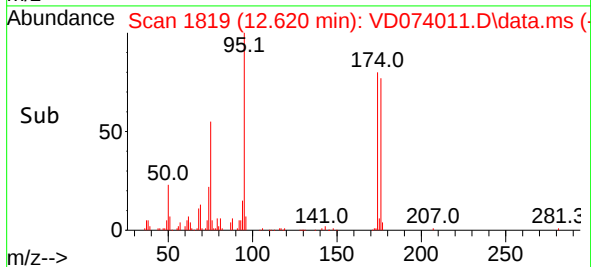
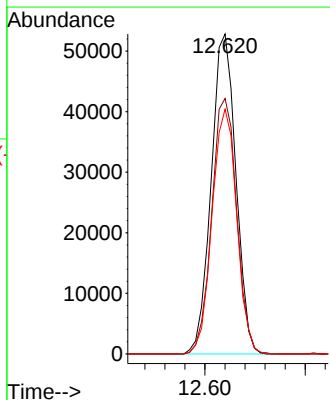
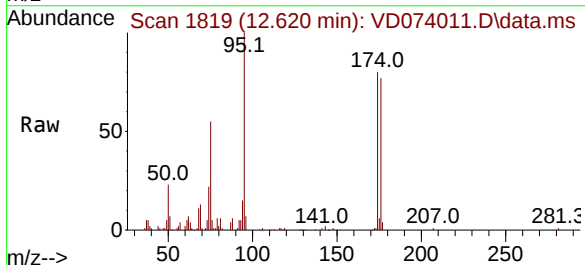


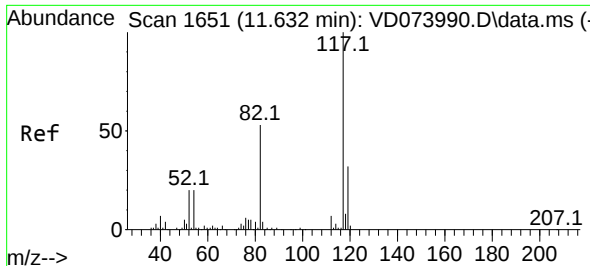

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.632 min Scan# 117
Delta R.T. 0.000 min
Lab File: VD074011.D
Acq: 10 Aug 2022 02:54

Instrument :
MSVOA_D
ClientSampleId :
BEACONPOINT-BACKFILL-08

Tgt Ion:117 Resp: 214711
Ion Ratio Lower Upper
117 100
82 53.2 42.7 64.1
119 31.0 25.8 38.8

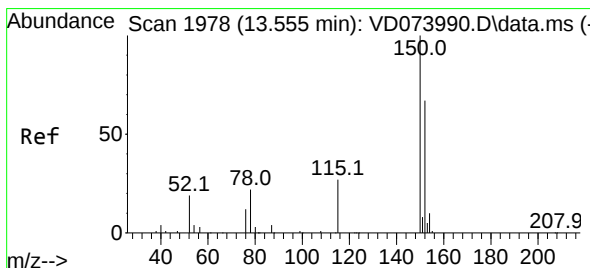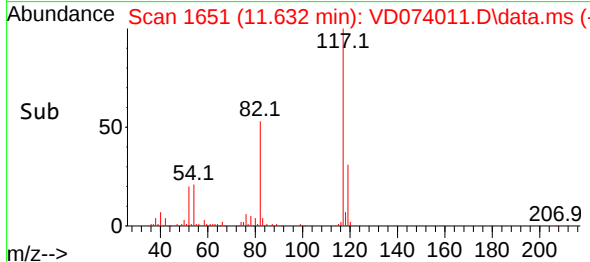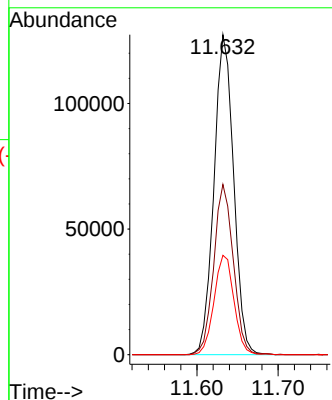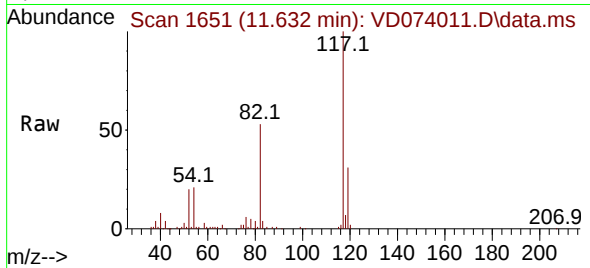

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. 0.006 min
Lab File: VD074011.D
Acq: 10 Aug 2022 02:54

Tgt Ion:152 Resp: 99462
Ion Ratio Lower Upper
152 100
115 59.7 29.9 89.8
150 155.3 0.0 342.8

