
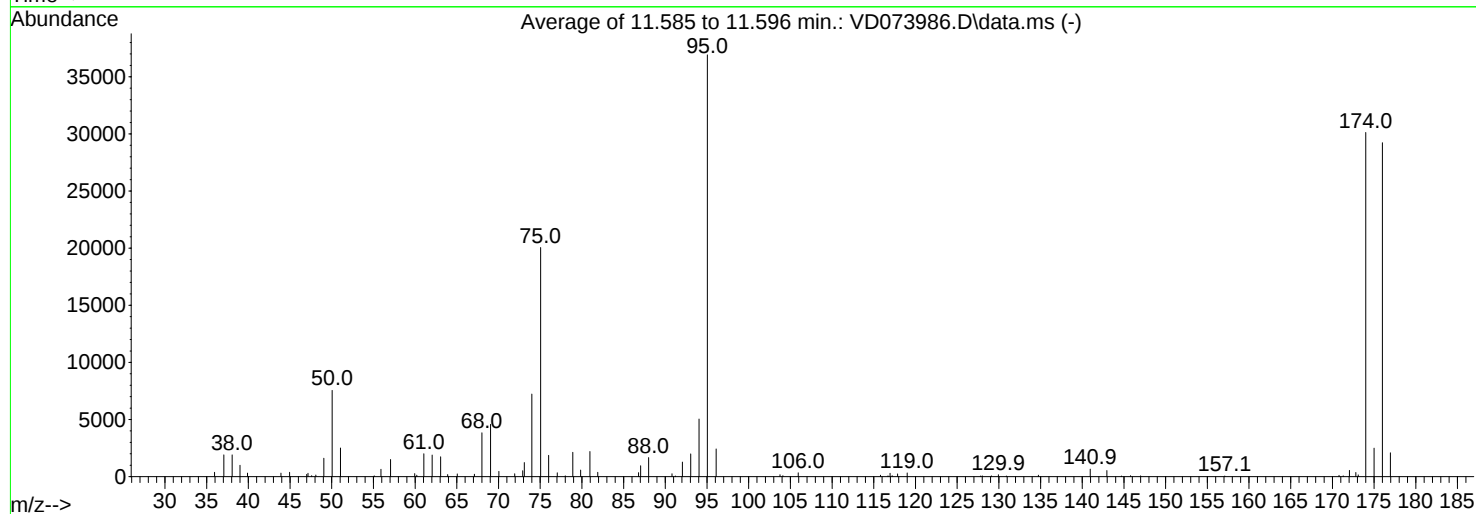


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080922\
Data File : VD073986.D
Acq On : 09 Aug 2022 09:12
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D080922S.M
Title : SW846 8260
Last Update : Wed Aug 10 01:05:43 2022

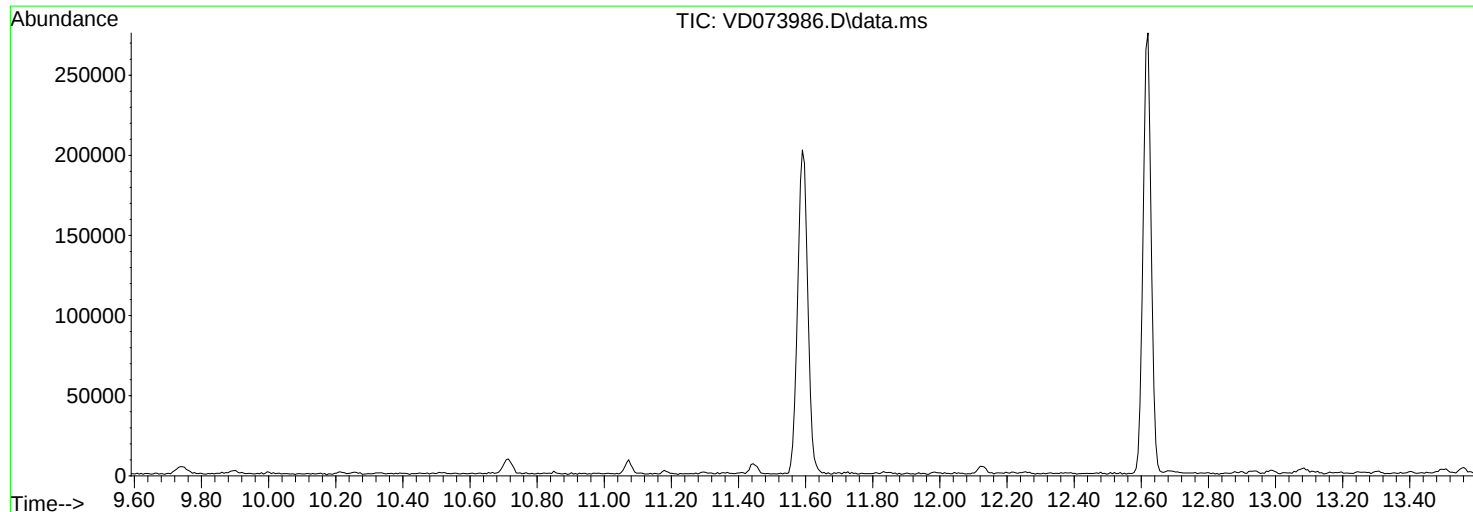

AutoFind: Scans 1643, 1644, 1645; Background Corrected with Scan 1634

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	7557	PASS
75	95	30	60	54.3	20061	PASS
95	95	100	100	100.0	36920	PASS
96	95	5	9	6.6	2428	PASS
173	174	0.00	2	1.2	369	PASS
174	95	50	100	81.6	30131	PASS
175	174	5	9	8.3	2498	PASS
176	174	95	101	97.0	29235	PASS
177	176	5	9	7.2	2092	PASS