
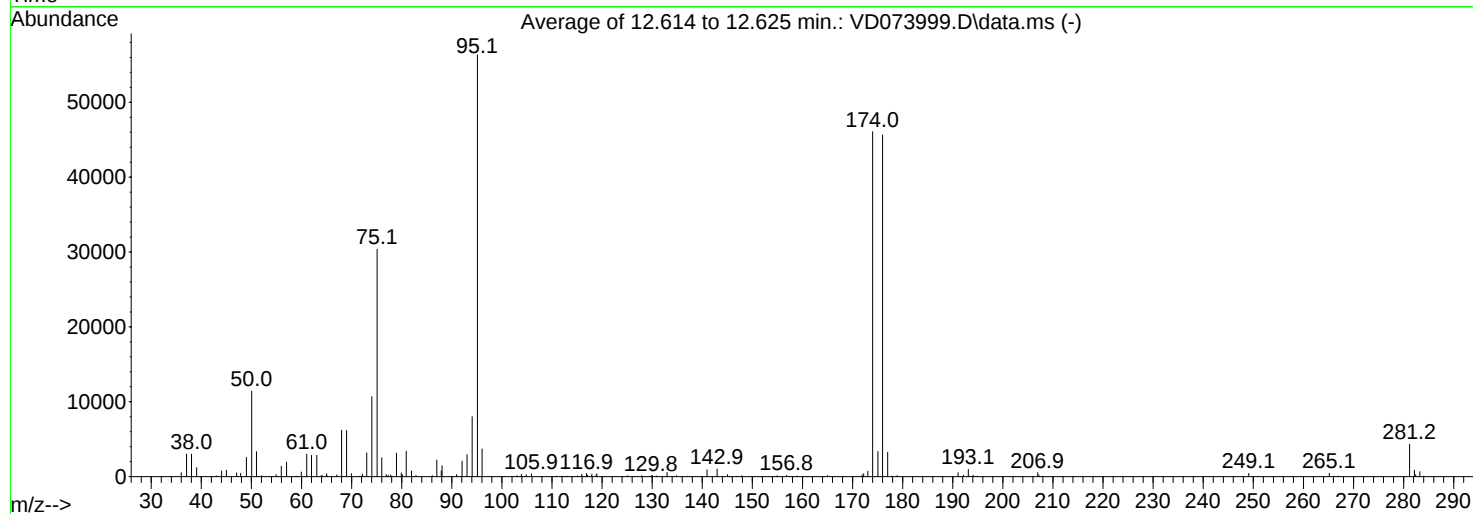


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD080922\  
Data File : VD073999.D  
Acq On : 09 Aug 2022 19:26  
Operator : VA/SY  
Sample : BFB  
Misc : 5.00G/5.00ml/MSVOA\_D/SOIL  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D080922S.M  
Title : SW846 8260  
Last Update : Wed Aug 10 01:05:43 2022

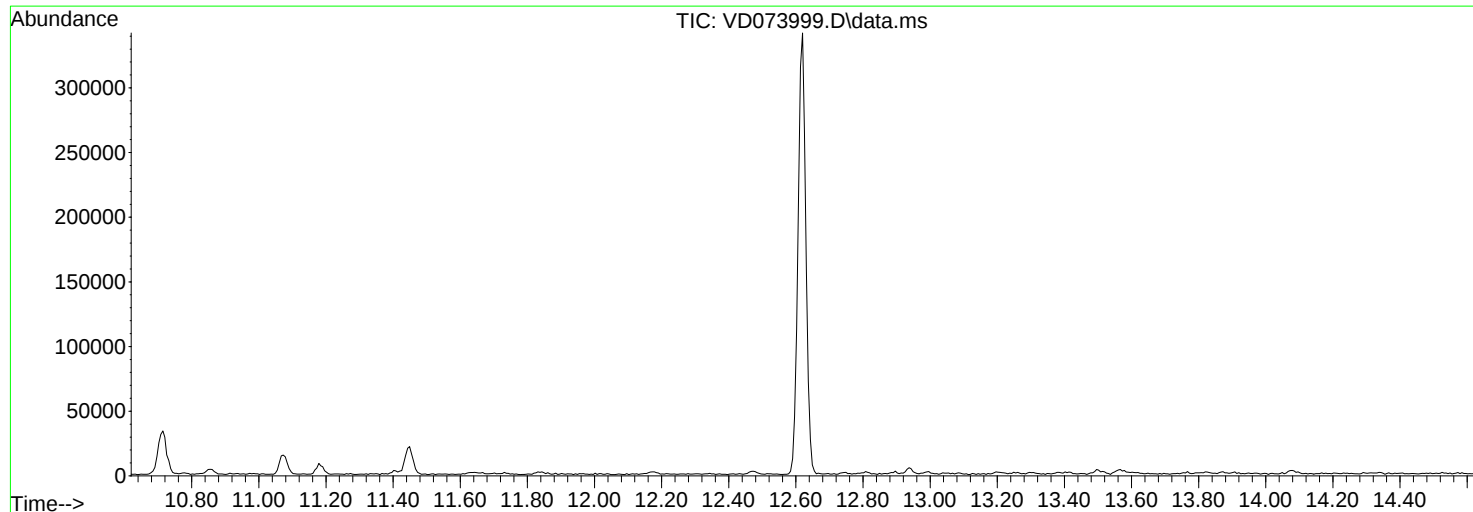

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1810

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 20.2         | 11406      | PASS                |
| 75             | 95              | 30              | 60              | 53.9         | 30387      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 56336      | PASS                |
| 96             | 95              | 5               | 9               | 6.5          | 3688       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.6          | 737        | PASS                |
| 174            | 95              | 50              | 100             | 81.8         | 46077      | PASS                |
| 175            | 174             | 5               | 9               | 7.3          | 3373       | PASS                |
| 176            | 174             | 95              | 101             | 99.0         | 45616      | PASS                |
| 177            | 176             | 5               | 9               | 7.1          | 3244       | PASS                |